

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033183.D
 Acq On : 02 Aug 2024 00:54
 Operator : MA/JU
 Sample : P3359-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GF3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 02 02:11:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.482	152	3176m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.235	136	10143	0.400	ng/ul	#-0.08
9) Acenaphthene-d10	14.125	164	6106	0.400	ng/ul	#-0.04
13) Phenanthrene-d10	16.895	188	12700m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.151	240	9867	0.400	ng/ul	0.00
23) Perylene-d12	23.308	264	5294m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.048	96	16882	4.202	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.879	152	4436	0.268	ng/ul	-0.05
18) Fluoranthene-d10	18.944	212	11195	0.401	ng/ul	-0.03
Target Compounds						Qvalue
5) Naphthalene	10.284	128	1336	0.051	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033183.D
Acq On : 02 Aug 2024 00:54
Operator : MA/JU
Sample : P3359-16
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GF3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Aug 02 02:11:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

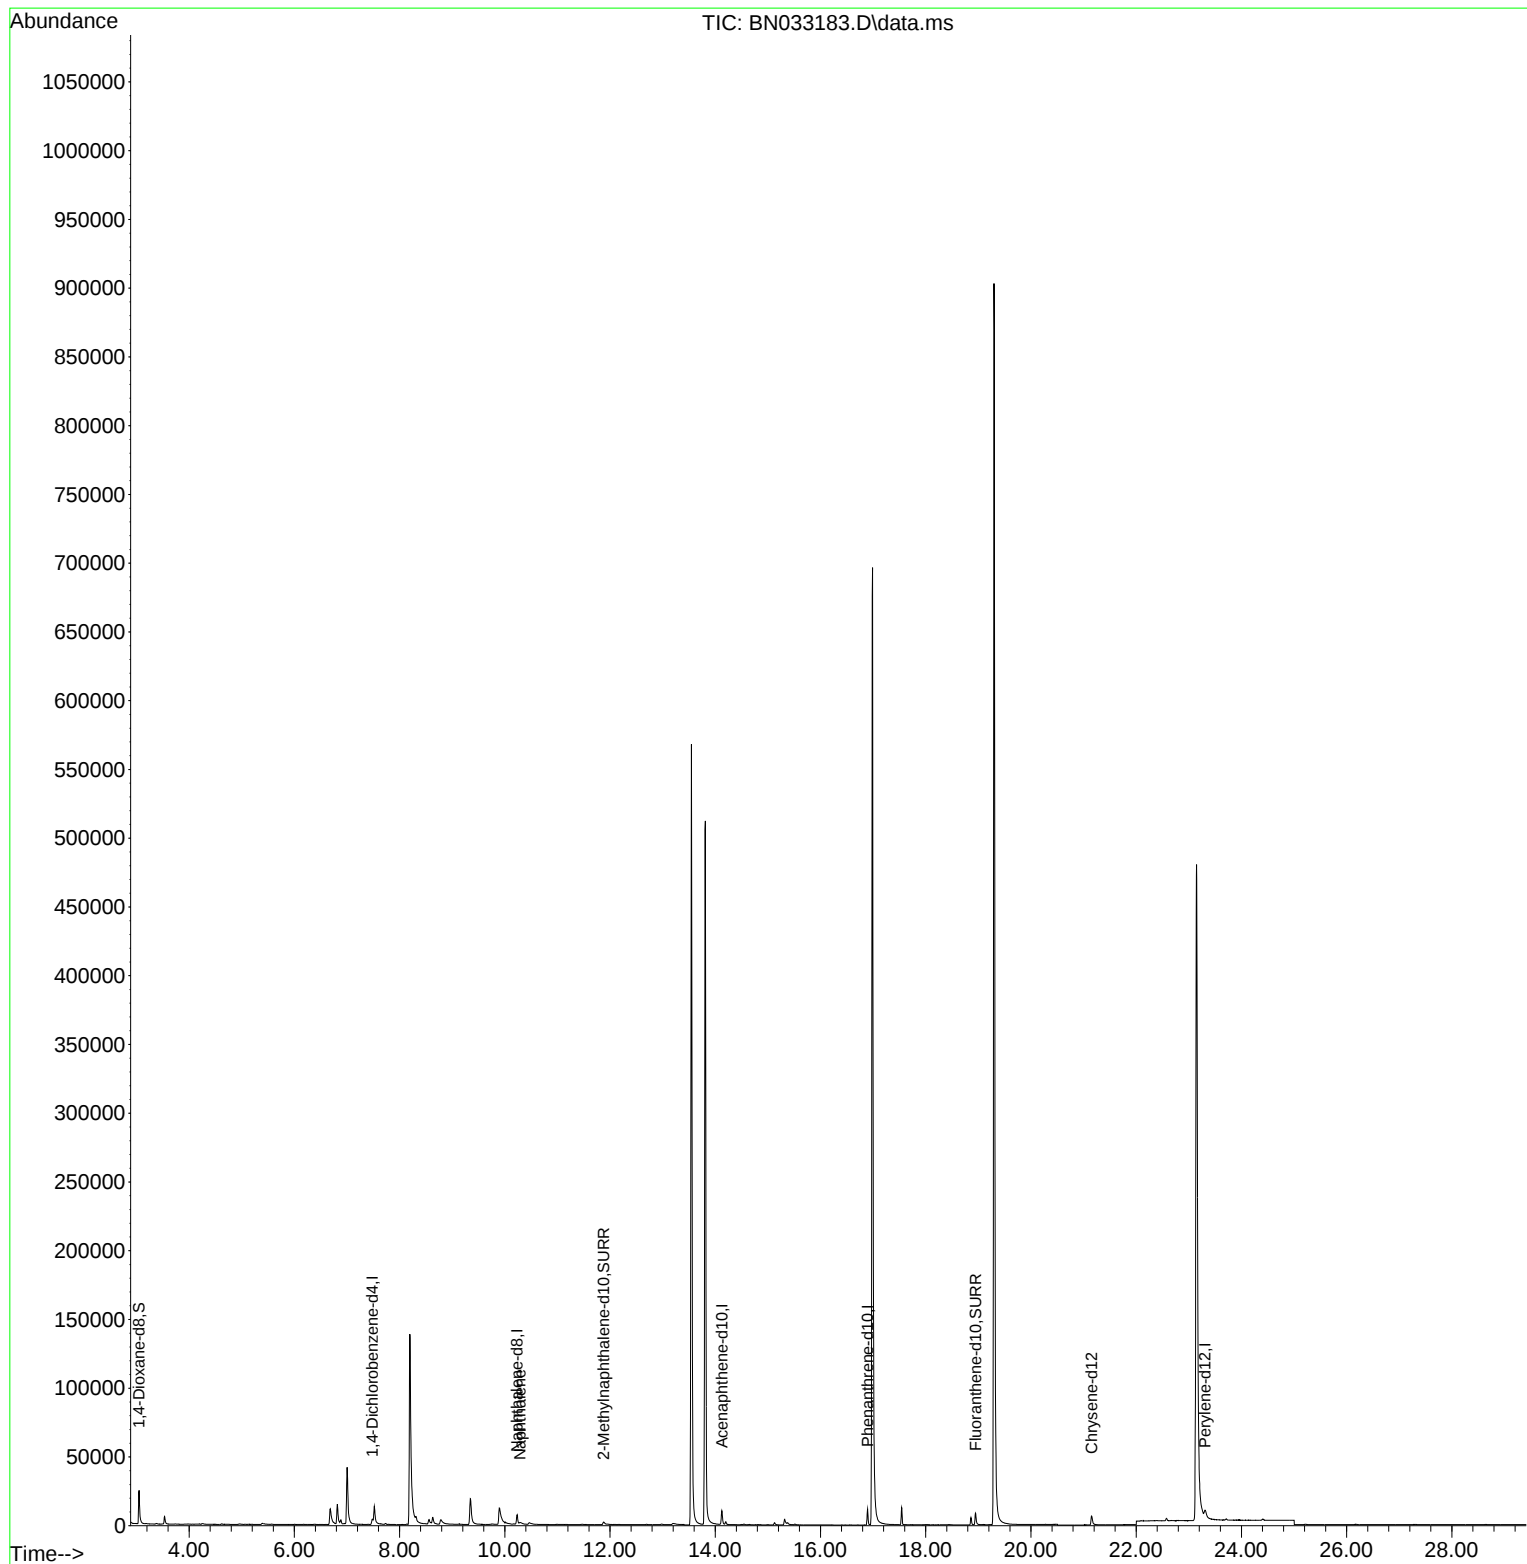

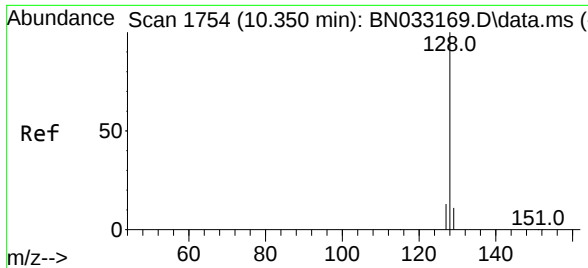

#5
Naphthalene
Concen: 0.051 ng/ul
RT: 10.284 min Scan# 11
Delta R.T. -0.093 min
Lab File: BN033183.D
Acq: 02 Aug 2024 00:54

Instrument :
BNA_N
ClientSampleId :
E1GF3

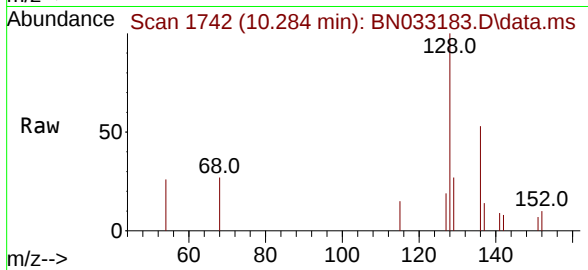

Tgt Ion:128 Resp: 1330
Ion Ratio Lower Upper
128 100
129 26.9 12.0 18.0
127 19.4 12.7 19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

