

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033195.D
 Acq On : 02 Aug 2024 08:46
 Operator : MA/JU
 Sample : P3359-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GF6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 02 09:12:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.465	152	4321m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.223	136	13426	0.400	ng/ul	#-0.09
9) Acenaphthene-d10	14.115	164	7058	0.400	ng/ul	-0.05
13) Phenanthrene-d10	16.886	188	13390m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.134	240	10580m	0.400	ng/ul	-0.02
23) Perylene-d12	23.299	264	11466m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.048	96	23029	4.213	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.851	152	5664	0.259	ng/ul	-0.08
18) Fluoranthene-d10	18.935	212	9671	0.323	ng/ul	-0.04
Target Compounds						Qvalue
5) Naphthalene	10.273	128	2633	0.076	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033195.D
Acq On : 02 Aug 2024 08:46
Operator : MA/JU
Sample : P3359-17
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GF6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Aug 02 09:12:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

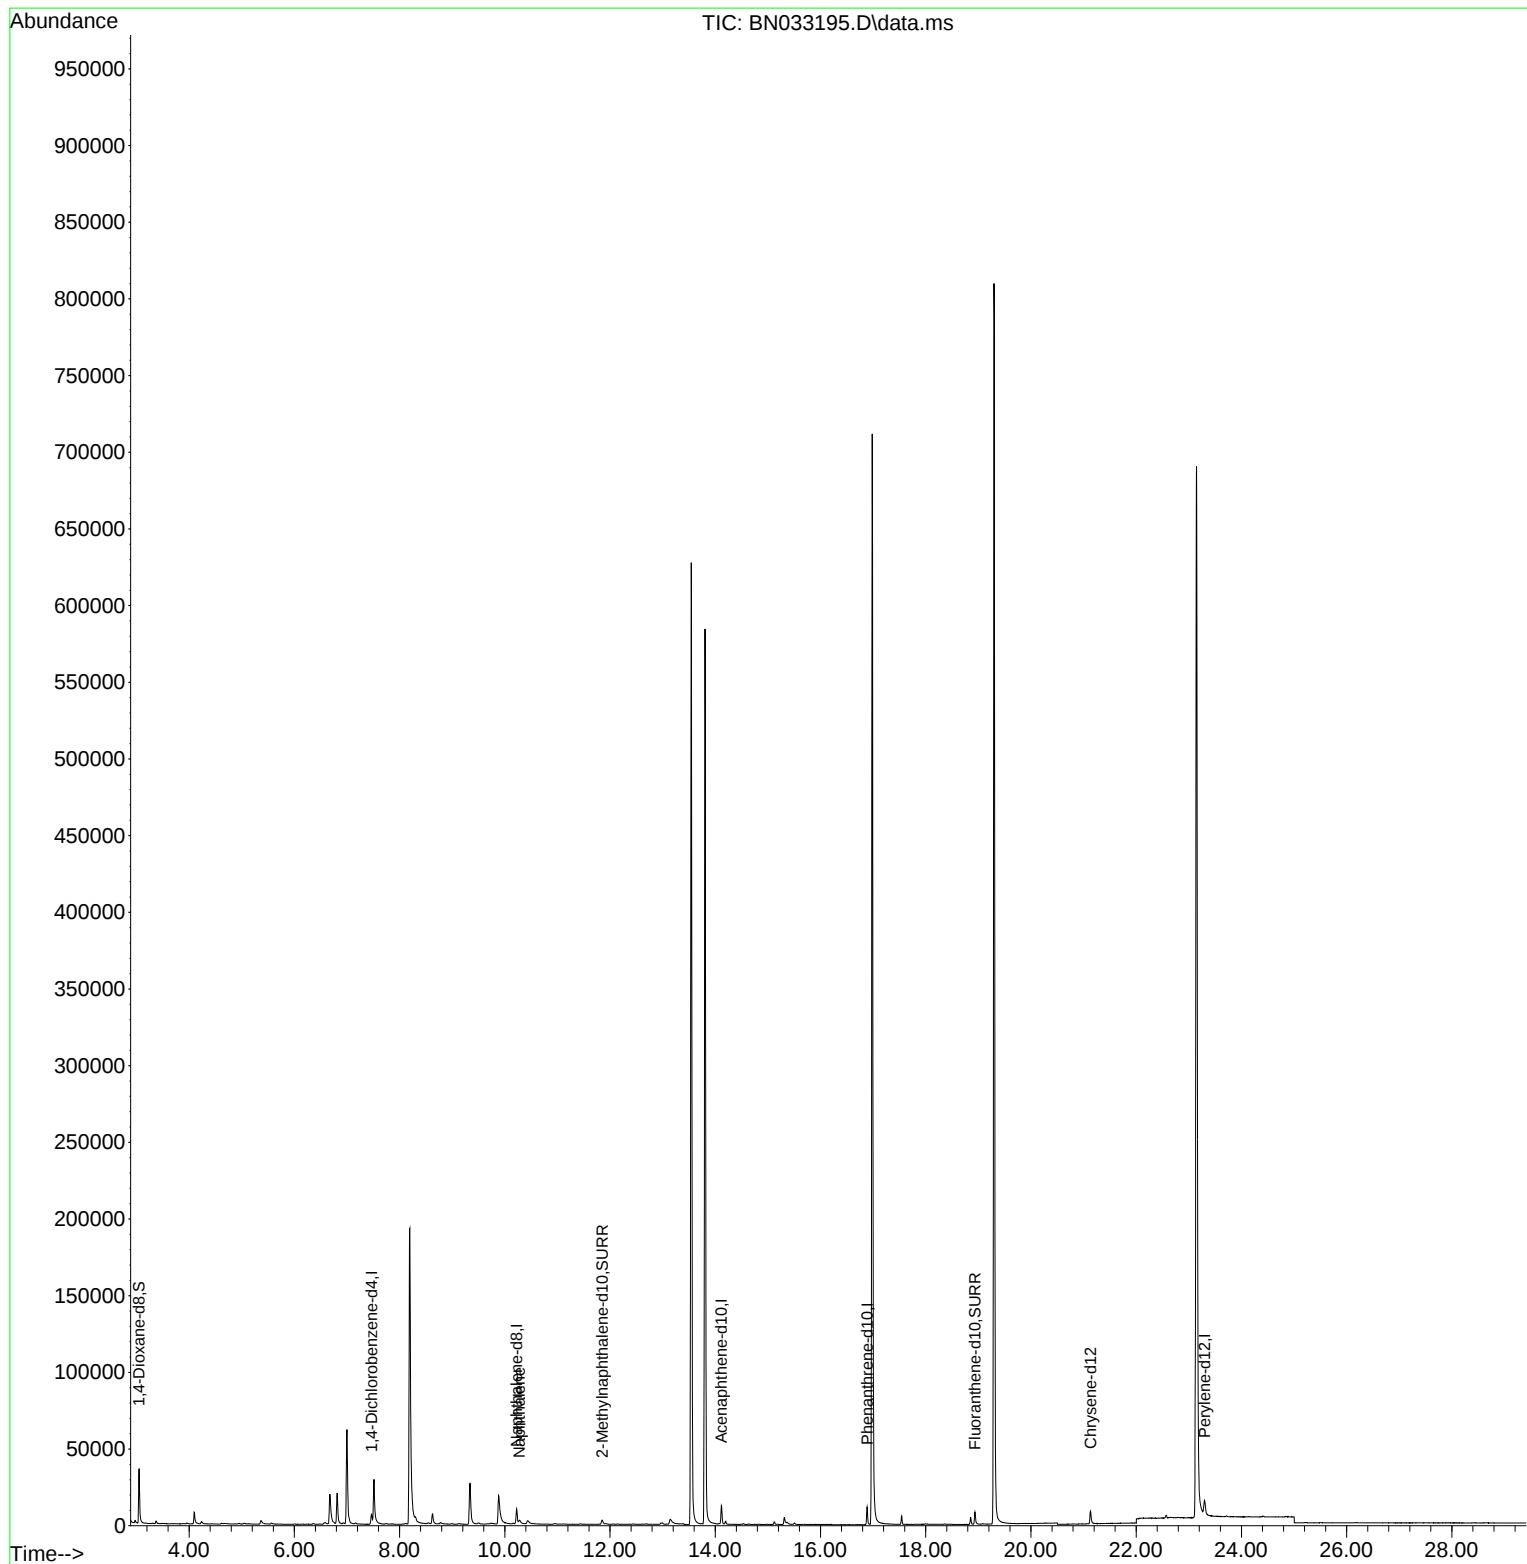

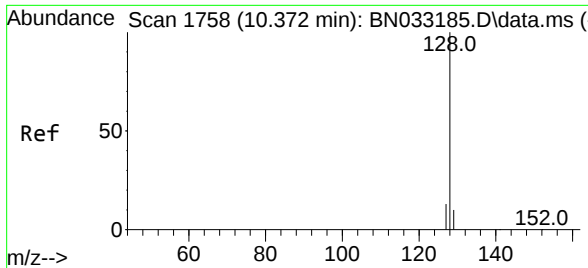

#5
 Naphthalene
 Concen: 0.076 ng/ul
 RT: 10.273 min Scan# 11
 Delta R.T. -0.104 min
 Lab File: BN033195.D
 Acq: 02 Aug 2024 08:46

Instrument :
 BNA_N
 ClientSampleId :
 E1GF6

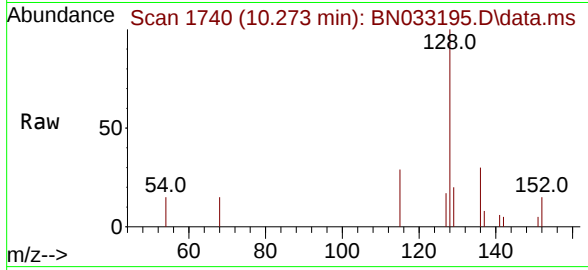

Tgt Ion:	128	Resp:	263
Ion	Ratio	Lower	Upper
128	100		
129	19.8	12.0	18.0
127	17.0	12.7	19.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

