

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033198.D
 Acq On : 02 Aug 2024 10:35
 Operator : MA/JU
 Sample : P3359-17RE
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GF6RE

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 02 12:59:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.470	152	4051m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.223	136	13262	0.400	ng/ul	#-0.09
9) Acenaphthene-d10	14.120	164	7749	0.400	ng/ul	-0.04
13) Phenanthrene-d10	16.886	188	16135m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.137	240	10159m	0.400	ng/ul	-0.01
23) Perylene-d12	23.305	264	8503m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.048	96	22291	4.350	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.851	152	5685	0.263	ng/ul	-0.08
18) Fluoranthene-d10	18.935	212	11598	0.403	ng/ul	-0.04
Target Compounds						Qvalue
5) Naphthalene	10.273	128	1676	0.049	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033198.D
Acq On : 02 Aug 2024 10:35
Operator : MA/JU
Sample : P3359-17RE
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GF6RE

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Aug 02 12:59:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

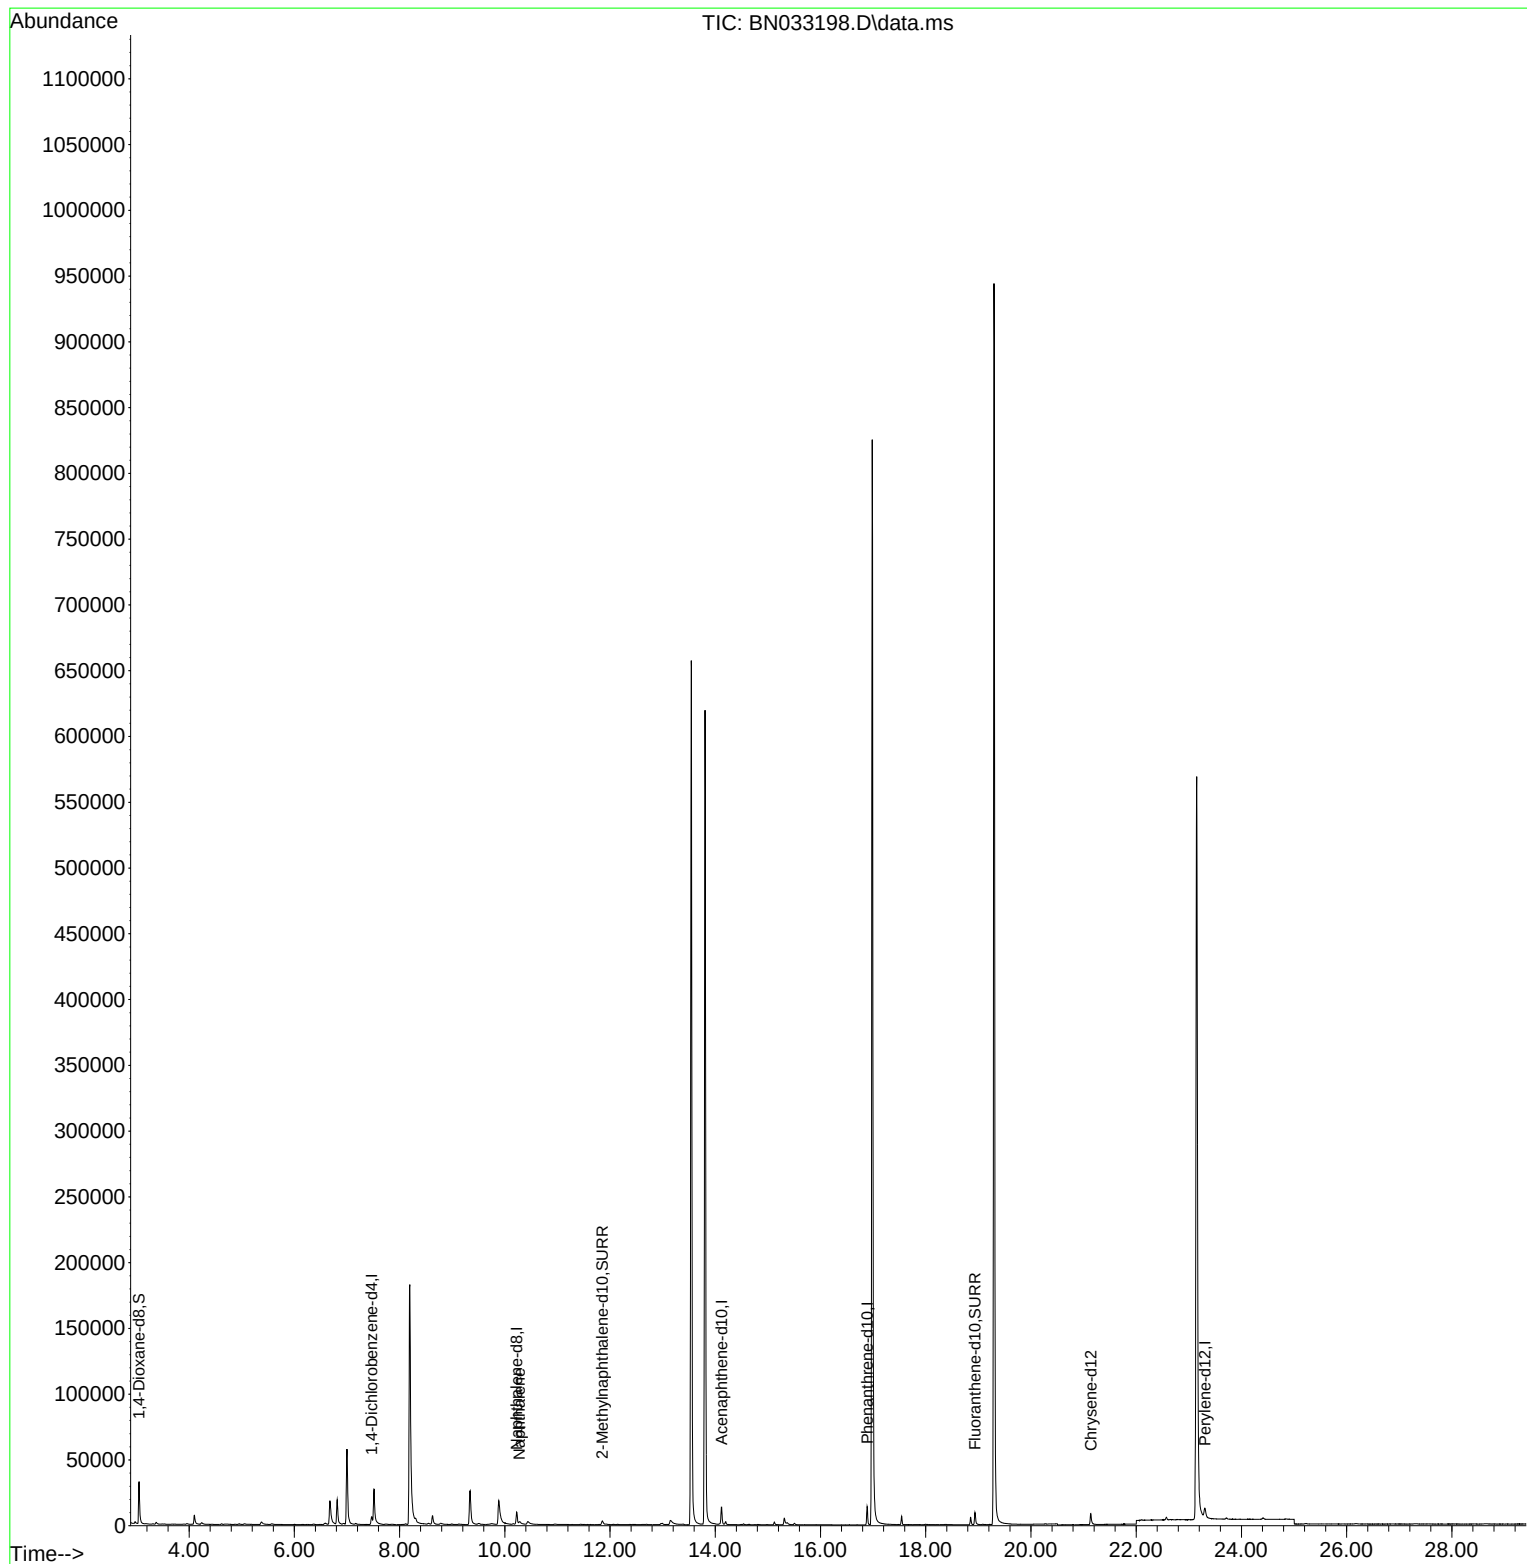

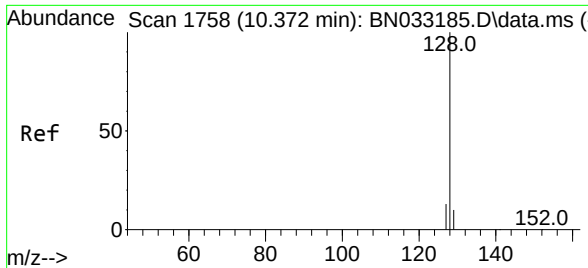

#5
Naphthalene
Concen: 0.049 ng/ul
RT: 10.273 min Scan# 1758
Delta R.T. -0.104 min
Lab File: BN033198.D
Acq: 02 Aug 2024 10:35

Instrument :
BNA_N
ClientSampleId :
E1GF6RE

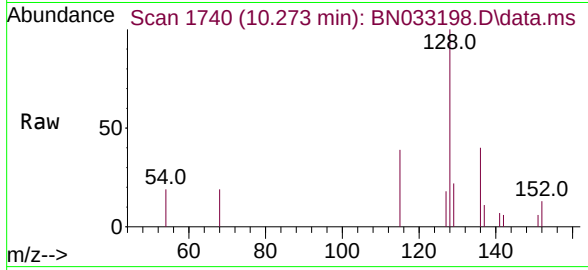

Tgt Ion:	128	Resp:	1670
Ion	Ratio	Lower	Upper
128	100		
129	21.7	12.0	18.0
127	18.2	12.7	19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

