

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080320\
 Data File : BN011340.D
 Acq On : 03 Aug 2020 19:27
 Operator : CG/JU
 Sample : L3419-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Quant Time: Aug 04 06:11:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	1346	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	5334	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.09	164	3108	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.85
16) Chrysene-d12	21.07	240	6597	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	7553	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	2260	0.17	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	6072	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.26	202	1028	0.034	ng/ul#	1
23) Benzo(a)pyrene	23.05	252	2482	0.091	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080320\
Data File : BN011340.D
Acq On : 03 Aug 2020 19:27
Operator : CG/JU
Sample : L3419-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA5

Quant Time: Aug 04 06:11:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 03 10:06:56 2020
Response via : Initial Calibration

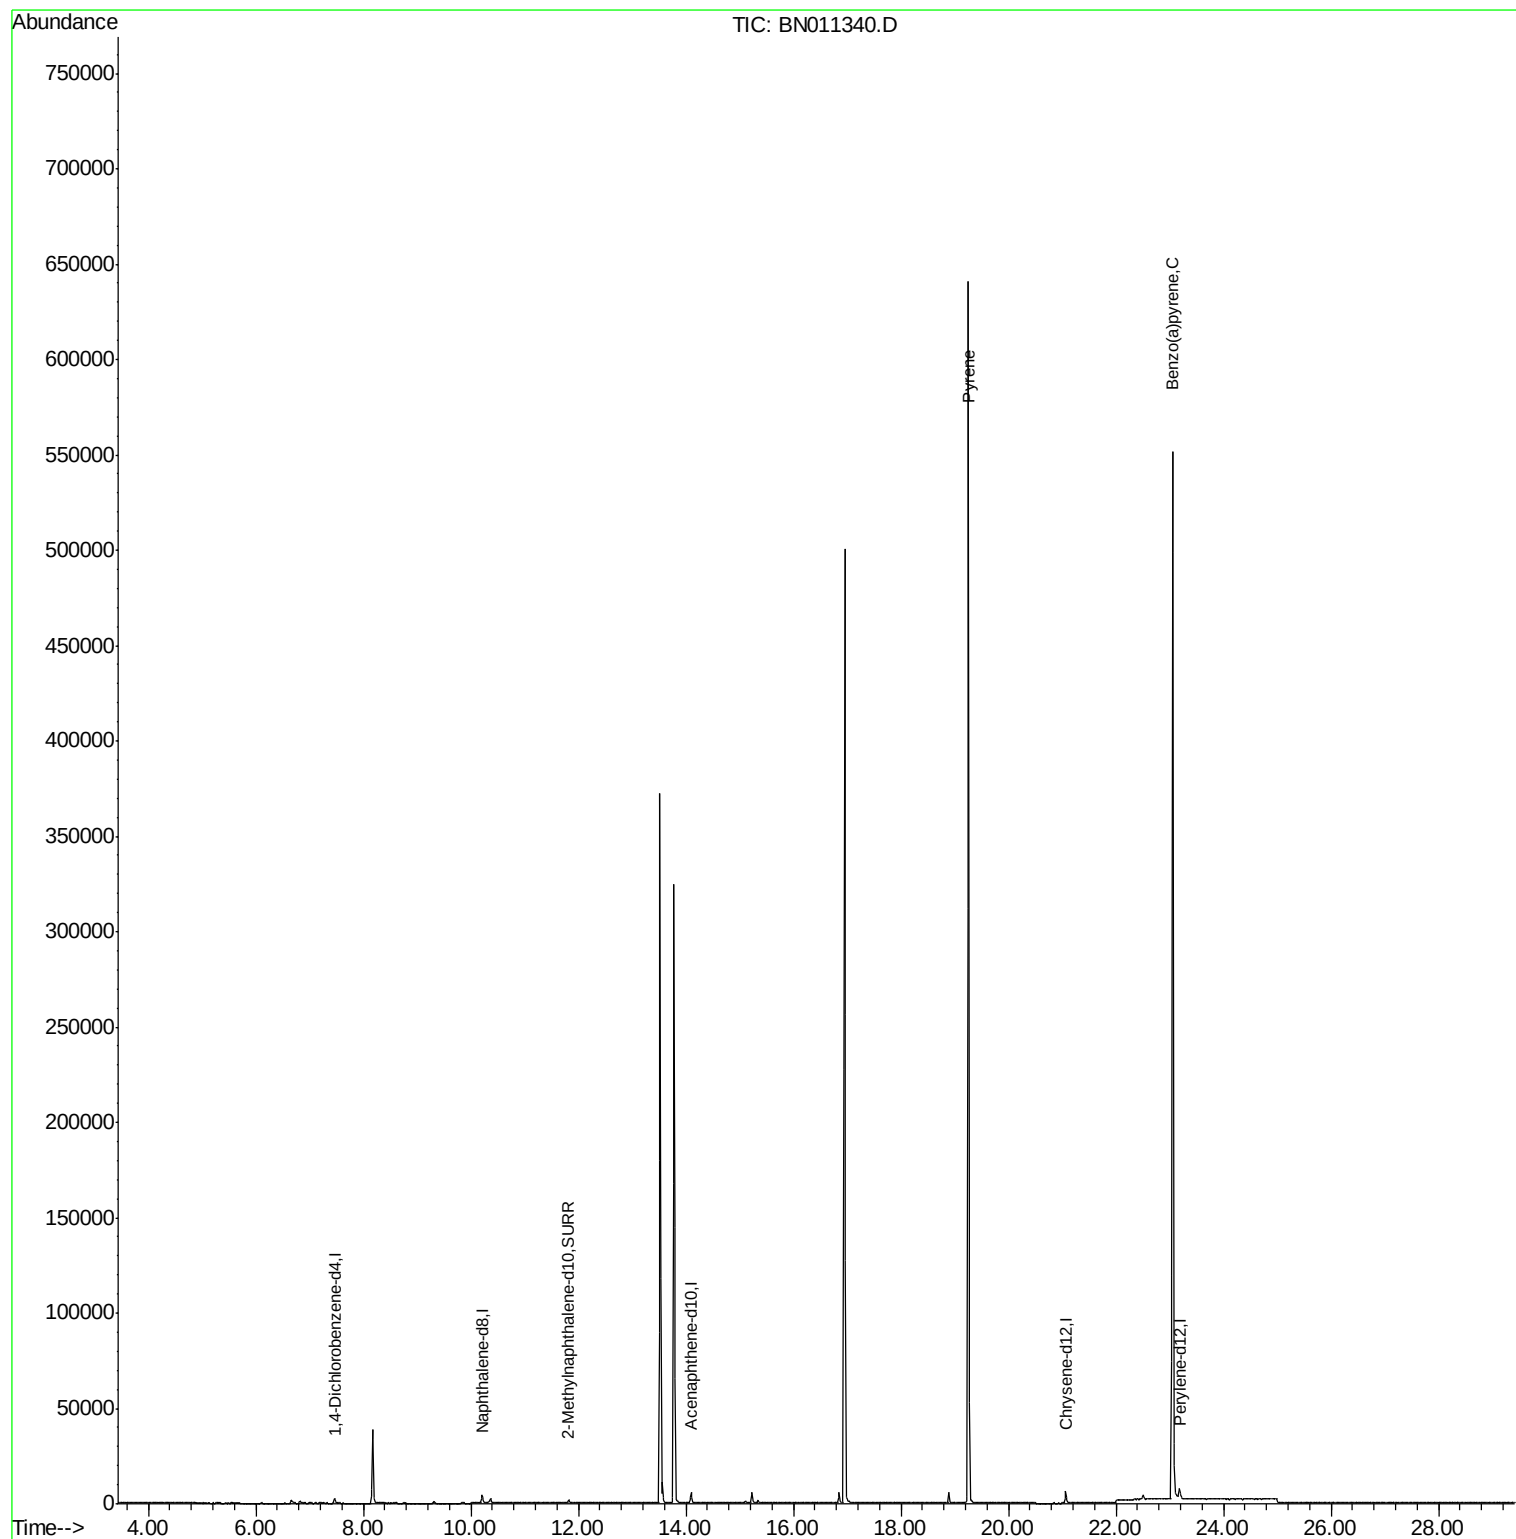

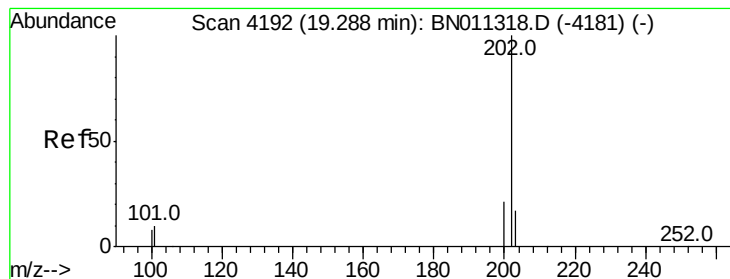

#17

Pyrene

Concen: 0.034 ng/ul

RT: 19.26 min Scan# 4185

Delta R.T. -0.03 min

Lab File: BN011340.D

Acq: 03 Aug 2020 19:27

Instrument :

BNA_N

ClientSampleId :

C0AA5


Tot Ion:202 Resp: 1028

Ion Ratio Lower Upper

202 100

101 183.4 8.5 12.7#




100 1308.7 7.1 10.7#

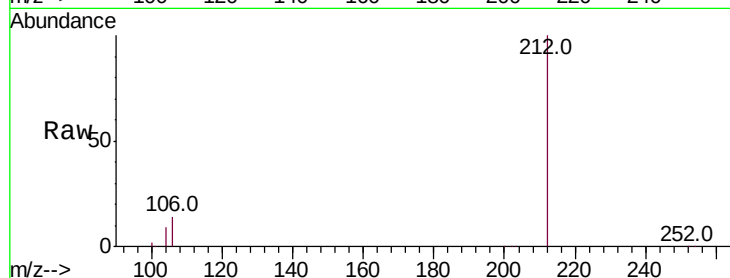

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

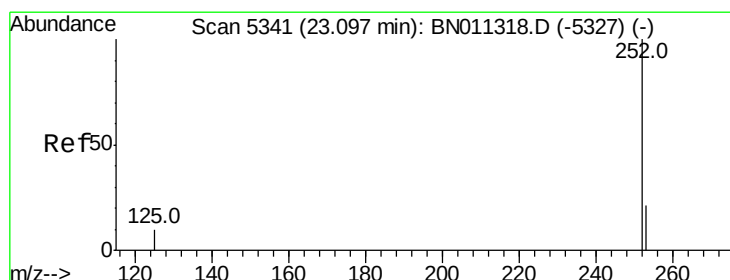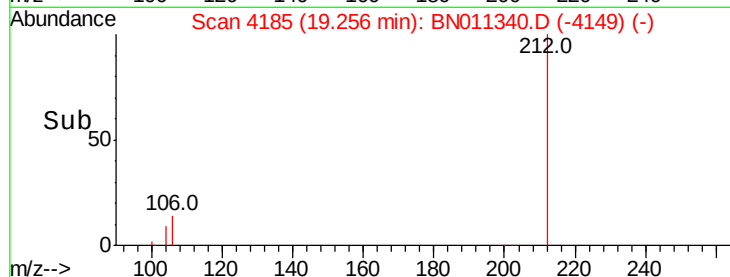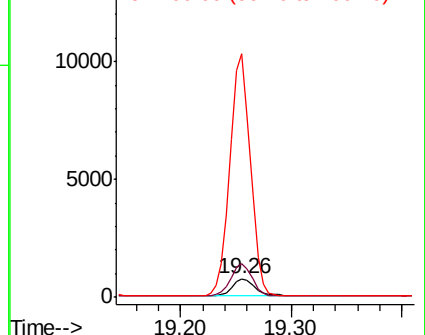

#23

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 23.05 min Scan# 5326

Delta R.T. -0.04 min

Lab File: BN011340.D

Acq: 03 Aug 2020 19:27


Tgt Ion:252 Resp: 2482

Ion Ratio Lower Upper

252 100

253 45.6 22.6 34.0#

125 36.6 12.6 18.8#

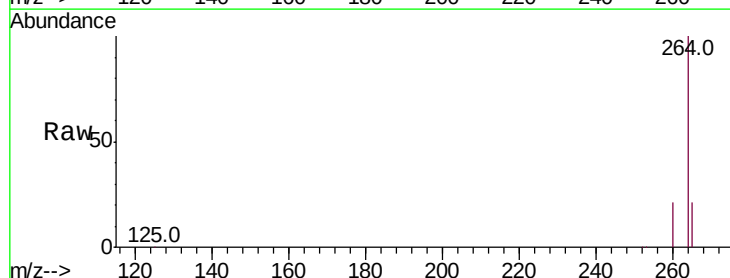

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

