

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080320\
 Data File : BN011347.D
 Acq On : 04 Aug 2020 00:51
 Operator : CG/JU
 Sample : L3419-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE9

Quant Time: Aug 04 06:47:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 04 06:45:43 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1940	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	7017	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.09	164	4125	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.85
16) Chrysene-d12	21.06	240	8703	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	9294	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	2755	0.16	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	6774	0.00	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.26	128	617	0.030	ng/ul#	75
7) Acenaphthylene	13.81	152	2358	0.120	ng/ul	97
17) Pyrene	19.28	202	17513	0.443	ng/ul	99
18) Benzo(a)anthracene	21.05	228	10977	0.328	ng/ul	97
19) Chrysene	21.10	228	13768	0.359	ng/ul	98
21) Benzo(b)fluoranthene	22.56	252	28628	0.738	ng/ul	99
22) Benzo(k)fluoranthene	22.56	252	28628	0.658	ng/ul#	95
23) Benzo(a)pyrene	23.09	252	10698	0.317	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	25.24	276	8754	0.247	ng/ul#	95
25) Dibenzo(a,h)anthracene	25.25	278	2050	0.073	ng/ul#	71
26) Benzo(g,h,i)perylene	25.87	276	7441	0.232	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080320\
Data File : BN011347.D
Acq On : 04 Aug 2020 00:51
Operator : CG/JU
Sample : L3419-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE9

Quant Time: Aug 04 06:47:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 04 06:45:43 2020
Response via : Initial Calibration

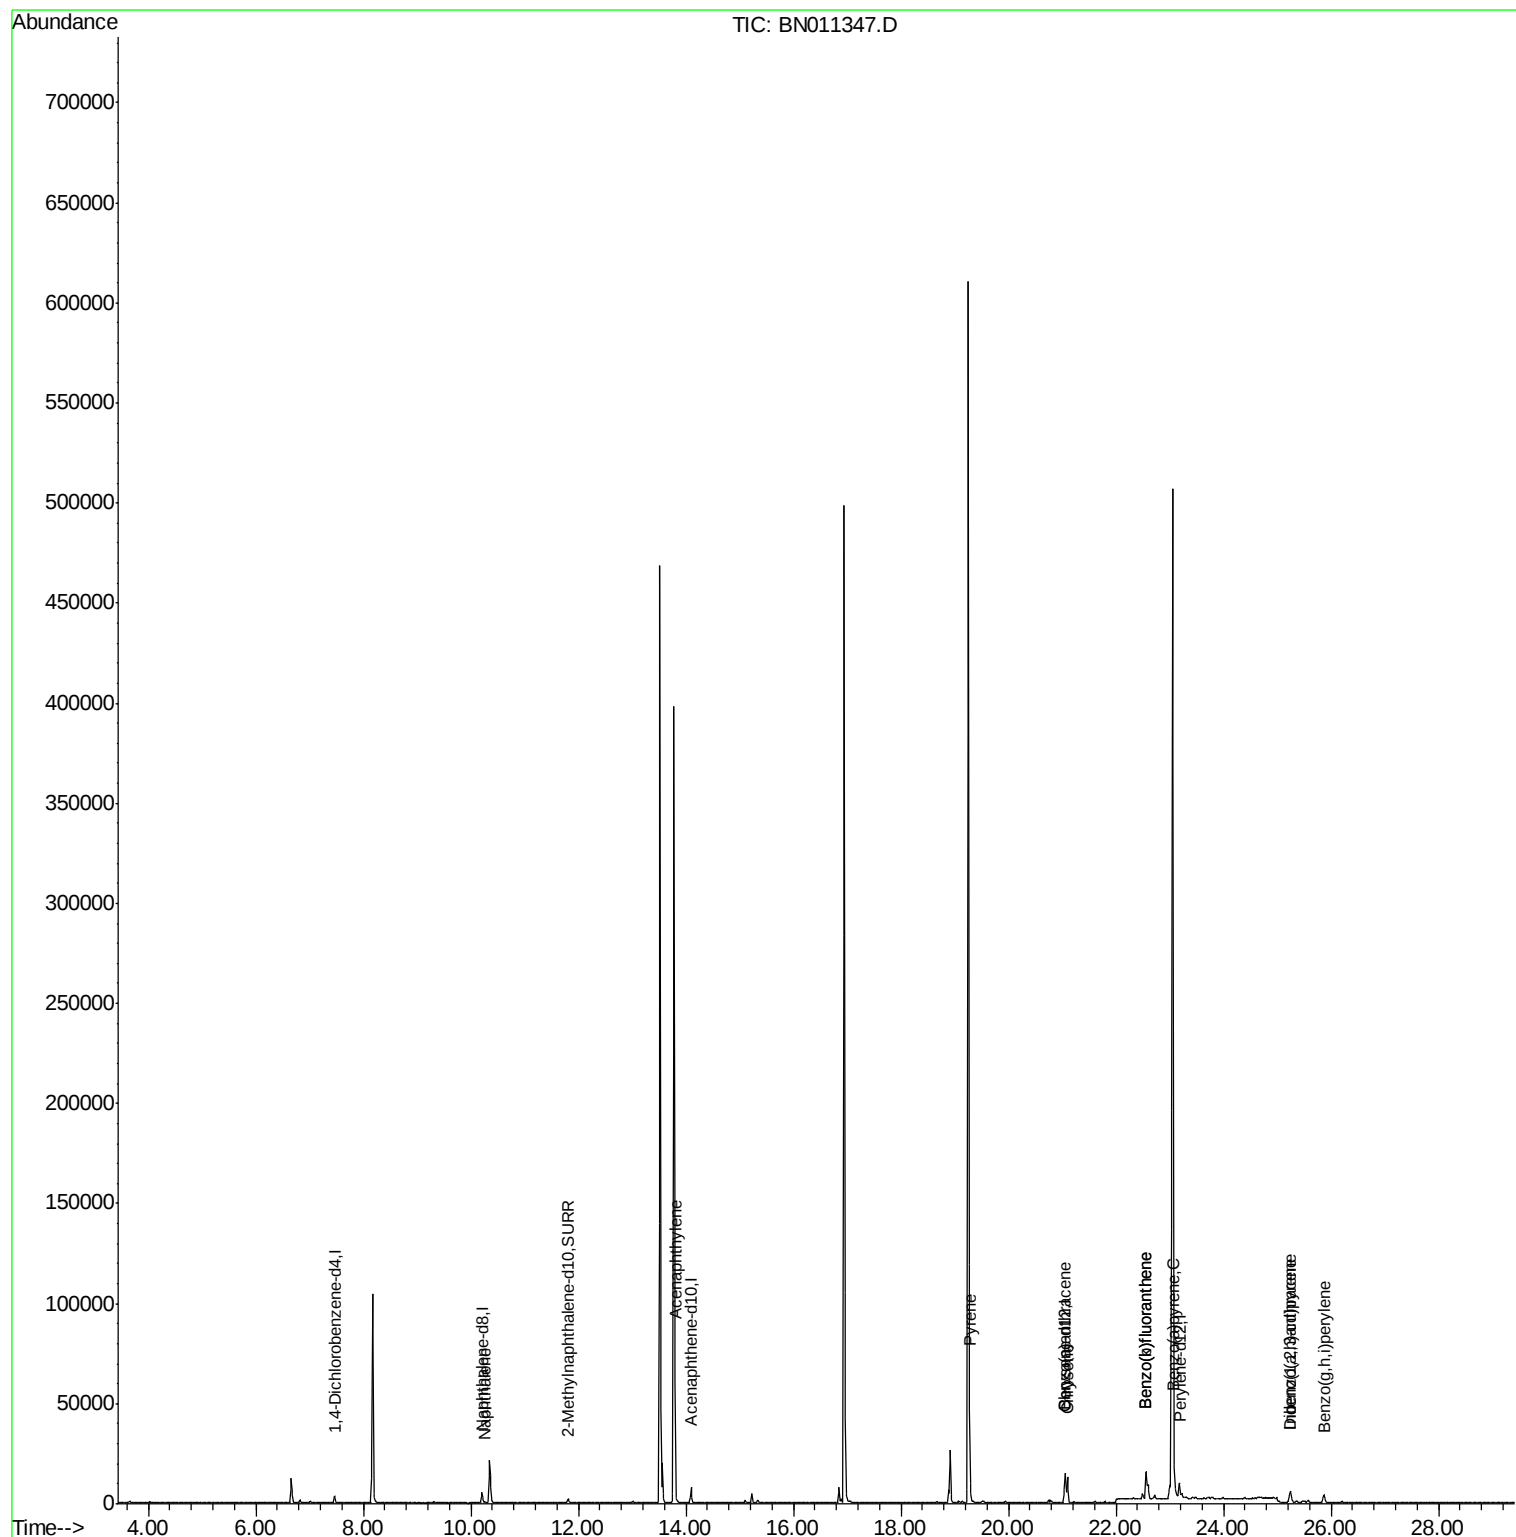

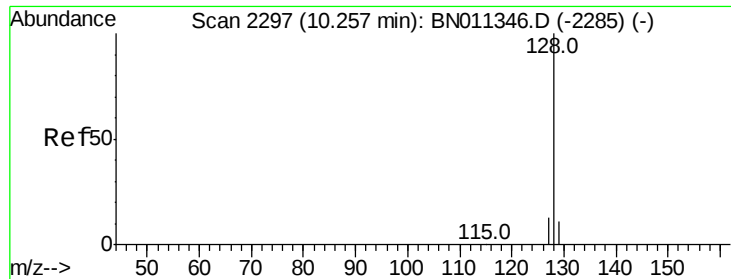

#3

Naphthalene

Concen: 0.030 ng/ul

RT: 10.26 min Scan# 2297

Delta R.T. 0.00 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51

Instrument :

BNA_N

ClientSampleId :

C0AE9


Tot Ion:128 Resp: 617

Ion Ratio Lower Upper

128 100

129 22.6 9.6 14.4#




127 23.3 11.2 16.8#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

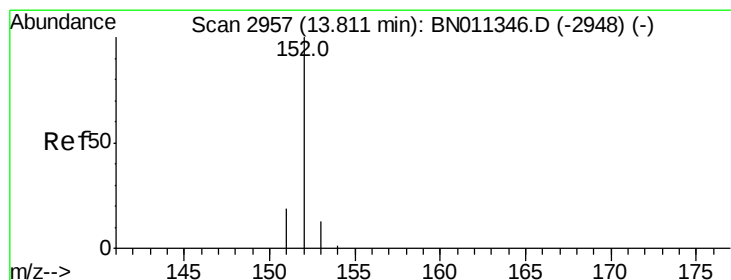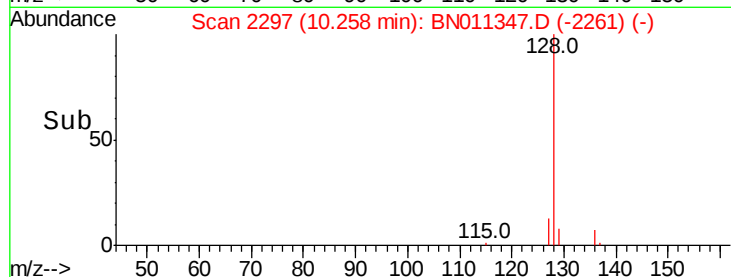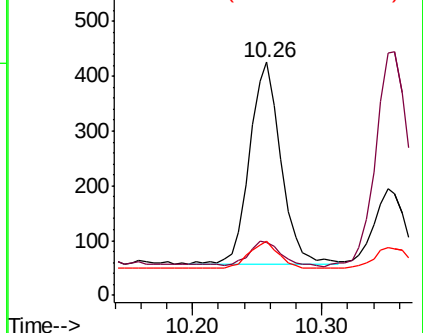

#7

Acenaphthylene

Concen: 0.120 ng/ul

RT: 13.81 min Scan# 2956

Delta R.T. -0.00 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51


Tgt Ion:152 Resp: 2358

Ion Ratio Lower Upper

152 100

151 22.3 17.1 25.7



153 16.1 11.4 17.0




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



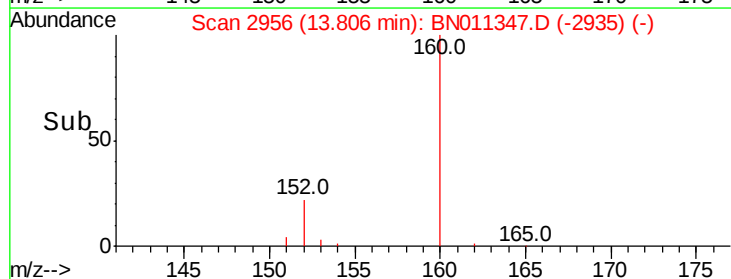
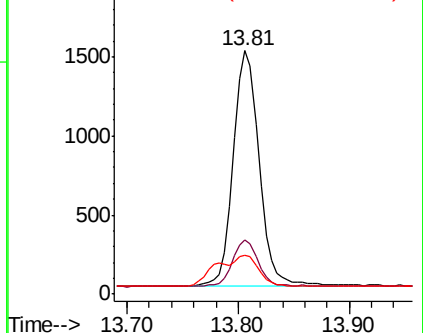


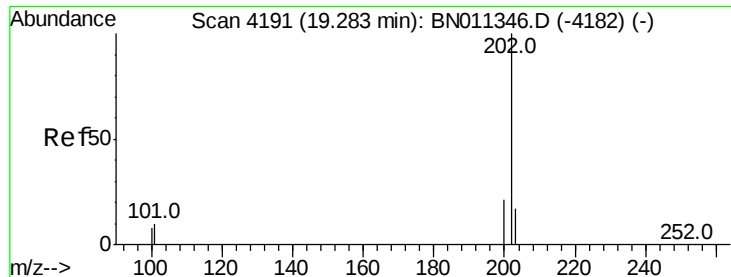

#17
Pvrene
Concen: 0.443 ng/ul
RT: 19.28 min Scan# 4191
Delta R.T. 0.00 min
Lab File: BN011347.D
Acq: 04 Aug 2020 00:51




Instrument :
BNA_N
ClientSampleId :
C0AE9


Tot Ion:202 Resp: 17513
Ion Ratio Lower Upper
202 100
101 10.0 8.5 12.7
100 8.8 7.1 10.7

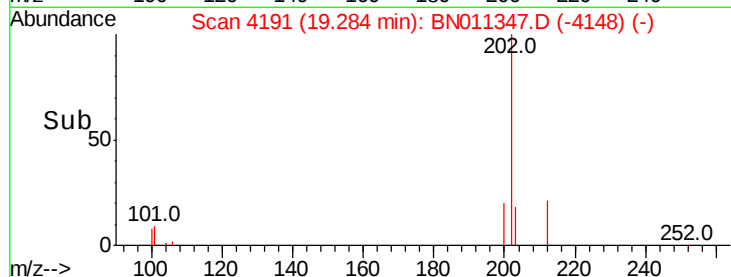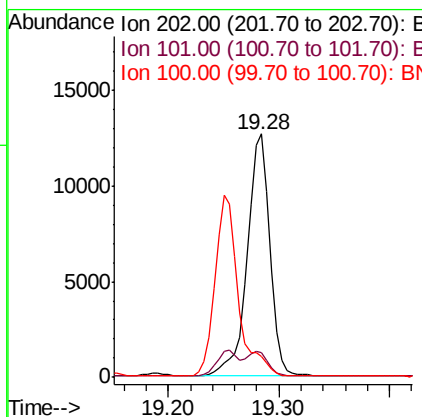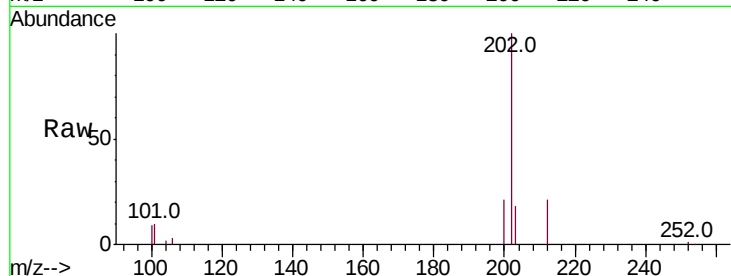

#18
Benzo(a)anthracene
Concen: 0.328 ng/ul
RT: 21.05 min Scan# 4639
Delta R.T. -0.00 min
Lab File: BN011347.D
Acq: 04 Aug 2020 00:51

Tgt Ion:228 Resp: 10977
Ion Ratio Lower Upper
228 100
229 20.6 16.1 24.1
226 29.8 22.2 33.2

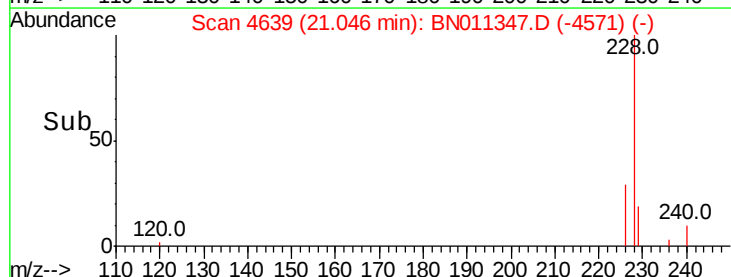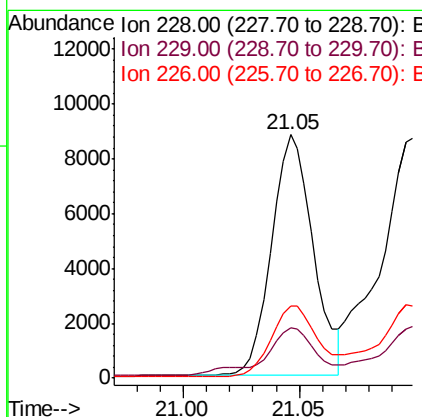

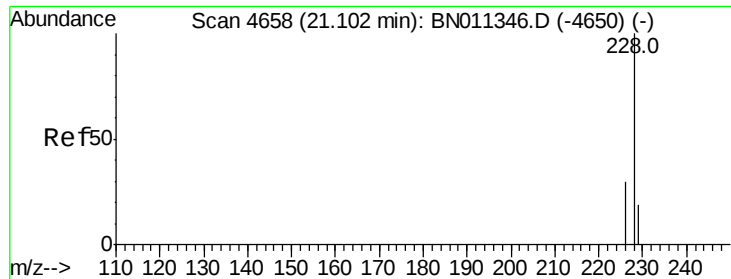

#19

Chrysene

Concen: 0.359 ng/ul

RT: 21.10 min Scan# 4657

Delta R.T. -0.00 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51

Instrument :

BNA_N

ClientSampleId :

C0AE9


Tot Ion:228 Resp: 13768

Ion Ratio Lower Upper

228 100

226 29.9 24.5 36.7




229 21.4 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

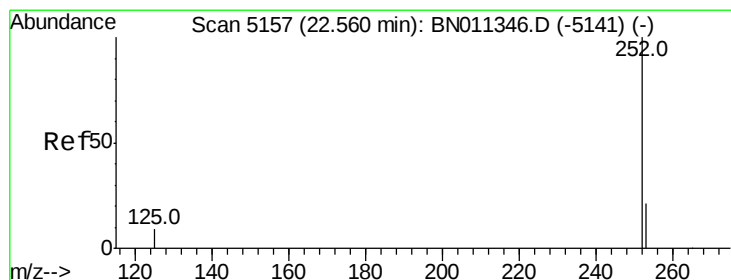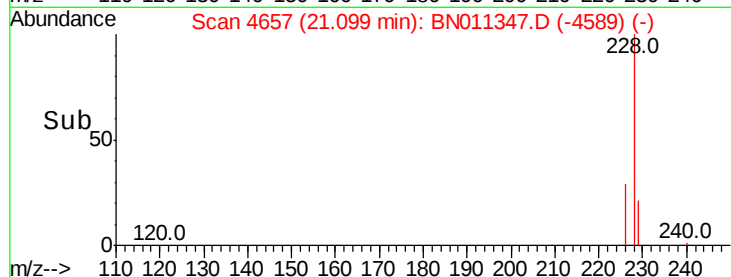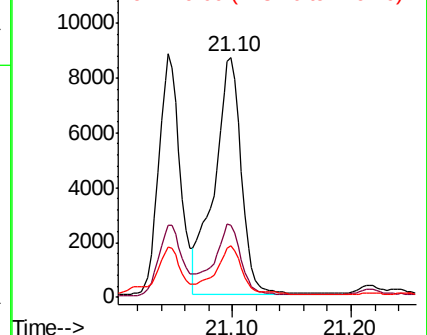

#21

Benzo(b)fluoranthene

Concen: 0.738 ng/ul

RT: 22.56 min Scan# 5156

Delta R.T. -0.00 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51


Tgt Ion:252 Resp: 28628

Ion Ratio Lower Upper

252 100

253 25.3 0.0 51.8



125 12.5 0.0 24.2

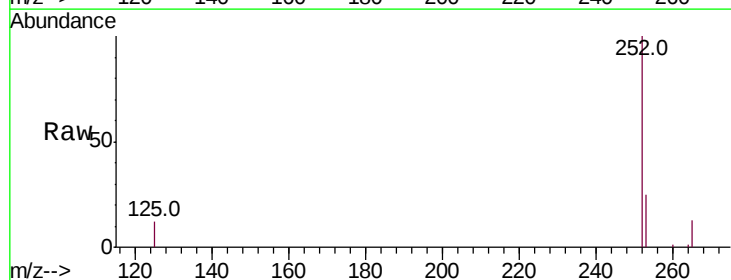


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

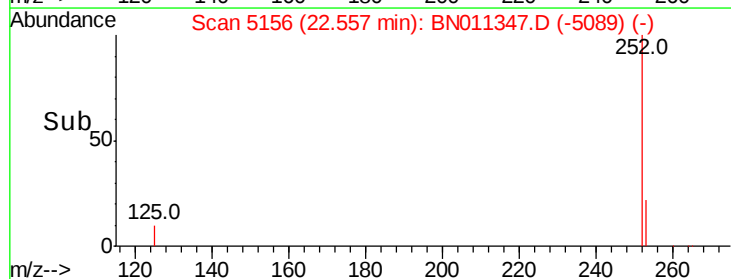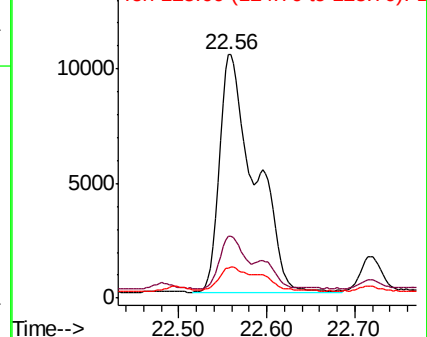

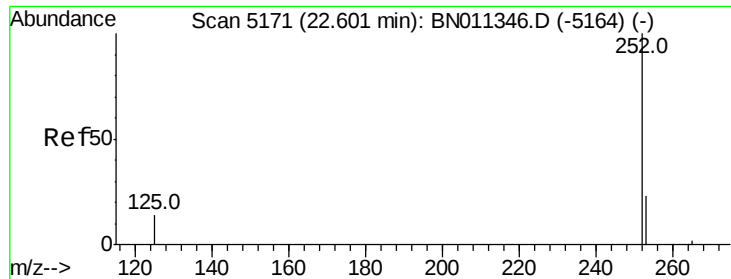

#22

Benzo(k)fluoranthene

Concen: 0.658 ng/ul

RT: 22.56 min Scan# 5156

Delta R.T. -0.04 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51

Instrument :

BNA_N

ClientSampleId :

C0AE9


Tot Ion:252 Resp: 28628

Ion Ratio Lower Upper

252 100

253 25.3 21.4 32.0




125 12.5 12.6 18.8#

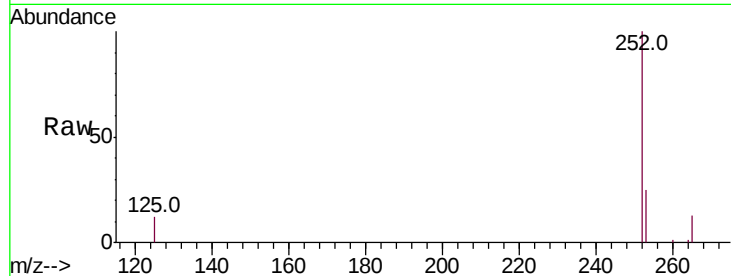

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

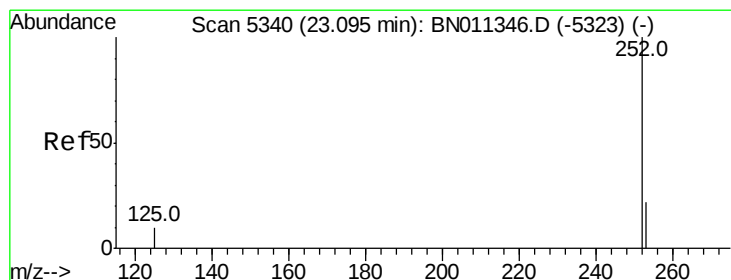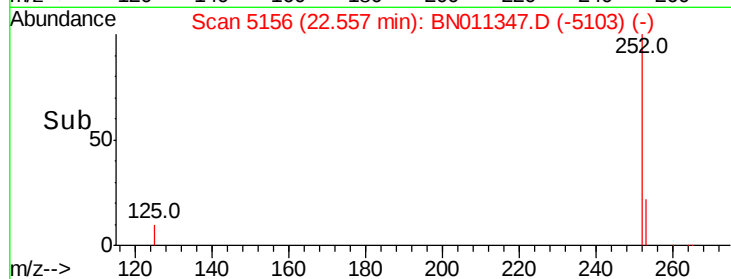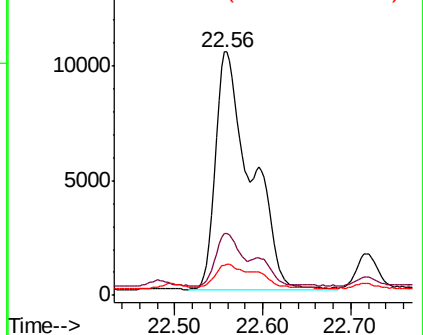

#23

Benzo(a)pyrene

Concen: 0.317 ng/ul

RT: 23.09 min Scan# 5338

Delta R.T. -0.01 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51


Tgt Ion:252 Resp: 10698

Ion Ratio Lower Upper

252 100

253 27.4 22.6 34.0



125 13.9 12.6 18.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

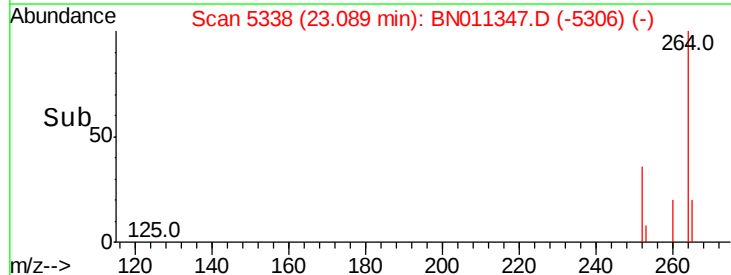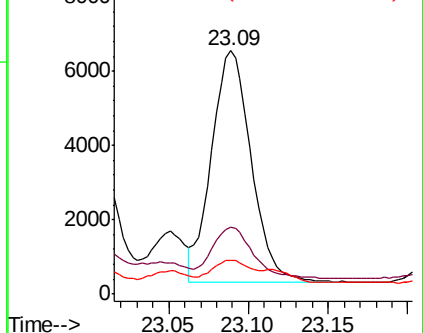

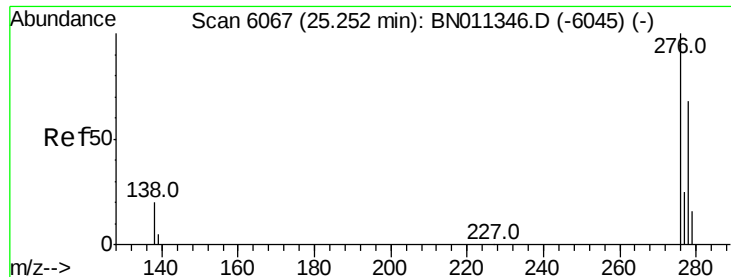

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.247 ng/ul

RT: 25.24 min Scan# 6064

Delta R.T. -0.01 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51

Instrument :

BNA_N

ClientSampleId :

C0AE9


Tot Ion:276 Resp: 8754

Ion Ratio Lower Upper

276 100

138 20.3 18.1 27.1




227 0.0 0.2 0.4#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

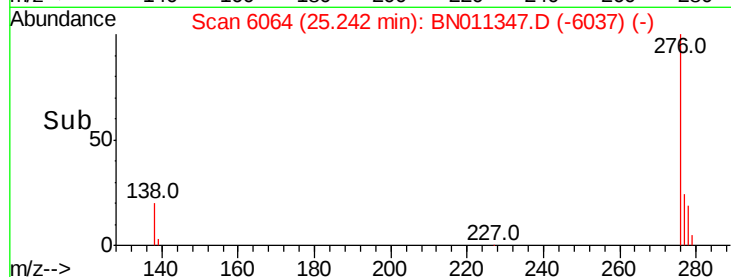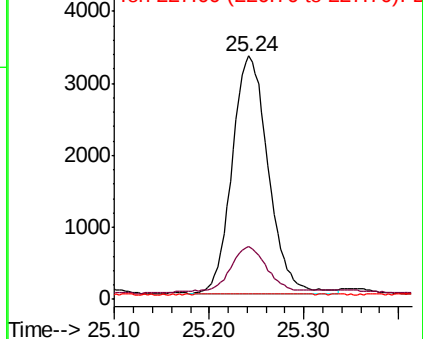

#25

Dibenzo(a,h)anthracene

Concen: 0.073 ng/ul

RT: 25.25 min Scan# 6067

Delta R.T. -0.01 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51


Tgt Ion:278 Resp: 2050

Ion Ratio Lower Upper

278 100

139 25.3 14.0 21.0#



279 47.5 22.9 34.3#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

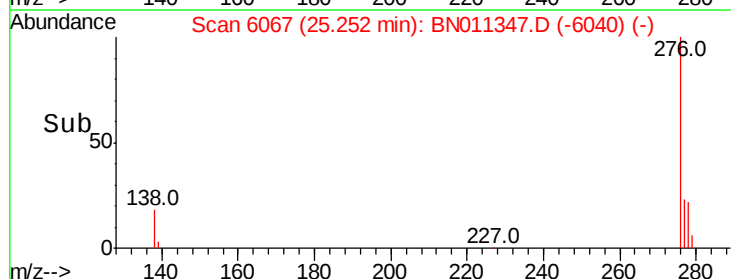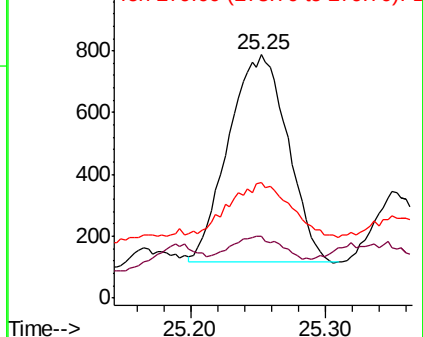

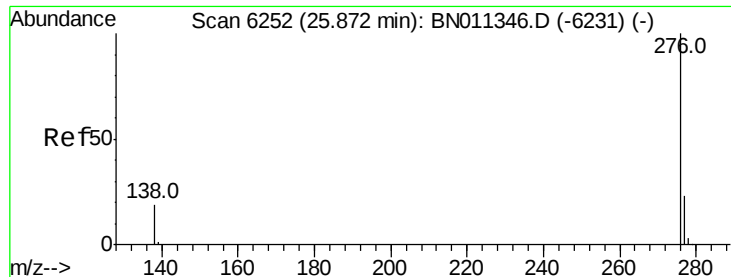

#26

Benzo(a,h,i)perylene

Concen: 0.232 ng/ul

RT: 25.87 min Scan# 6251

Delta R.T. -0.00 min

Lab File: BN011347.D

Acq: 04 Aug 2020 00:51

Instrument :

BNA_N

ClientSampleId :

C0AE9


Tot Ion:276 Resp: 7441

Ion Ratio Lower Upper

276 100

138 22.4 16.4 24.6

277 26.1 20.2 30.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

