

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011332.D
 Acq On : 03 Aug 2020 14:39
 Operator : CG/JU
 Sample : PB130482BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Quant Time: Aug 03 15:18:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:27:20 AM

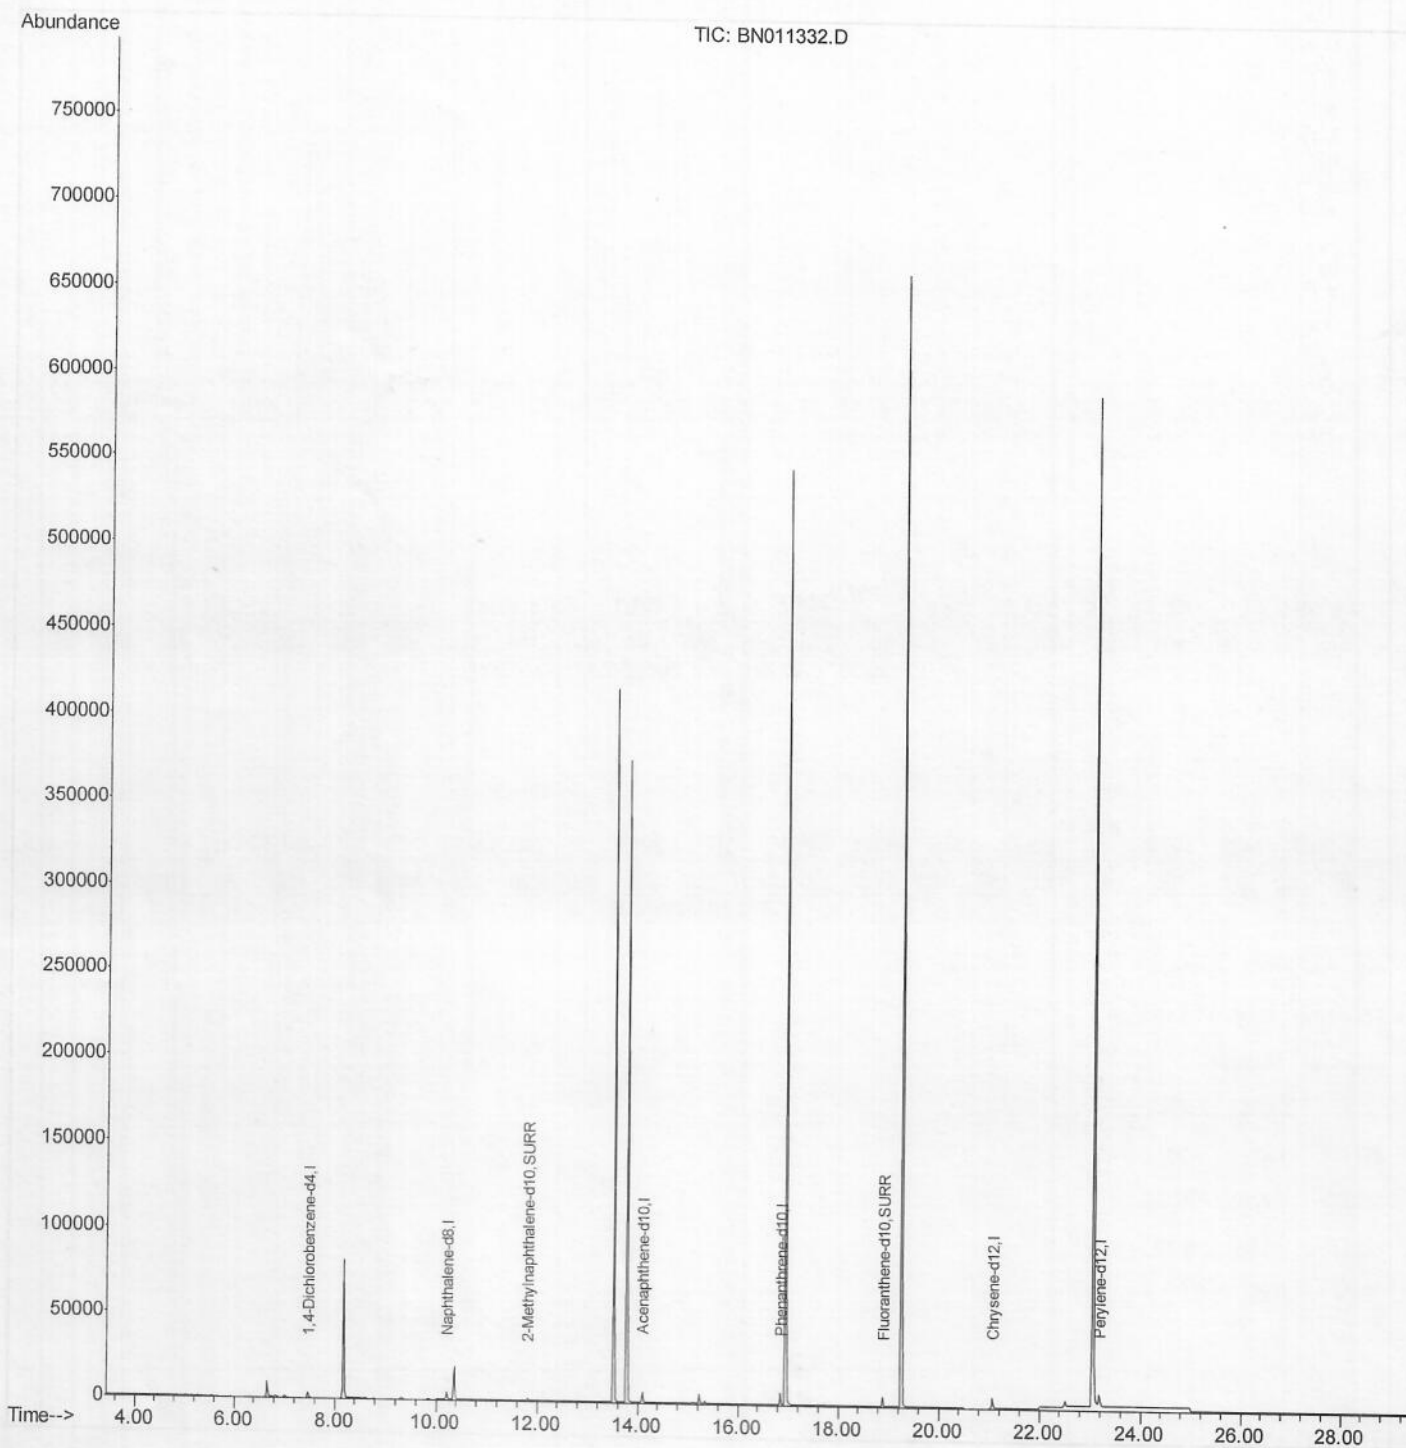

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011332.D
 Acq On : 03 Aug 2020 14:39
 Operator : CG/JU
 Sample : PB130482BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:27:20 AM

Quant Time: Aug 03 15:17:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

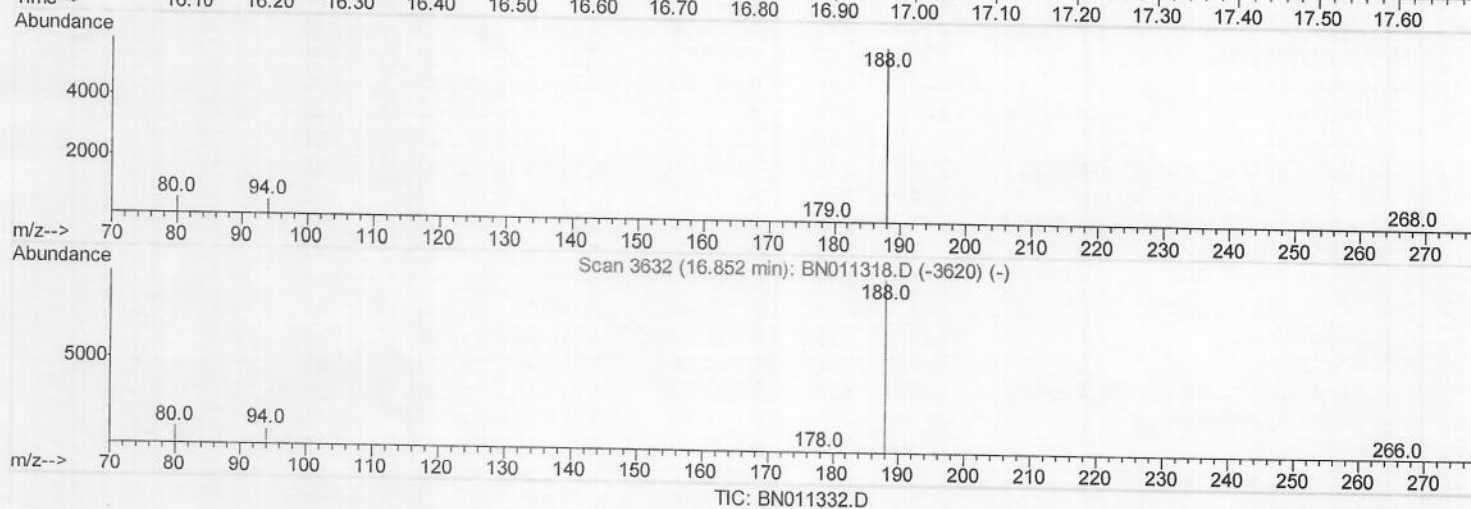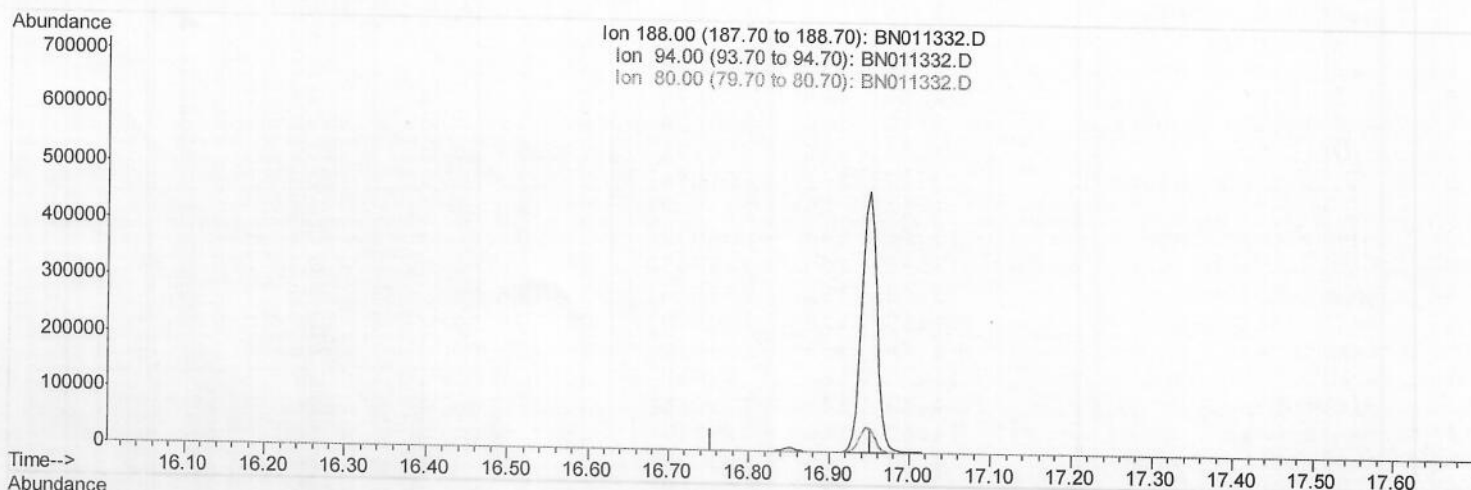

(10) Phenanthrene-d10 (I)

16.853min (-16.853) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011332.D
 Acq On : 03 Aug 2020 14:39
 Operator : CG/JU
 Sample : PB130482BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:27:20 AM

Quant Time: Aug 03 15:17:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

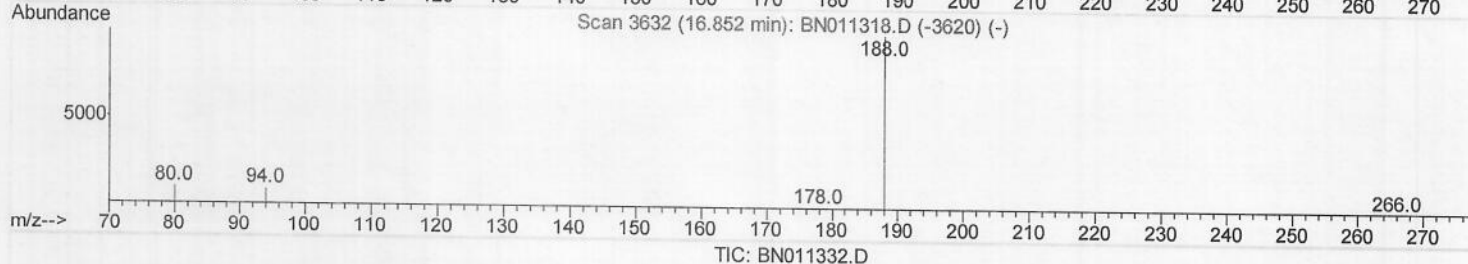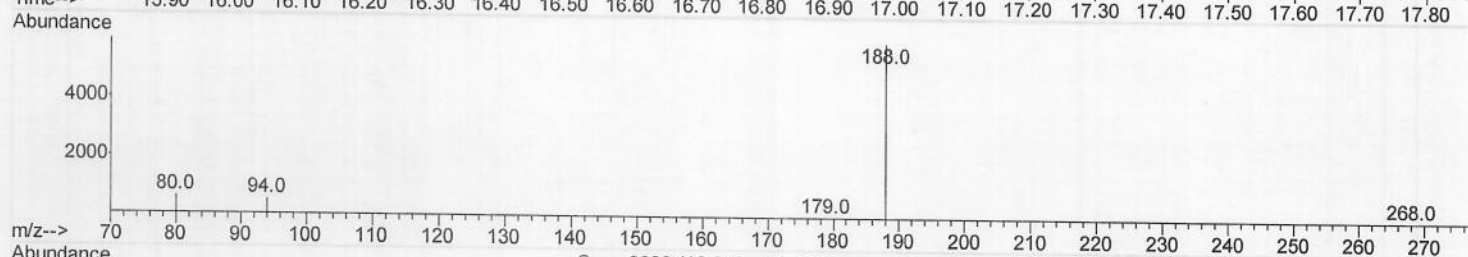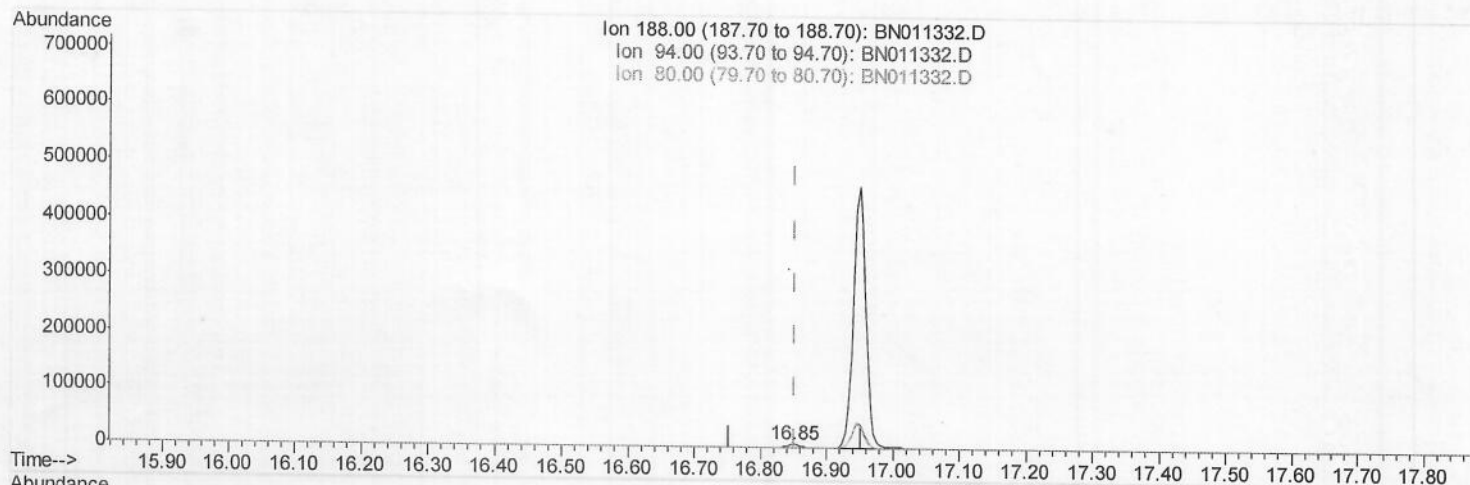

(10) Phenanthrene-d10 (I)

16.848min (-0.004) 0.40ng/ul m

8 JU 08/05/20

response 8070

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	9.19
80.00	10.30	10.70
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011332.D
 Acq On : 03 Aug 2020 14:39
 Operator : CG/JU
 Sample : PB130482BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:27:20 AM

Quant Time: Aug 03 15:18:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	1496	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	5627	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	3620	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	8070m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	7090	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	8808	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	2494	0.18	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	6424	0.16	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

3 JU
 08/05/20