

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011357.D
 Acq On : 04 Aug 2020 08:56
 Operator : CG/JU
 Sample : L3443-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AA7

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:27 AM

Quant Time: Aug 04 11:48:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

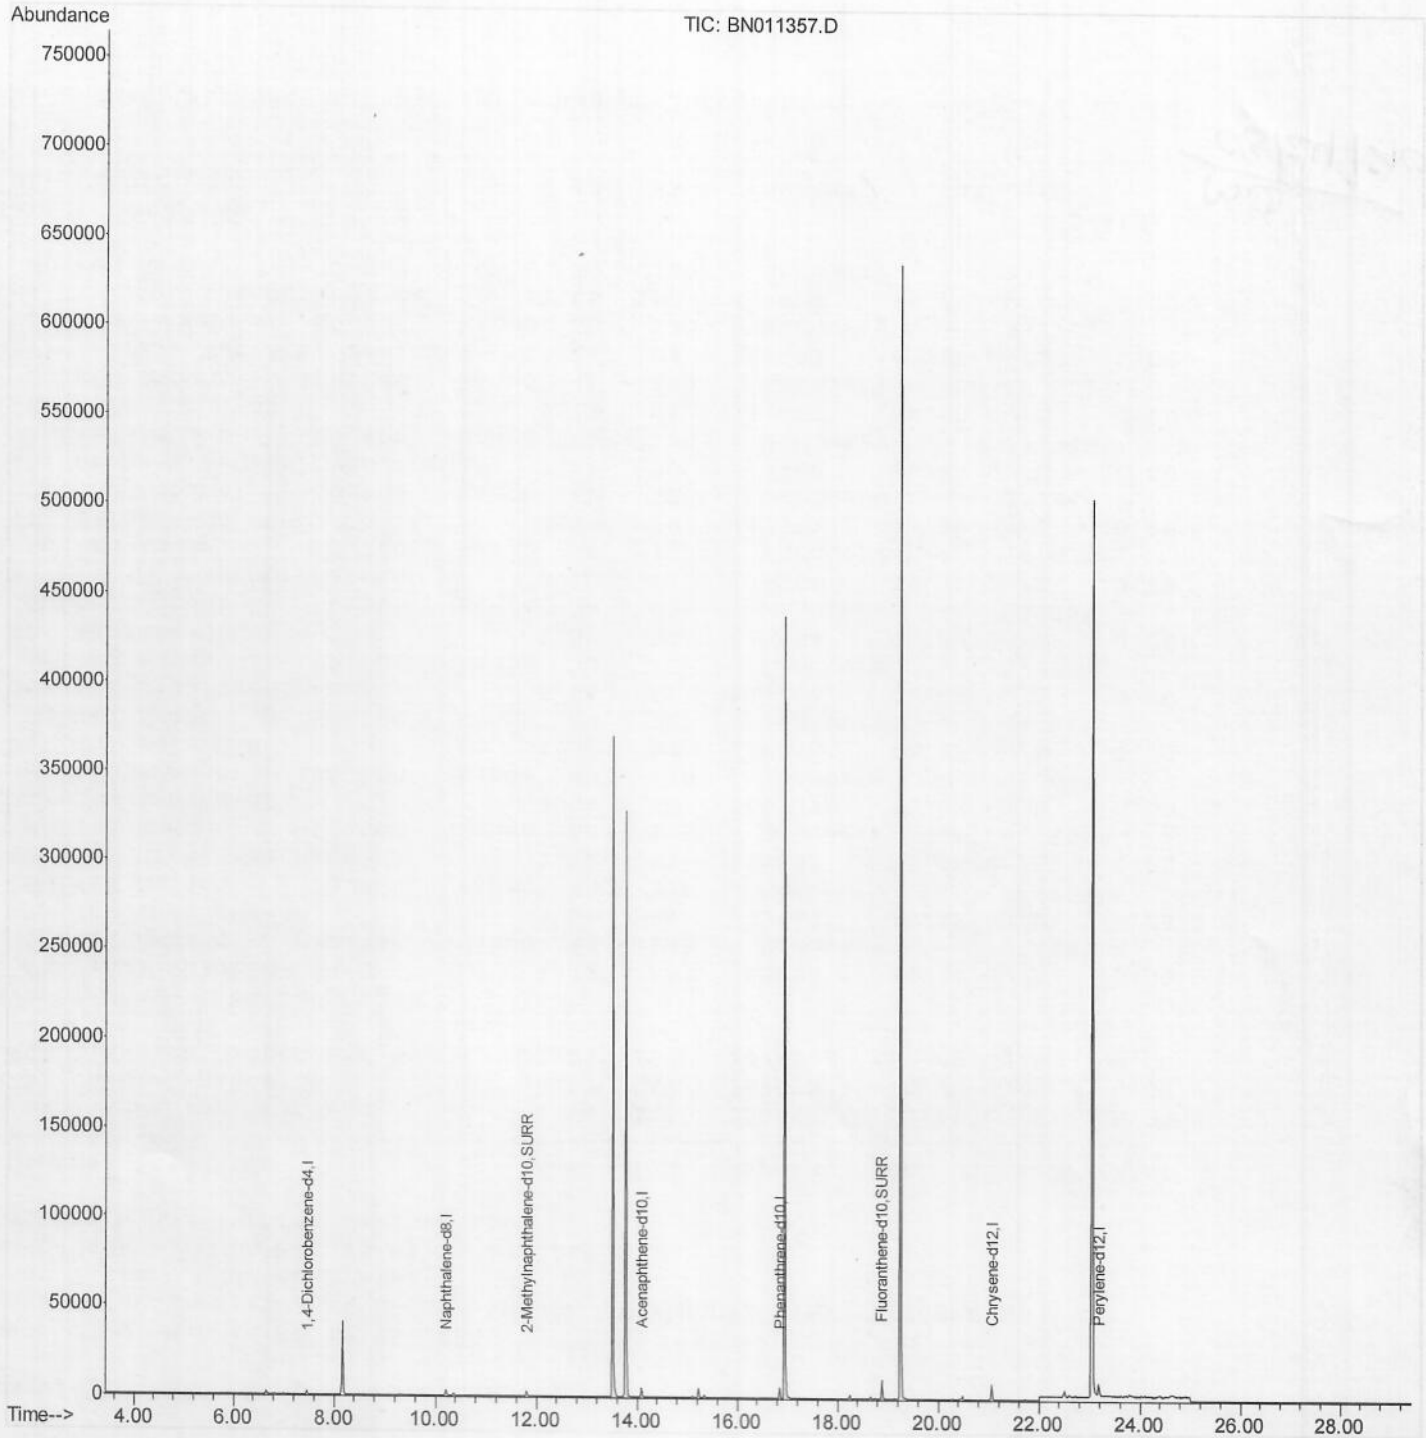

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011357.D
 Acq On : 04 Aug 2020 08:56
 Operator : CG/JU
 Sample : L3443-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA7

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:27 AM

Quant Time: Aug 04 11:48:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

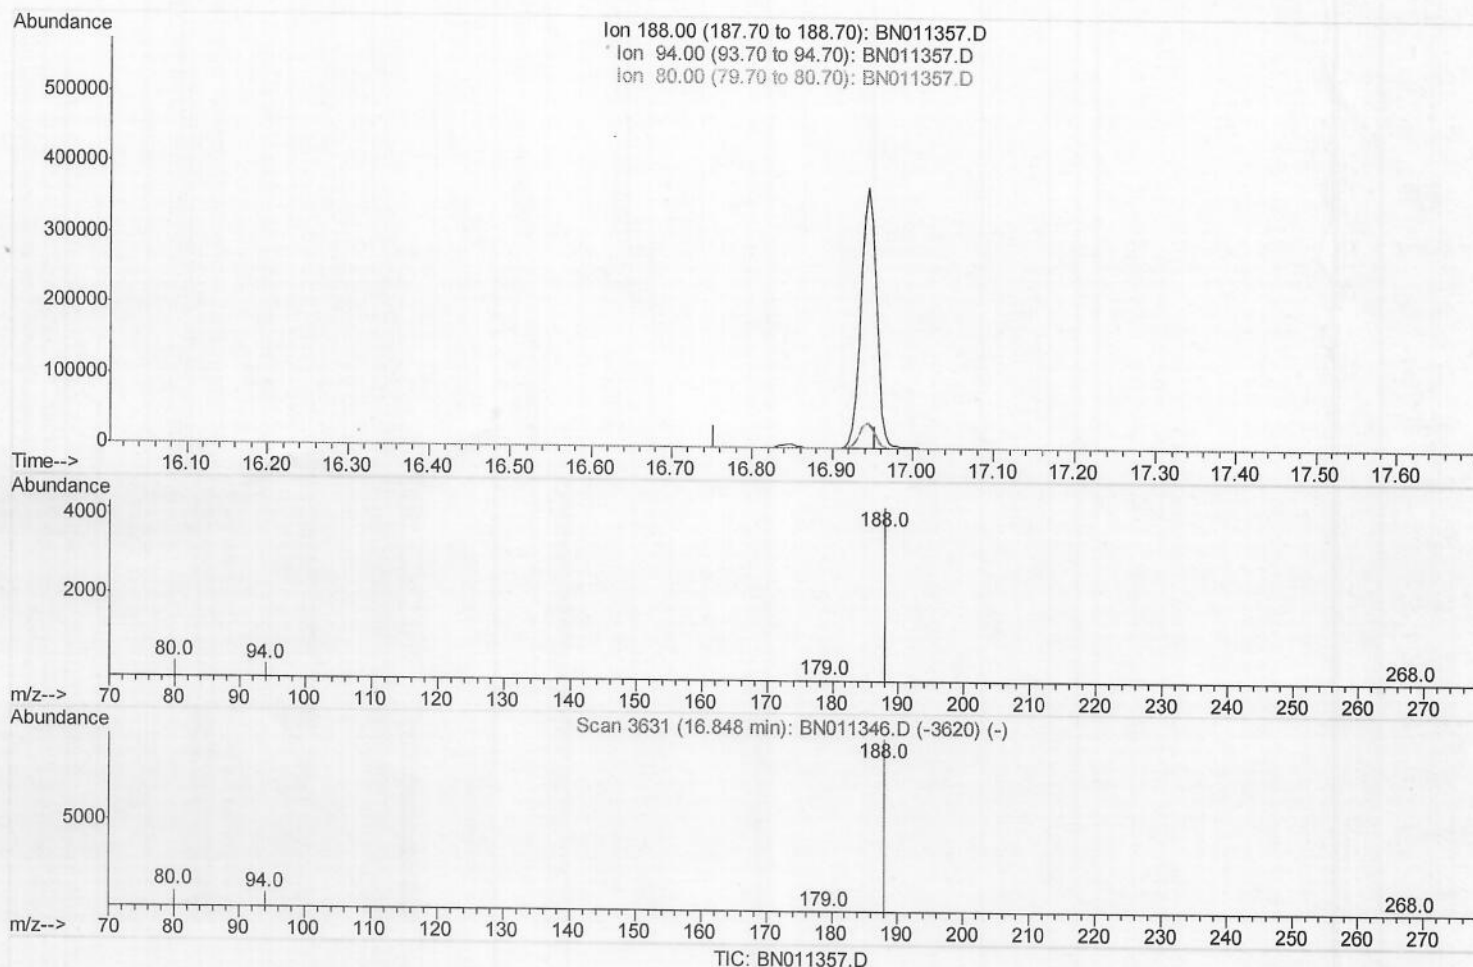

(10) Phenanthrene-d10 (I)

16.853min (-16.853) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011357.D
 Acq On : 04 Aug 2020 08:56
 Operator : CG/JU
 Sample : L3443-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA7

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:27 AM

Quant Time: Aug 04 11:48:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

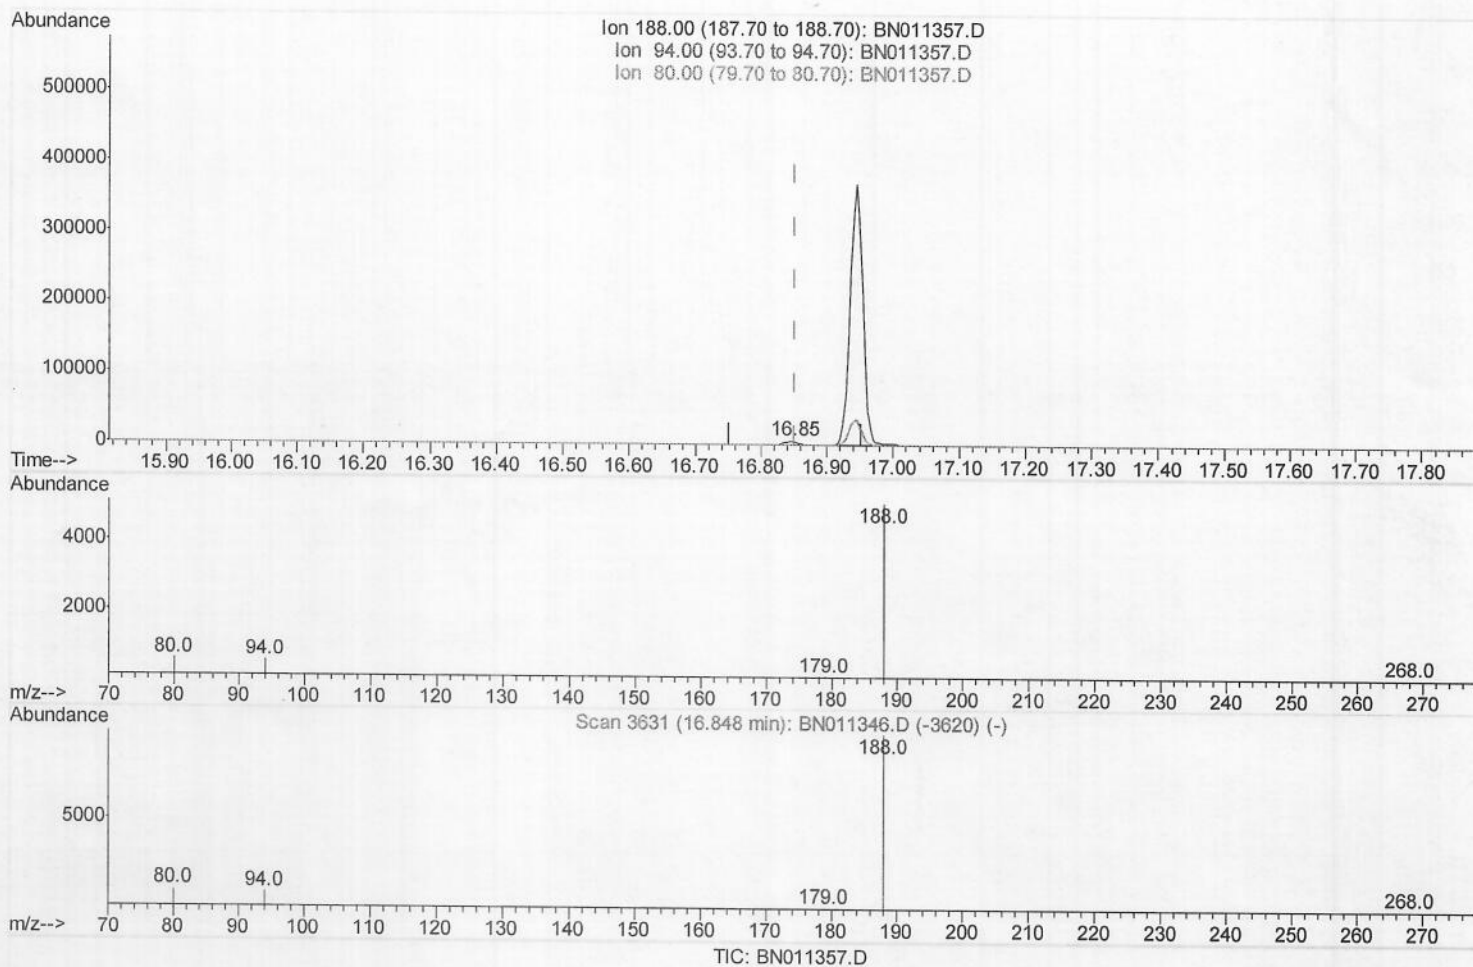

(10) Phenanthrene-d10 (I)

16.848min (-0.004) 0.40ng/ul m

response 7345

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	9.41
80.00	10.30	10.30
0.00	0.00	0.00

2 JU 08/05/20

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011357.D
 Acq On : 04 Aug 2020 08:56
 Operator : CG/JU
 Sample : L3443-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA7

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:27 AM

Quant Time: Aug 04 11:48:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1273	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	4861	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.09	164	3038	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	7345m	0.40	ng/ul	0.00
16) Chrysene-d12	21.06	240	7746	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	8666	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.80	152	3631	0.30	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	11497	0.32	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

3 JU
 08/05/20