

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 12:00:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

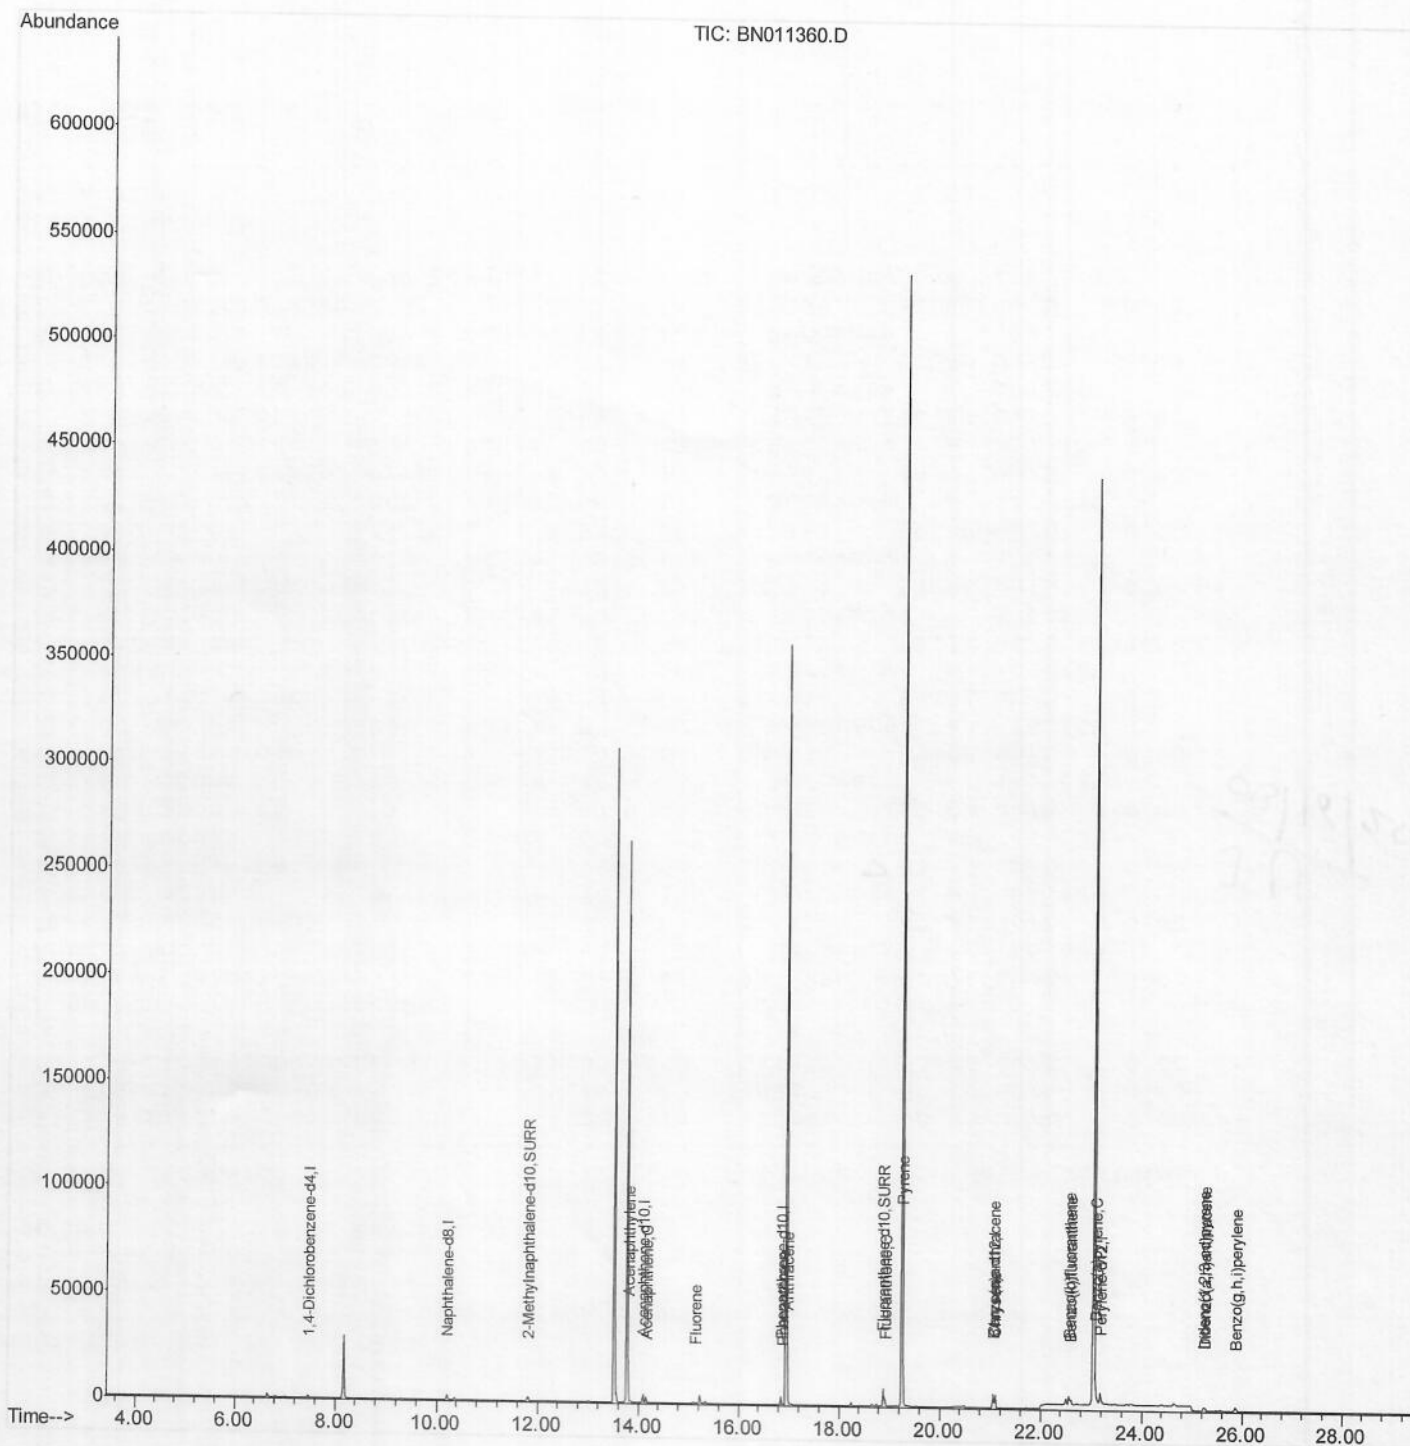

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:57:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

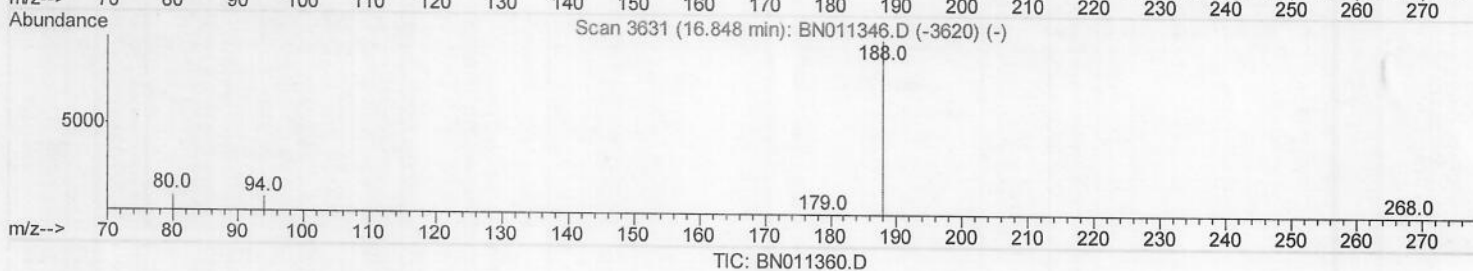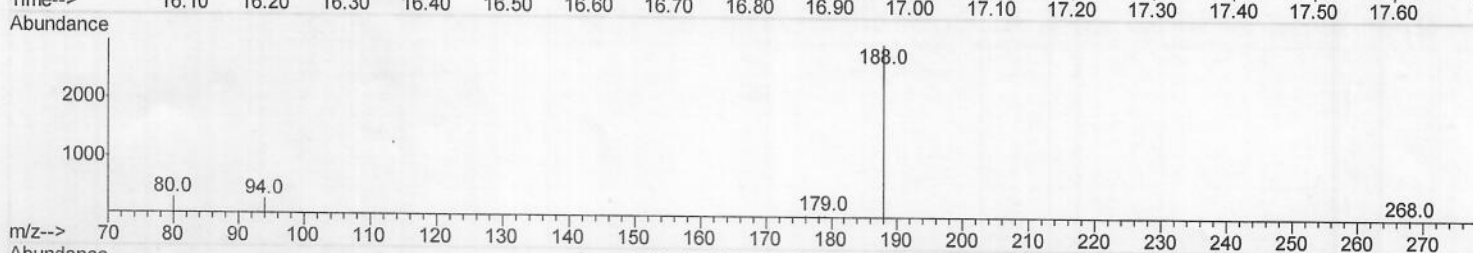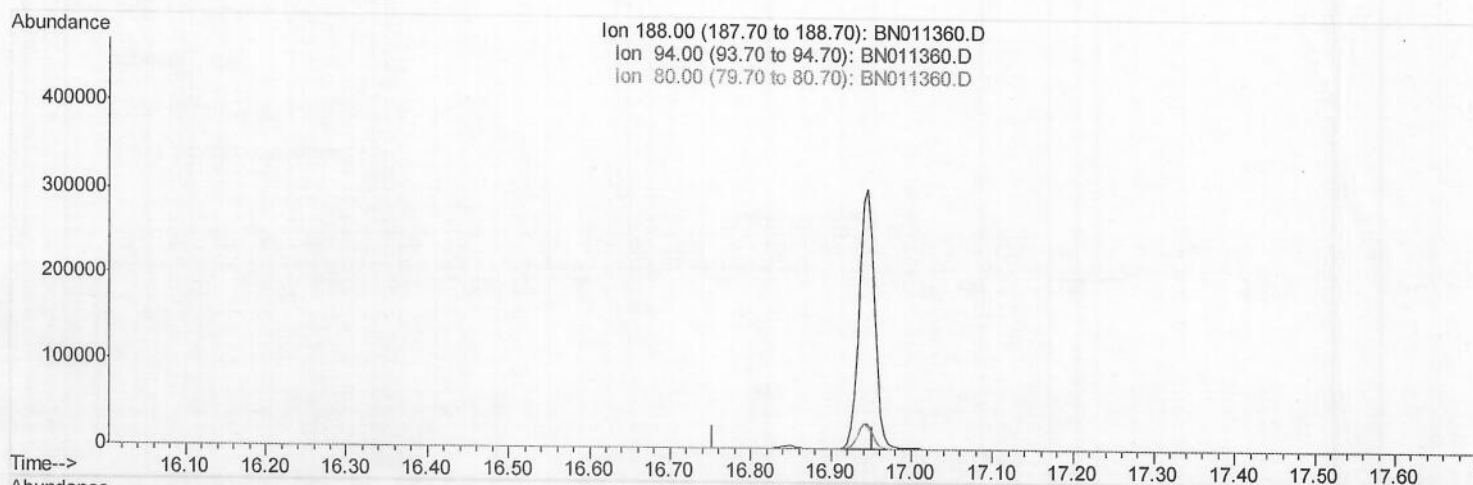

(10) Phenanthrene-d10 (I)

16.853min (-16.853) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:57:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

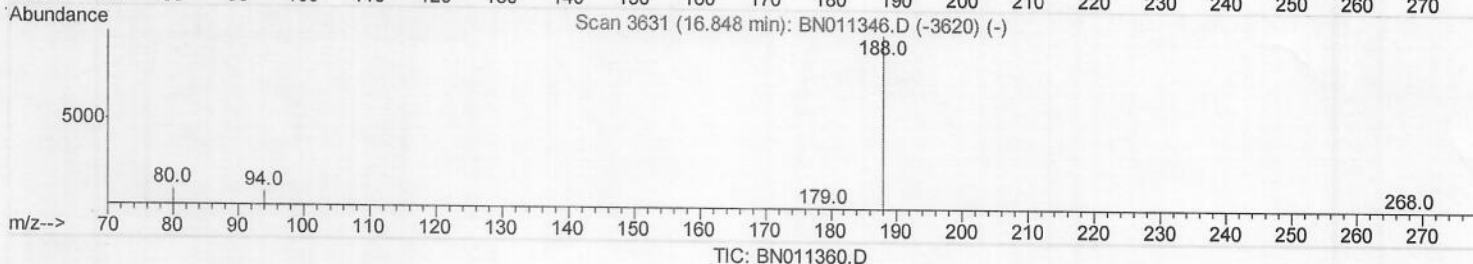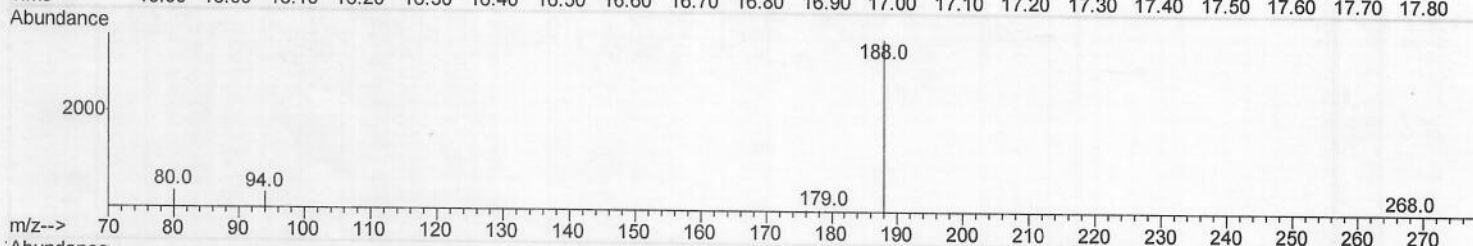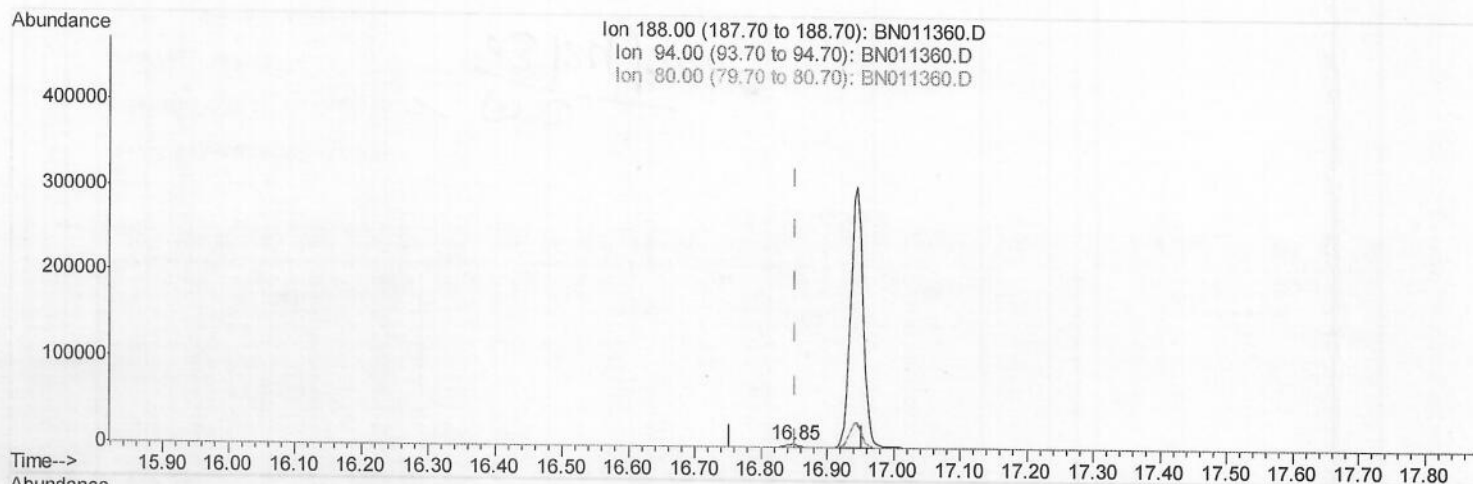

(10) Phenanthrene-d10 (I)

16.848min (-0.004) 0.40ng/ul m

JU 08/05/20

response 5022

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	9.80
80.00	10.30	10.90
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

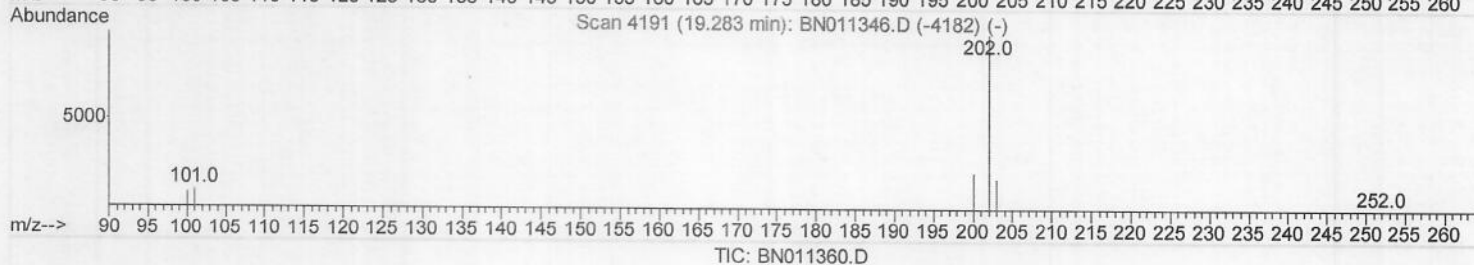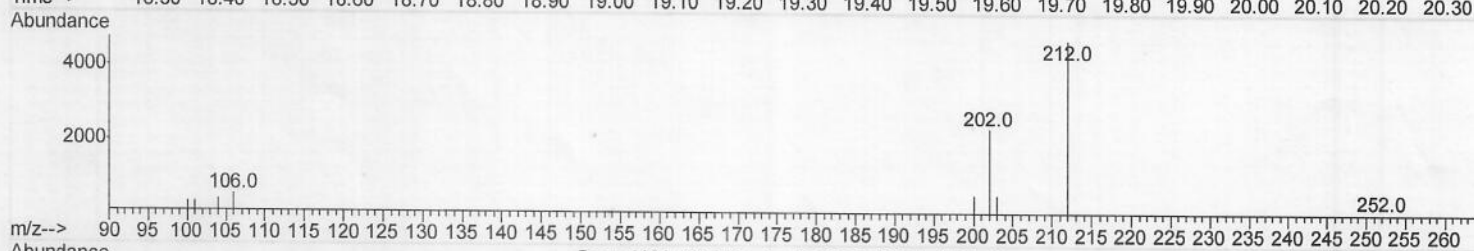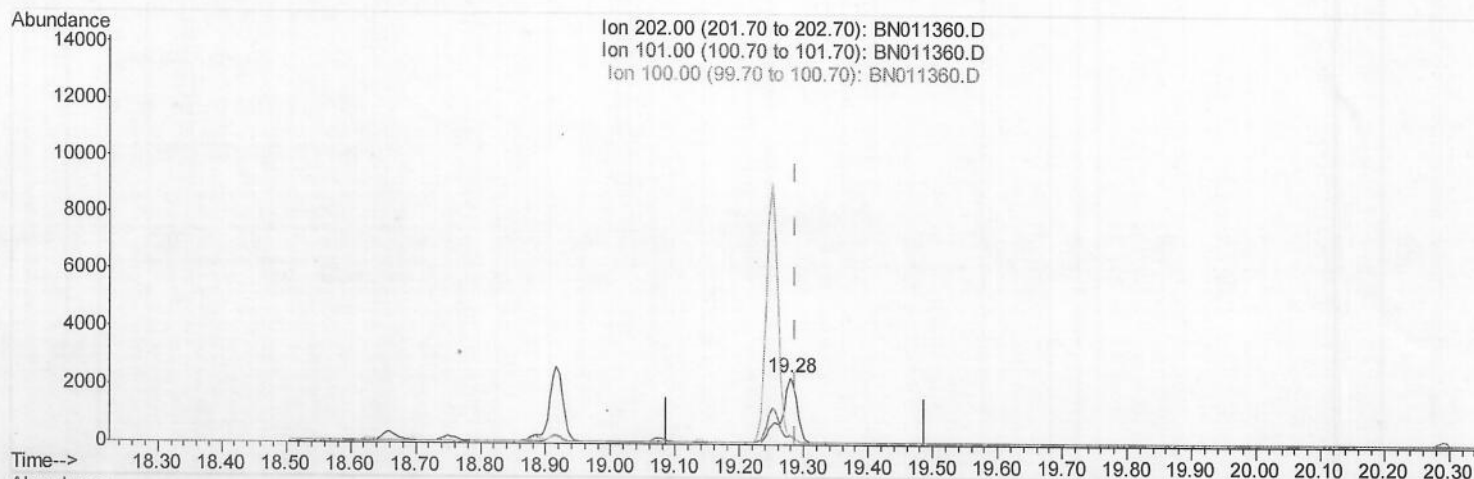

(17) Pyrene

19.279min (-0.009) 0.16ng/ul

response 3869

Ion	Exp%	Act%
202.00	100	100
101.00	10.60	13.56#
100.00	8.90	13.90#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

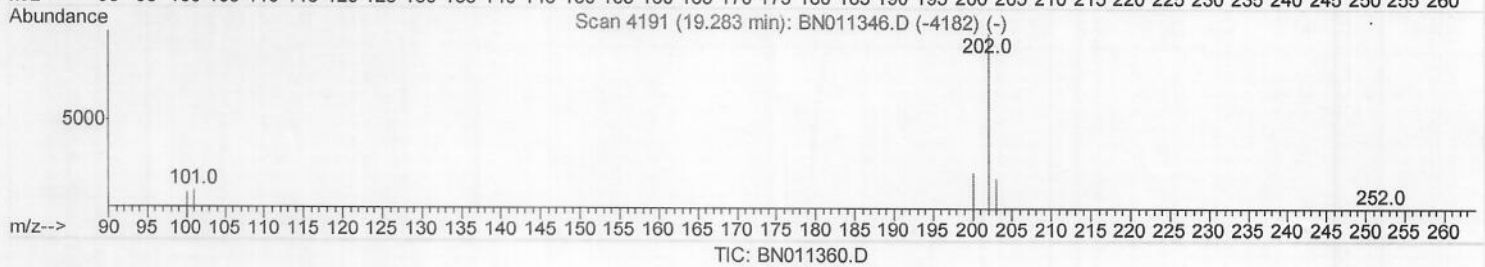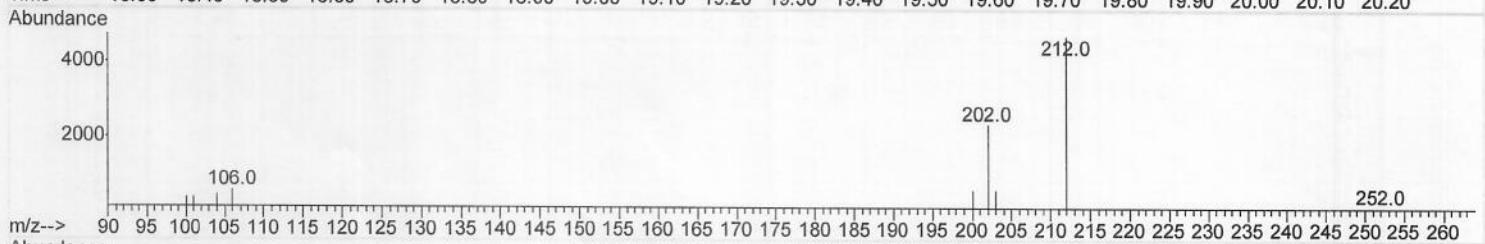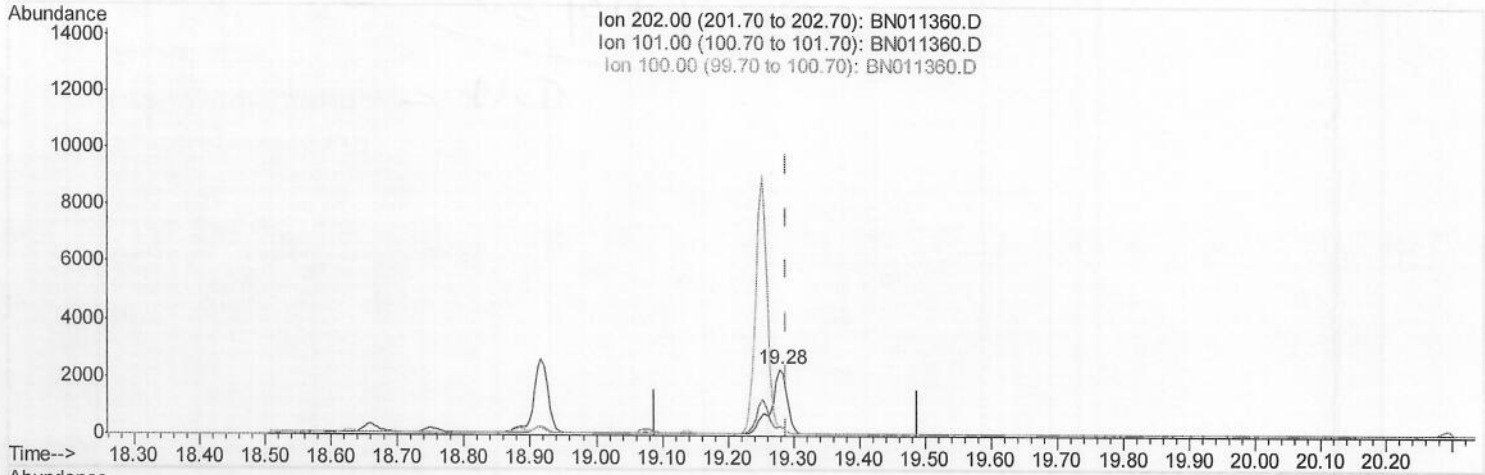

(17) Pyrene

19.279min (-0.009) 0.12ng/ul m

Handwritten: JU 08/05/20

response 3097

Ion	Exp%	Act%
202.00	100	100
101.00	10.60	13.56#
100.00	8.90	13.90#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

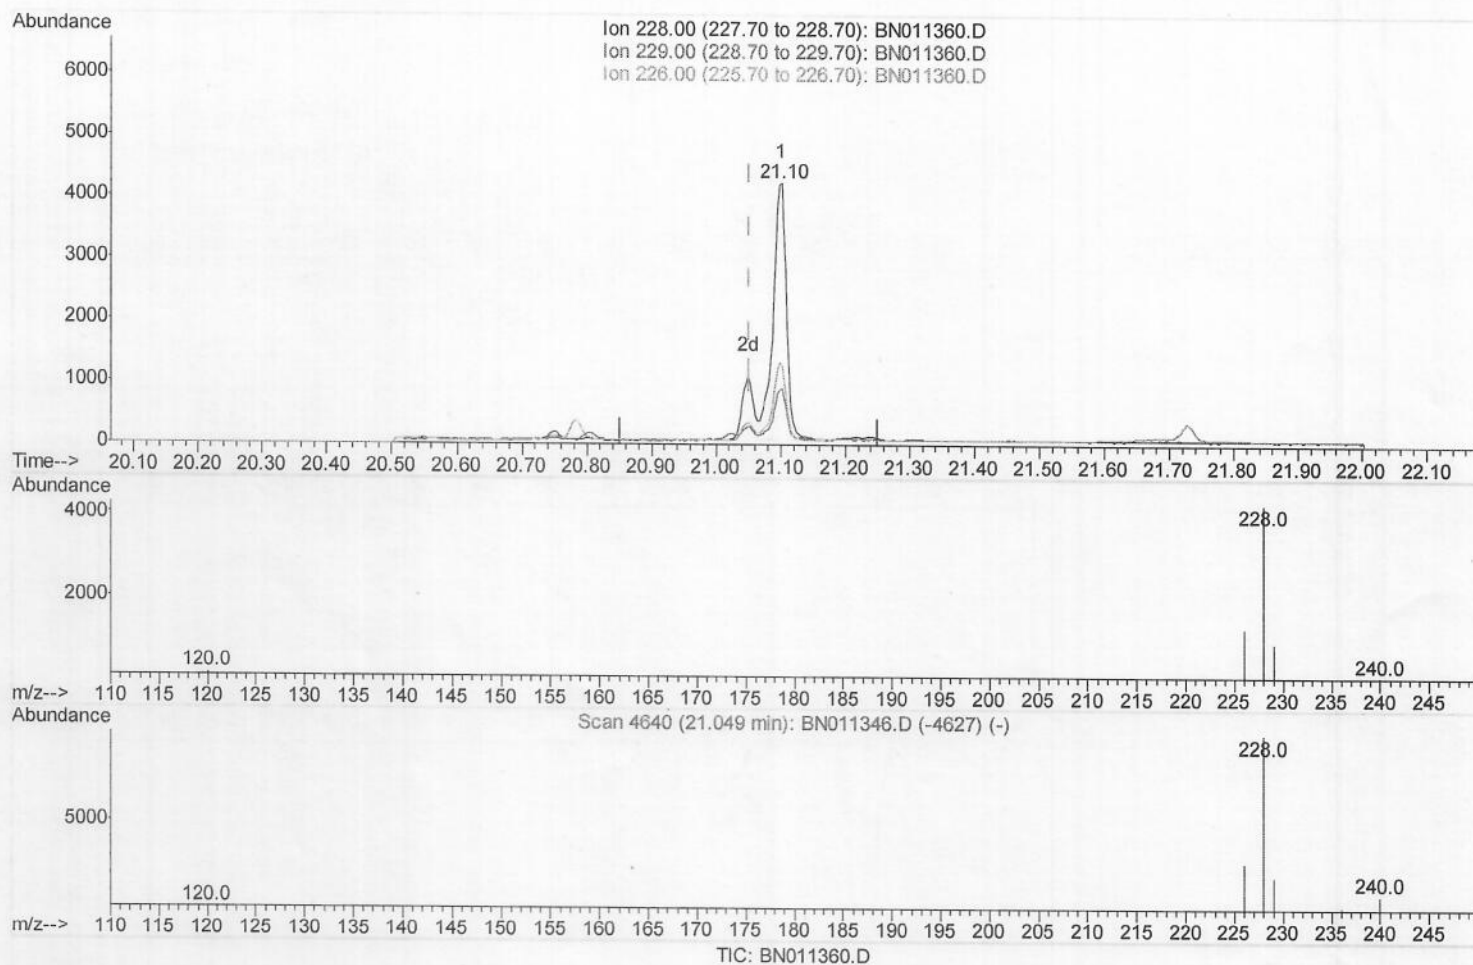

(18) Benzo(a)anthracene
 21.102min (+0.050) 0.28ng/ul
 response 5978

Ion	Exp%	Act%
228.00	100	100
229.00	20.10	21.57
226.00	27.70	30.49
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
Data File : BN011360.D
Acq On : 04 Aug 2020 10:43
Operator : CG/JU
Sample : L3443-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

mohammad
8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 03 10:06:56 2020
Response via : Initial Calibration

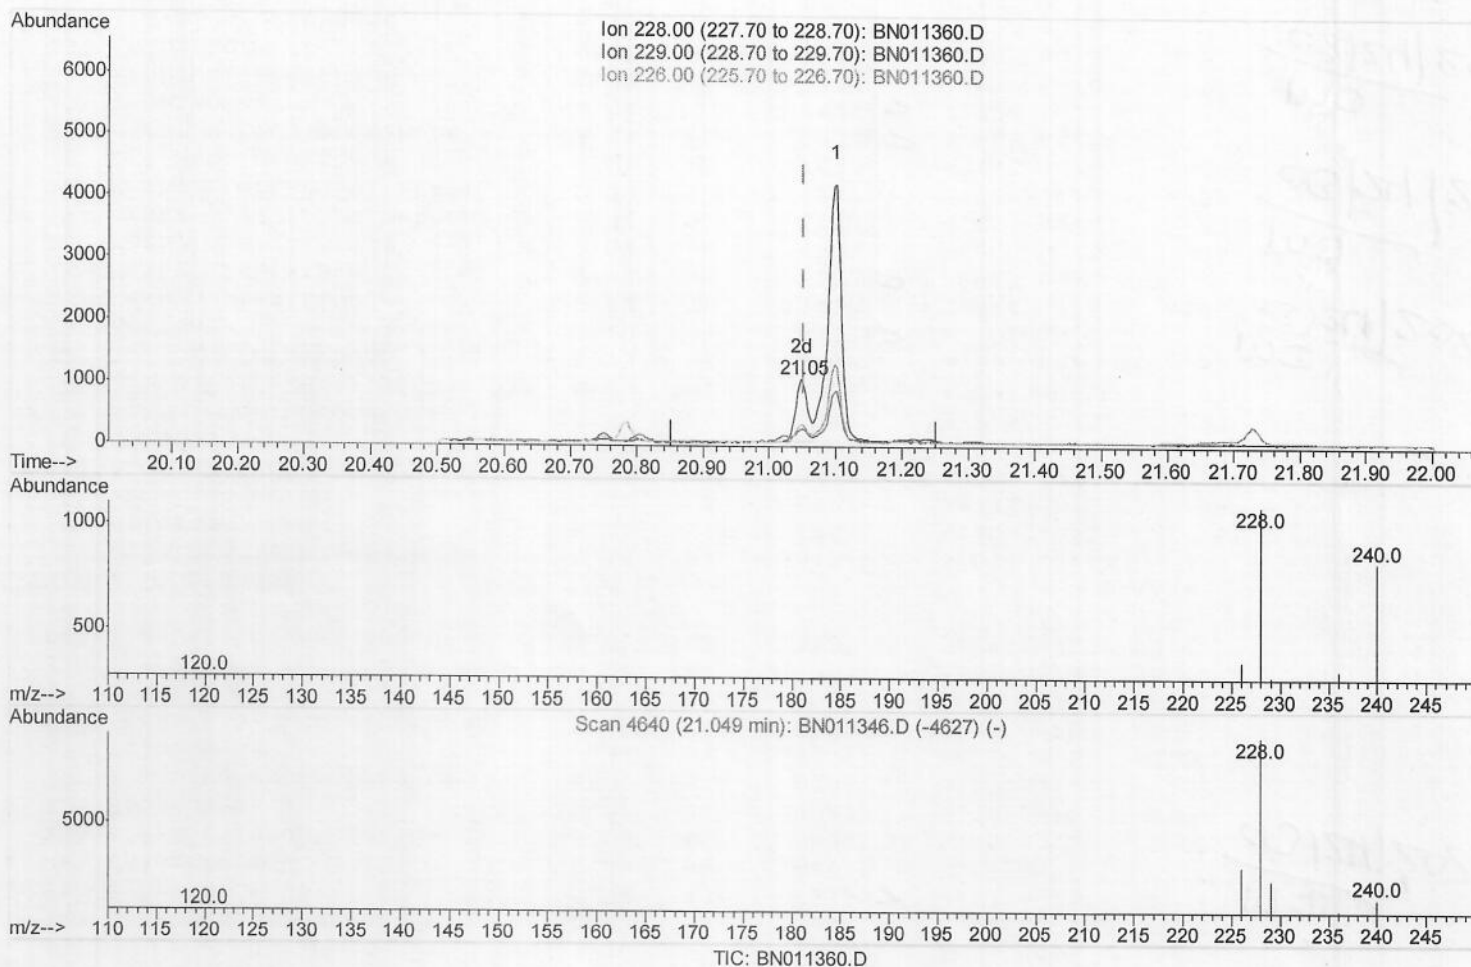

(18) Benzo(a)anthracene

21.049min (-0.003) 0.06ng/ul m

response 1328

Ion	Exp%	Act%
228.00	100	100
229.00	20.10	25.96#
226.00	27.70	32.72
0.00	0.00	0.00

S JU 08/05/20

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

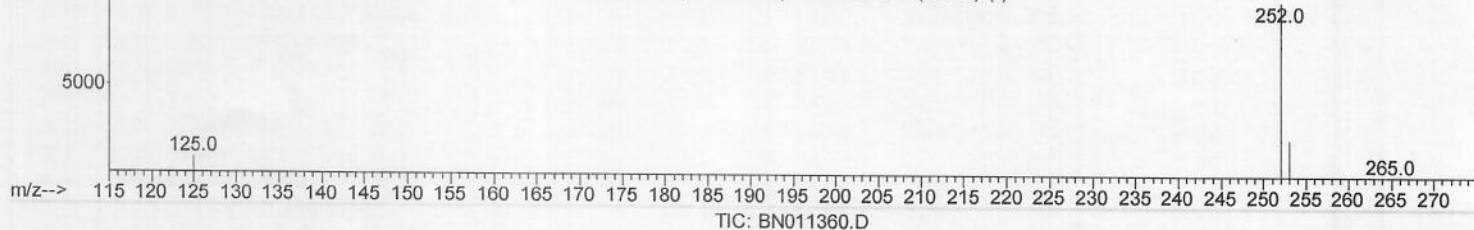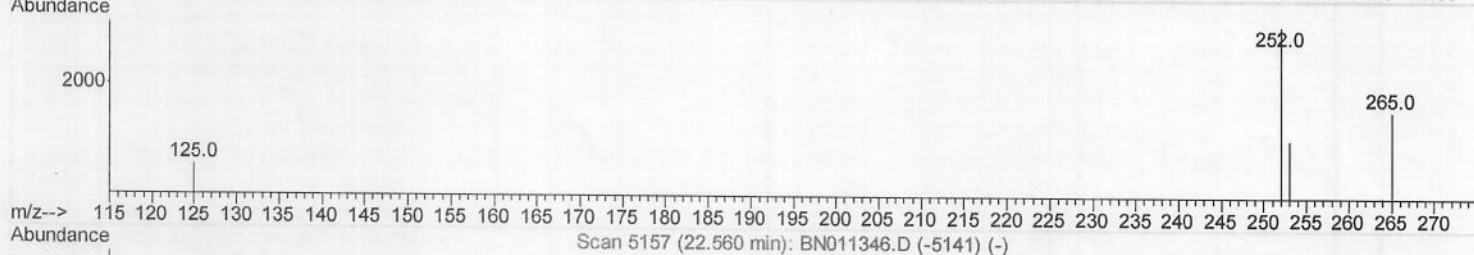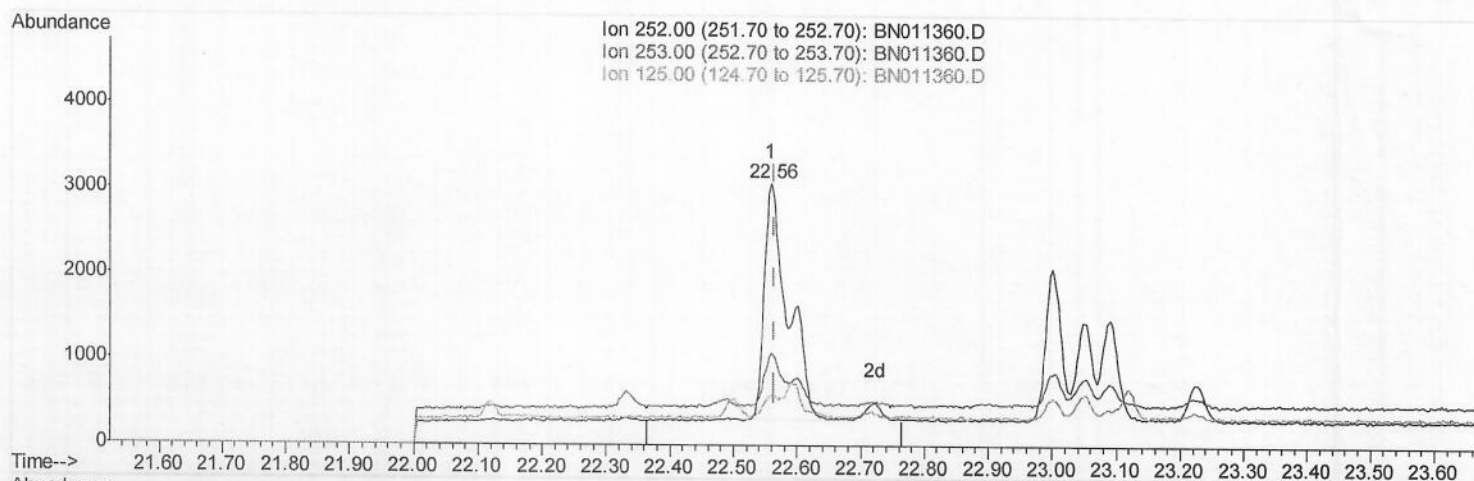

(21) Benzo(b)fluoranthene
 22.560min (-0.006) 0.27ng/ul
 response 7312

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	35.27
125.00	12.10	19.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

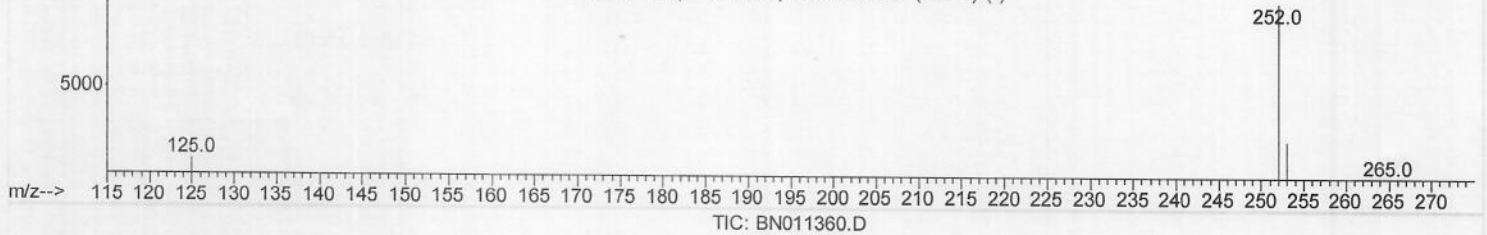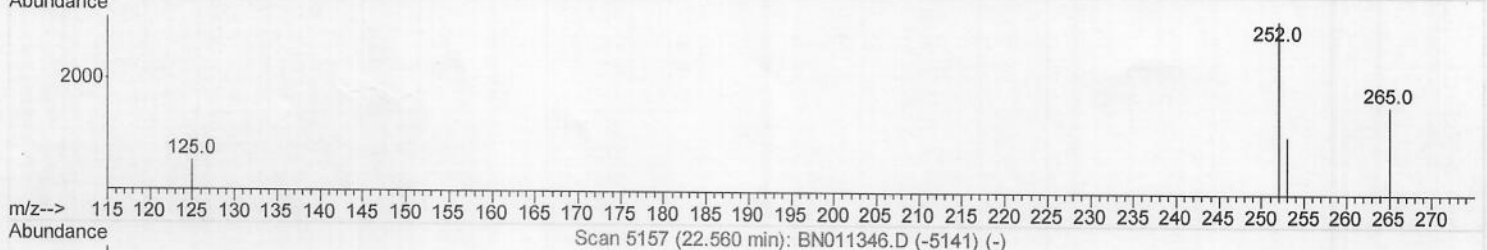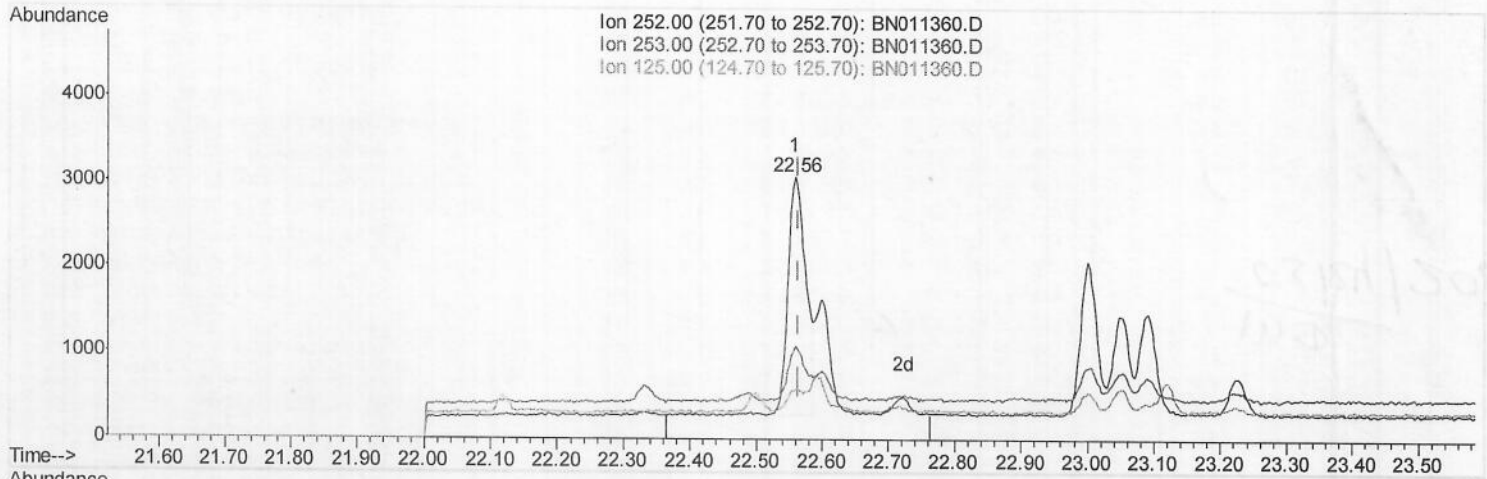

(21) Benzo(b)fluoranthene

22.560min (-0.006) 0.19ng/ul m

response 5214

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	35.27
125.00	12.10	19.23
0.00	0.00	0.00

2 JU 08/05/20

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

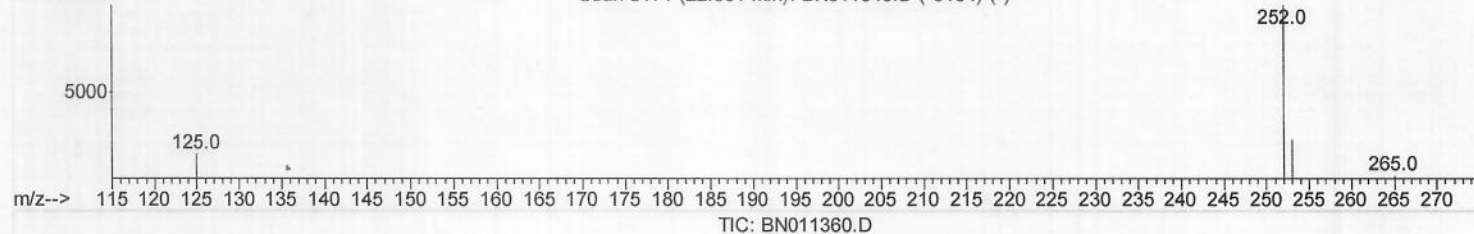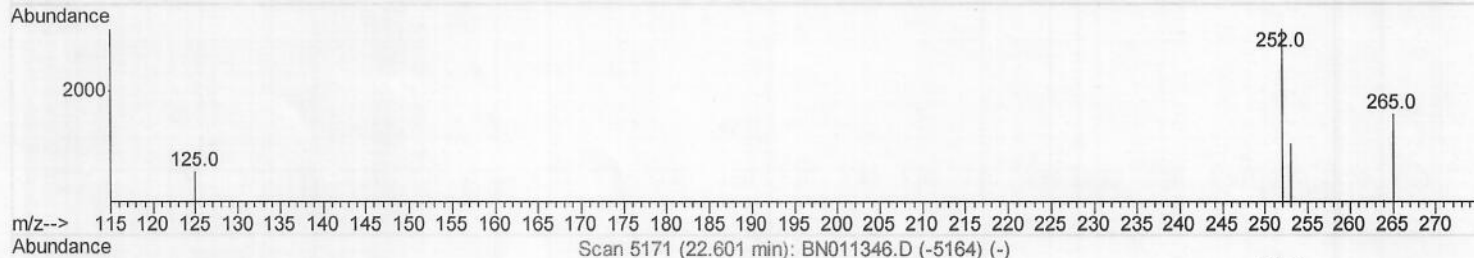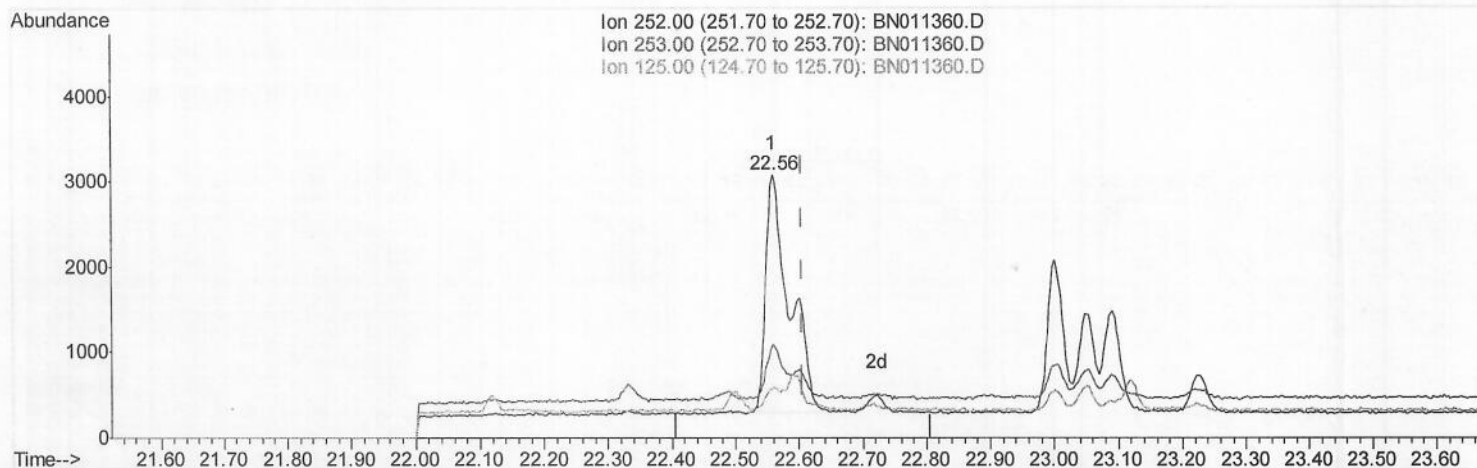

(22) Benzo(k)fluoranthene
 22.560min (-0.047) 0.24ng/ul
 response 7312

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	35.27#
125.00	15.70	19.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 11:58:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

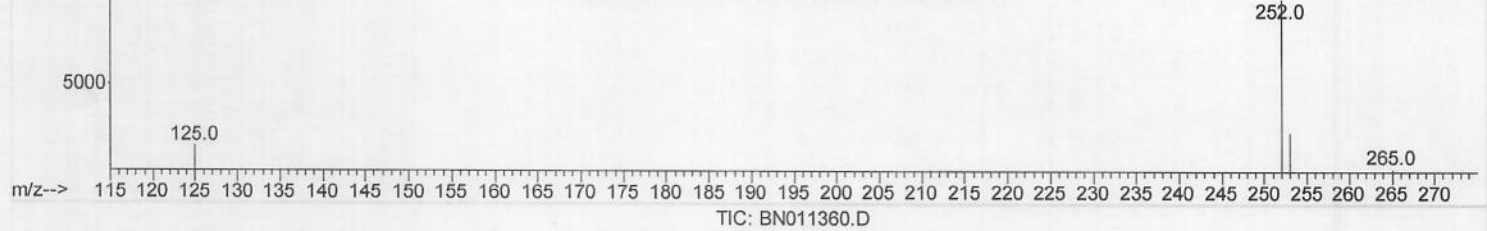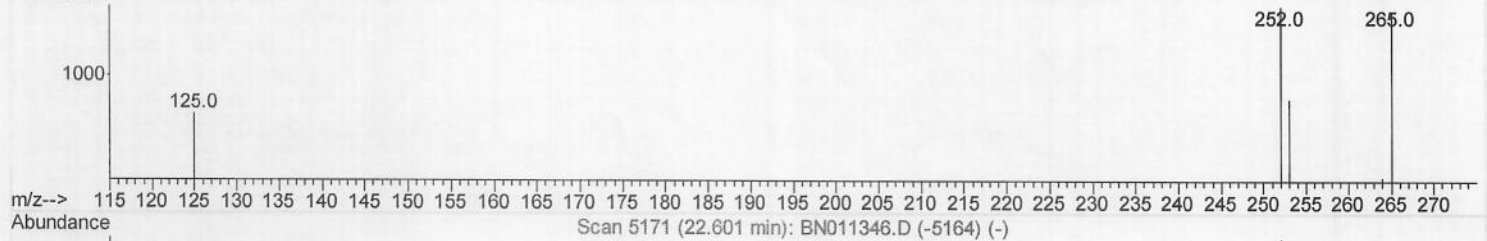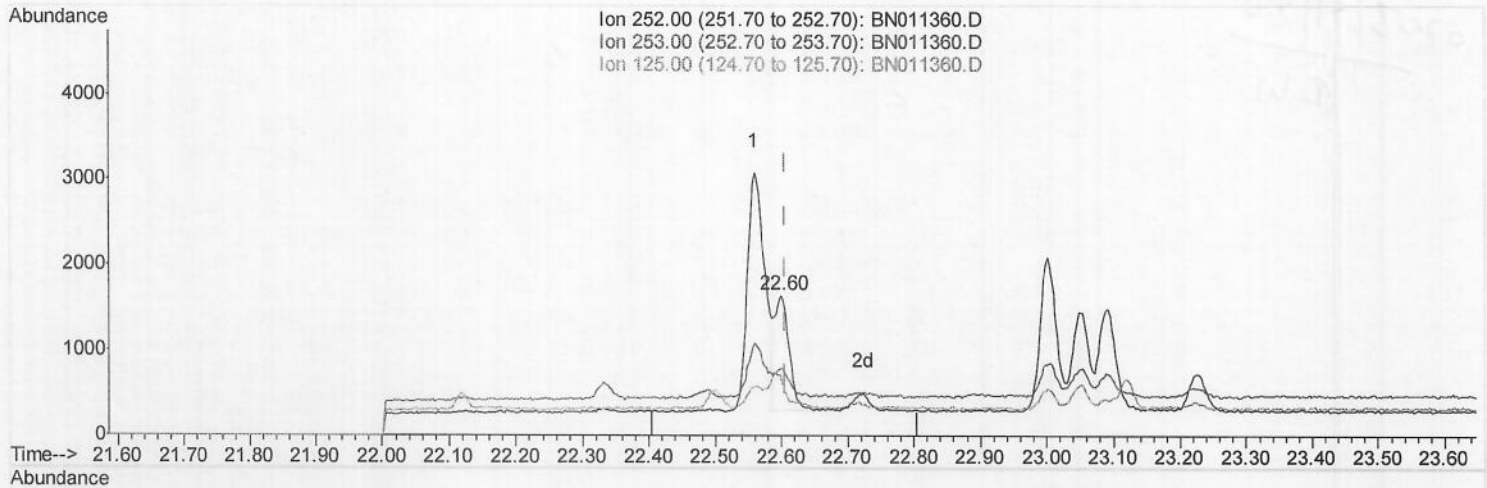

(22) Benzo(k)fluoranthene

22.600min (-0.006) 0.07ng/ul m

response 2070

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	48.74#
125.00	15.70	39.74#
0.00	0.00	0.00

> JU 08/05/20

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011360.D
 Acq On : 04 Aug 2020 10:43
 Operator : CG/JU
 Sample : L3443-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:30 AM

Quant Time: Aug 04 12:00:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	804	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	3158	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.09	164	2053	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	5022m	0.40	ng/ul	0.00
16) Chrysene-d12	21.06	240	5472	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	6532	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	2724	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	8895	0.37	ng/ul	0.00
Target Compounds						
					Ovalue	
7) Acenaphthylene	13.81	152	275	0.028	ng/ul#	59
8) Acenaphthene	14.15	153	1523	0.195	ng/ul	99
9) Fluorene	15.15	166	360	0.039	ng/ul#	93
12) Phenanthrene	16.89	178	676	0.041	ng/ul#	76
13) Anthracene	16.97	178	736	0.051	ng/ul#	78
15) Fluoranthene	18.92	202	3917	0.191	ng/ul	93
17) Pyrene	19.28	202	3097m	0.125	ng/ul	
18) Benzo(a)anthracene	21.05	228	1328m	0.063	ng/ul	
19) Chrysene	21.10	228	5978	0.248	ng/ul	98
21) Benzo(b)fluoranthene	22.56	252	5214m	0.191	ng/ul	
22) Benzo(k)fluoranthene	22.60	252	2070m	0.068	ng/ul	
23) Benzo(a)pyrene	23.09	252	2015	0.085	ng/ul#	65
24) Indeno(1,2,3-cd)pyrene	25.25	276	2984	0.120	ng/ul#	87
25) Dibenzo(a,h)anthracene	25.26	278	702	0.035	ng/ul#	19
26) Benzo(a,h,i)perylene	25.87	276	3197	0.142	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed