


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
Data File : BN011362.D
Acq On : 04 Aug 2020 11:55
Operator : CG/JU
Sample : L3443-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
8/5/2020 10:28:36 AM

Quant Time: Aug 04 13:42:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 03 10:06:56 2020
Response via : Initial Calibration

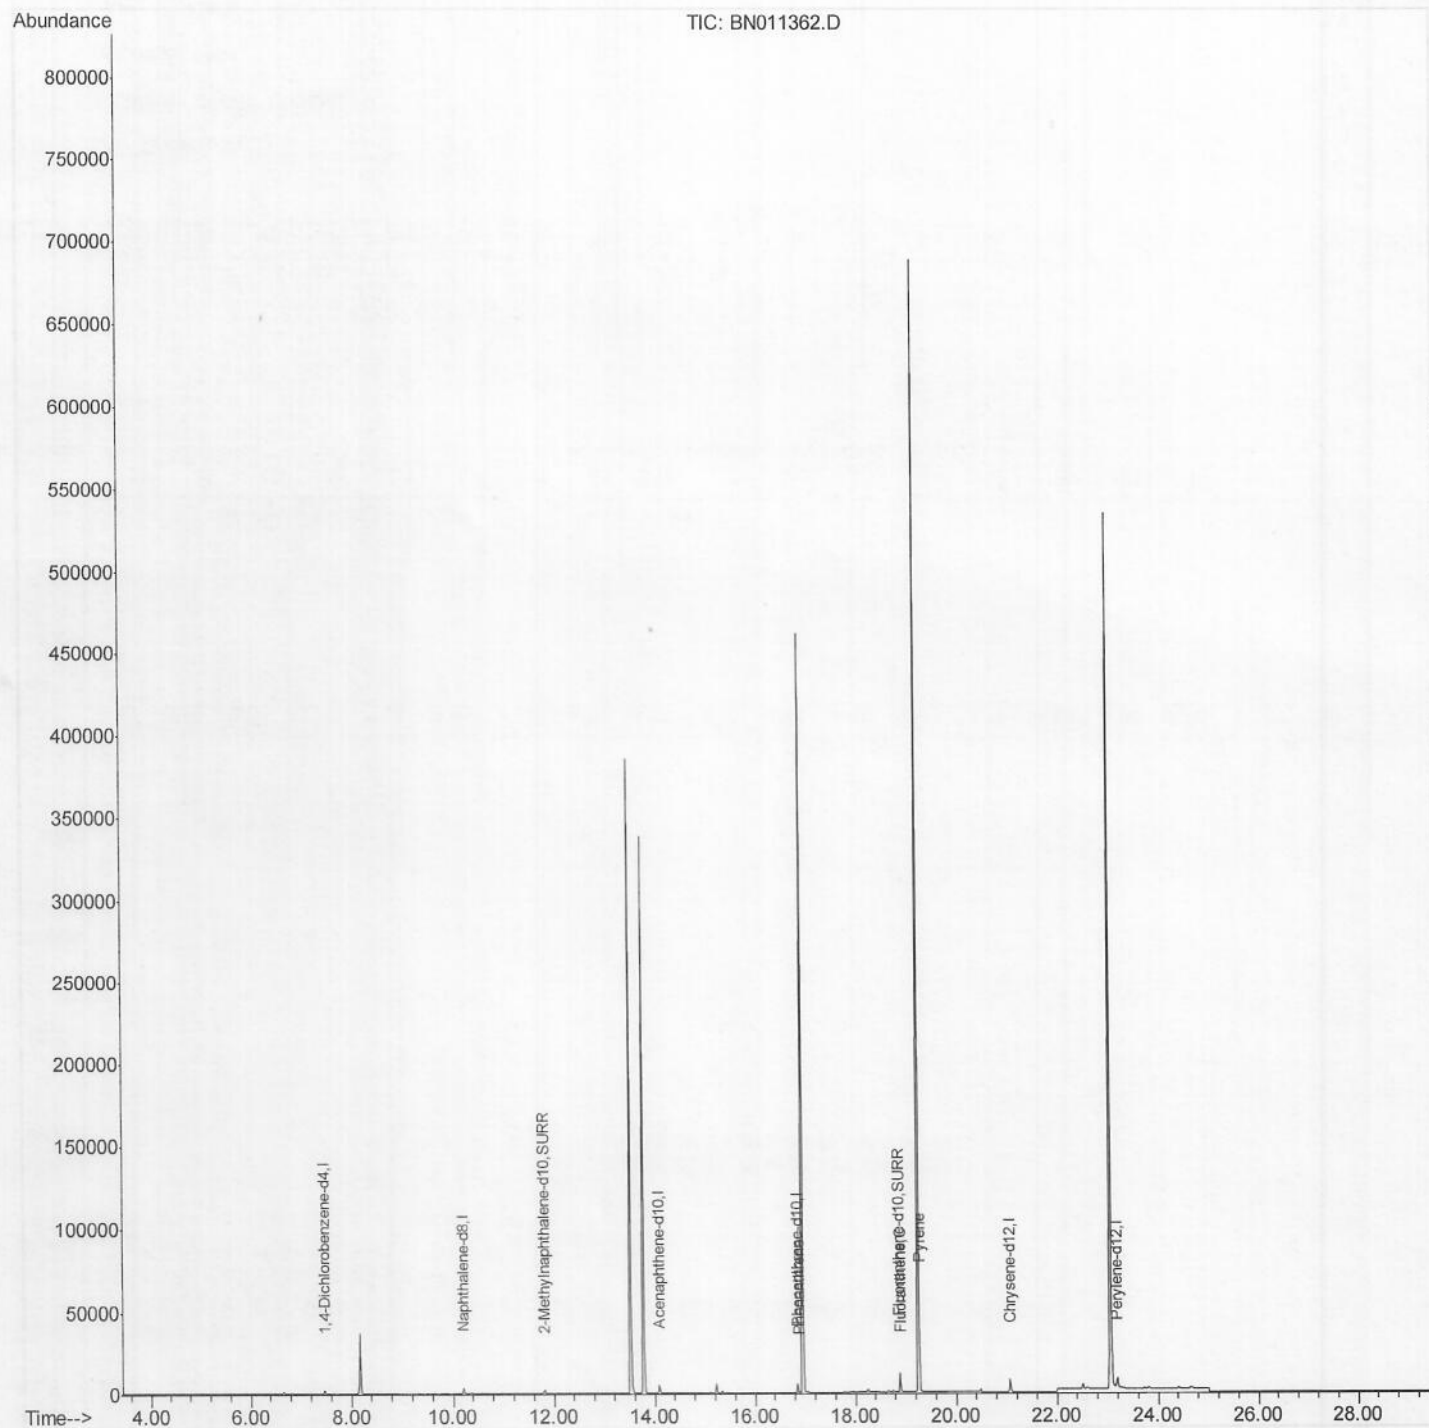

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011362.D
 Acq On : 04 Aug 2020 11:55
 Operator : CG/JU
 Sample : L3443-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:36 AM

Quant Time: Aug 04 13:16:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

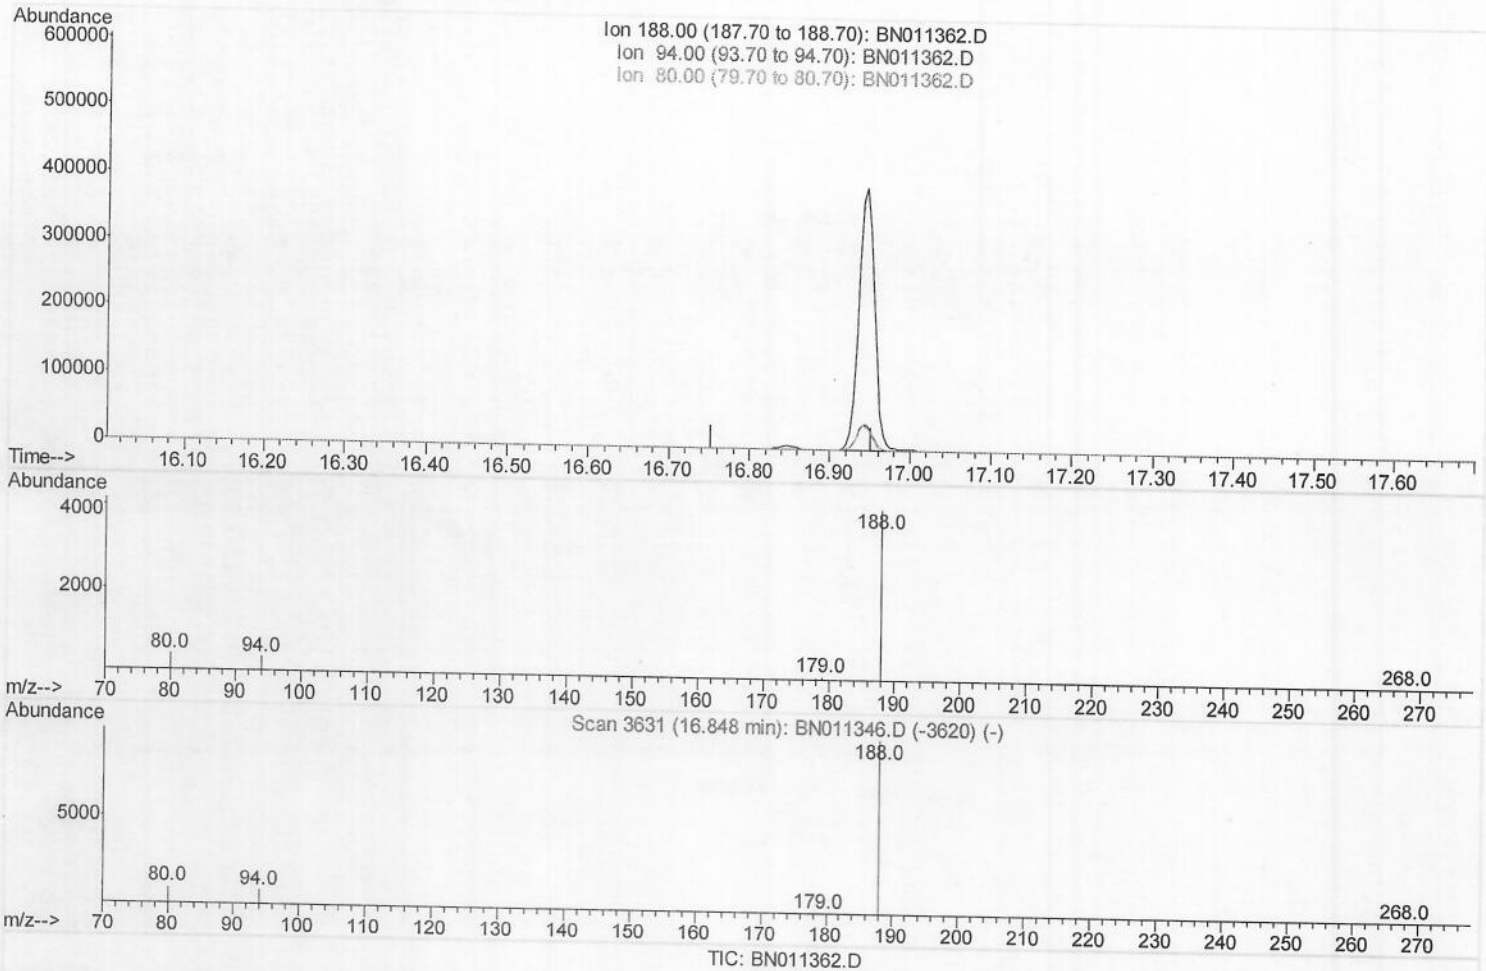

(10) Phenanthrene-d10 (I)

16.853min (-16.853) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011362.D
 Acq On : 04 Aug 2020 11:55
 Operator : CG/JU
 Sample : L3443-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:36 AM

Quant Time: Aug 04 13:16:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

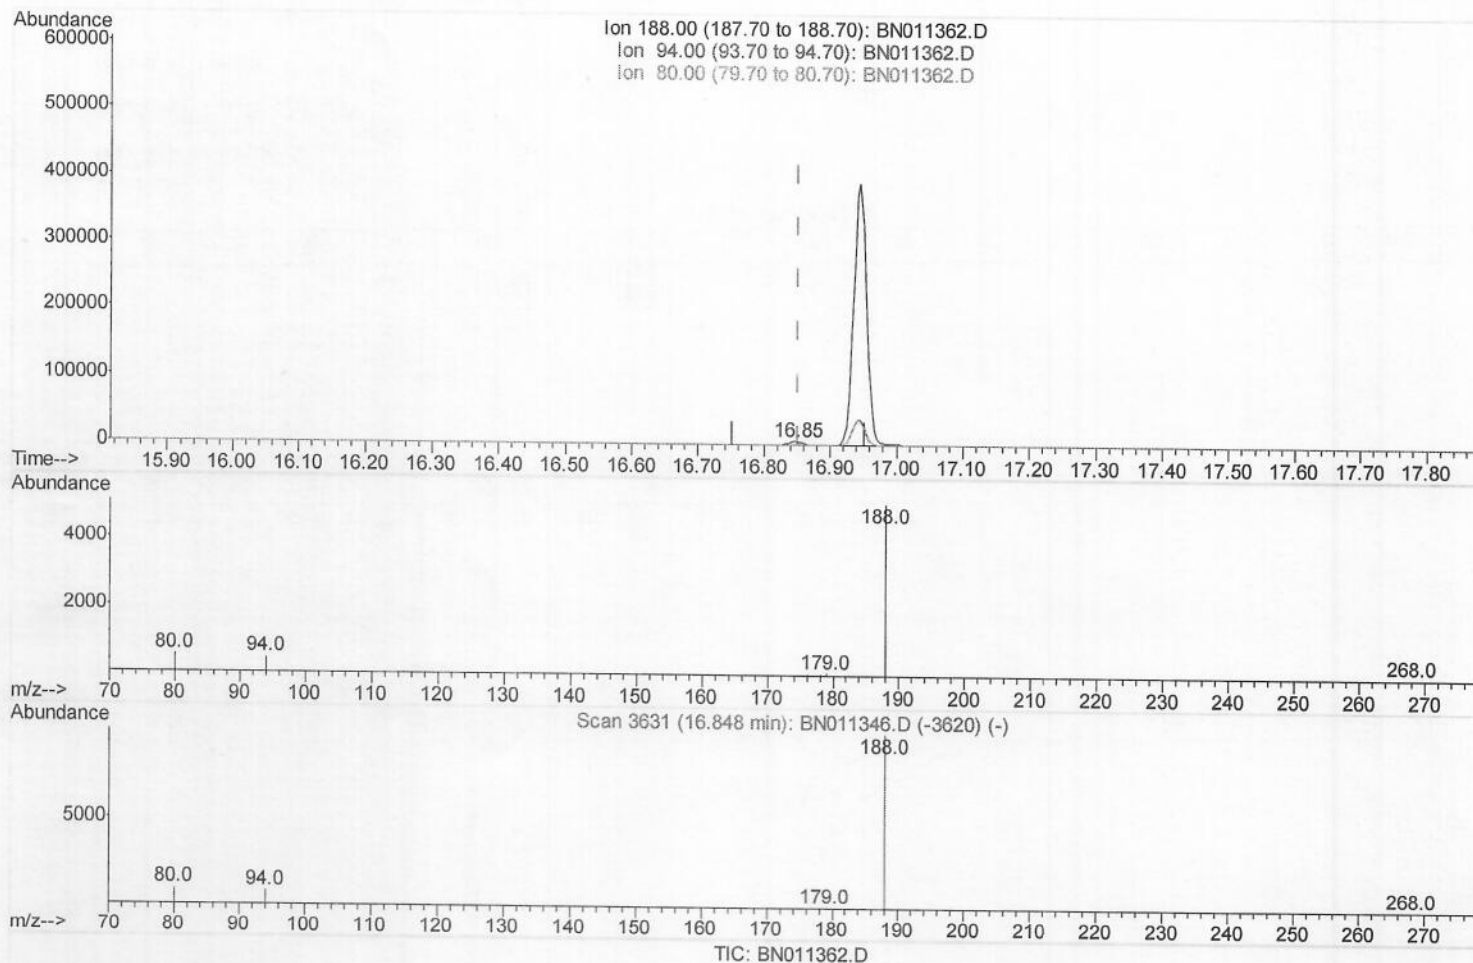

(10) Phenanthrene-d10 (I)

16.848min (-0.004) 0.40ng/ul m

response 7112

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	9.38
80.00	10.30	10.82
0.00	0.00	0.00

JU 08/05/20

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080320\
 Data File : BN011362.D
 Acq On : 04 Aug 2020 11:55
 Operator : CG/JU
 Sample : L3443-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:28:36 AM

Quant Time: Aug 04 13:42:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 03 10:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1222	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	4602	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.09	164	2923	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	7112m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	7580	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	8052	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	3657	0.31	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	11972	0.35	ng/ul	0.00
Target Compounds						
12) Phenanthrene	16.89	178	534	0.023	ng/ul#	64
15) Fluoranthene	18.92	202	1078	0.037	ng/ul	76
17) Pyrene	19.28	202	804	0.023	ng/ul#	65

JU 08/05/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed