
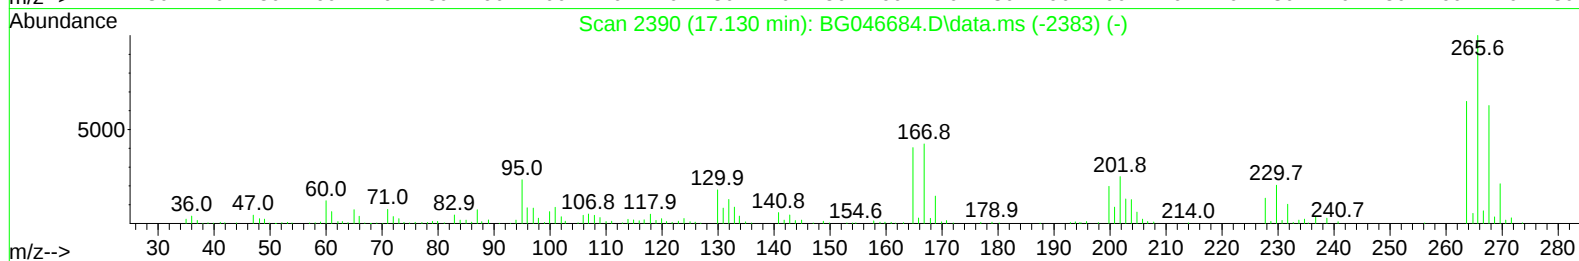
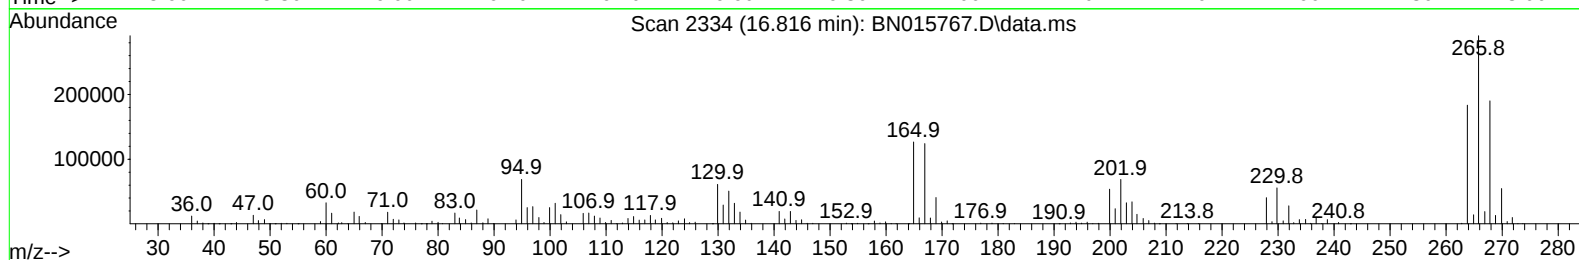


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
 Data File : BN015767.D
 Acq On : 03 Aug 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 15:52:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 04:52:40 2021
 Response via : Initial Calibration

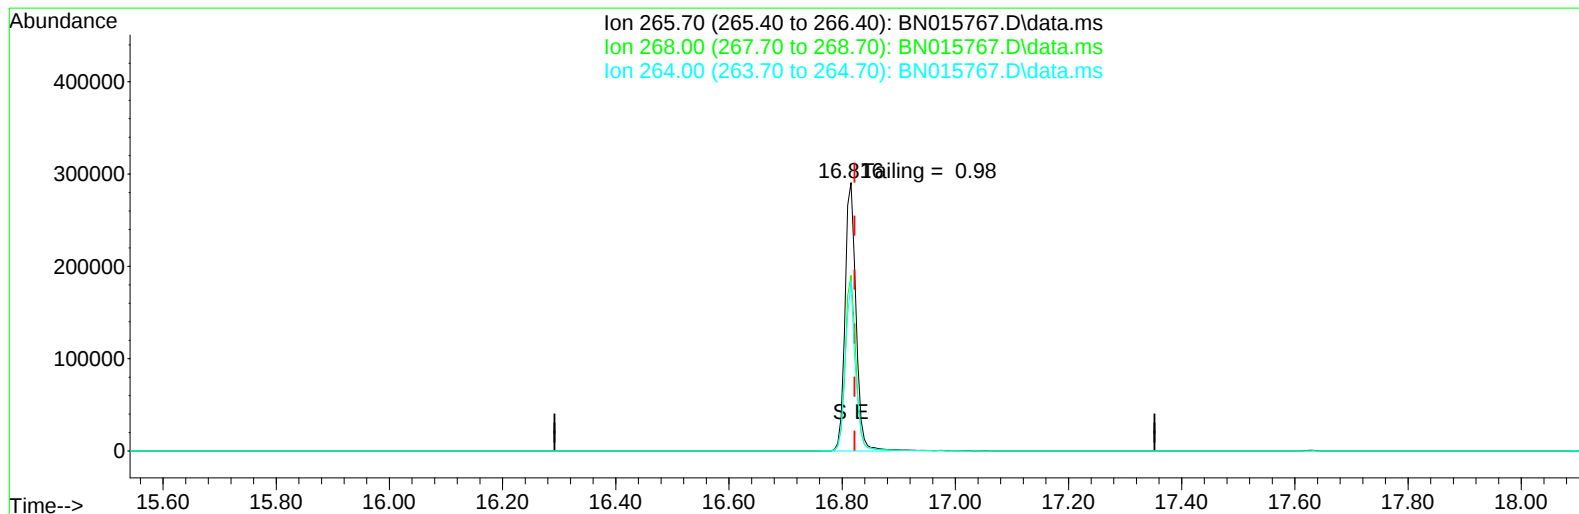

TIC: BN015767.D\data.ms

(70) Pentachlorophenol (C)




16.816min (-0.006) 19965.46 ng

response 391083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.40
264.00	61.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015767.D
Acq On : 03 Aug 2021 12:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 15:52:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 04:52:40 2021
Response via : Initial Calibration

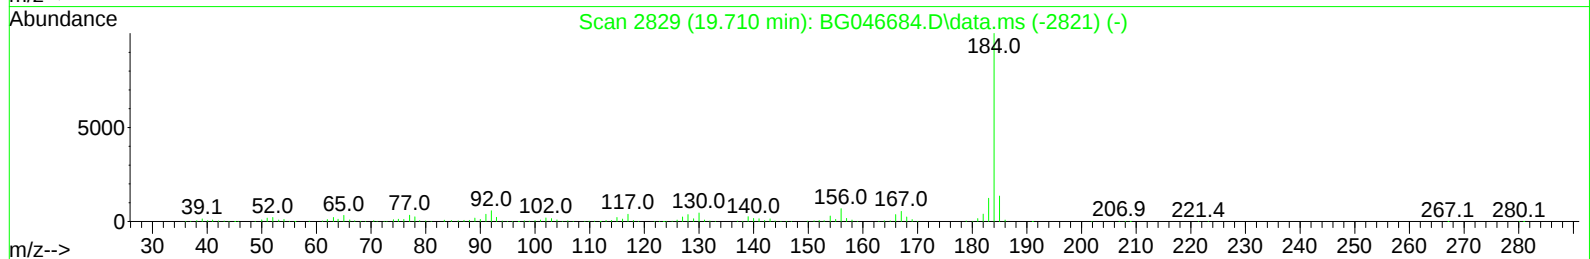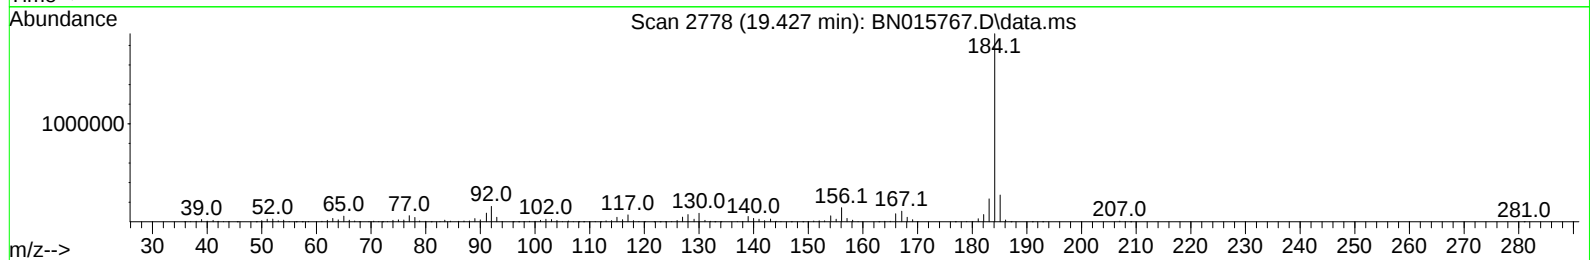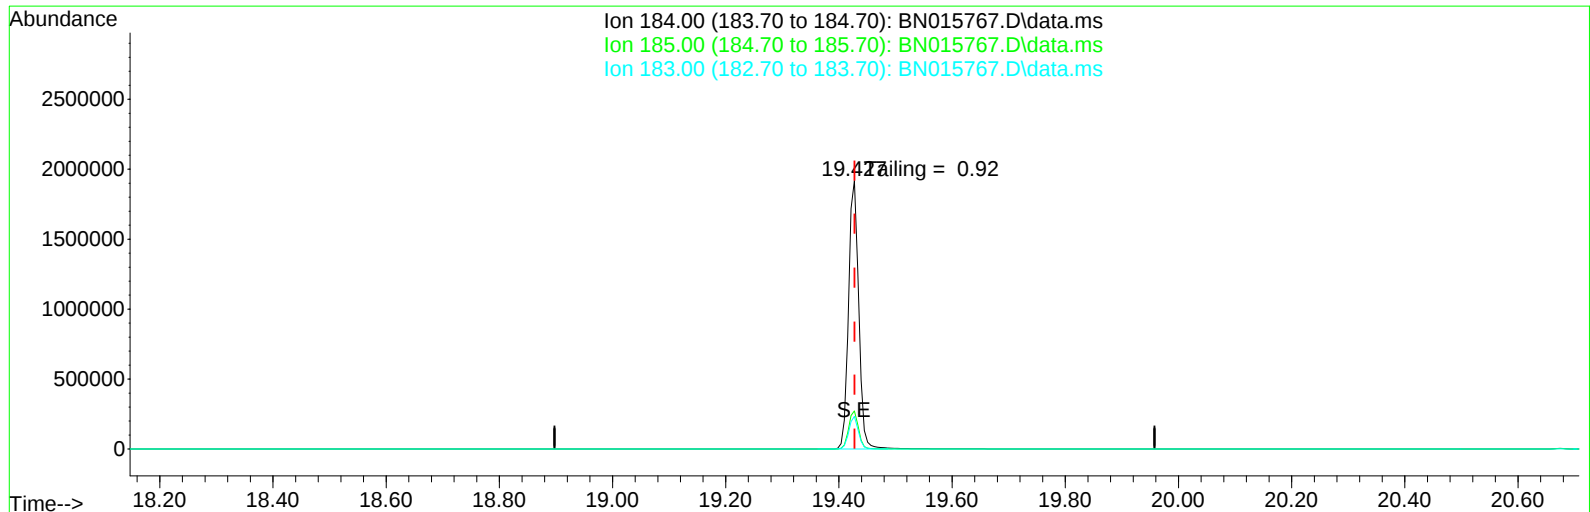

TIC: BN015767.D\data.ms

(77) Benzidine

19.427min (-0.000) 0.00 ng

response 2392373

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	12.18
0.00	0.00	0.00