

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
 Data File : BN015780.D
 Acq On : 03 Aug 2021 22:09
 Operator : CG/JU
 Sample : M2940-08
 Misc : LOQ-WATER-0.1ng
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT3-2021

Manual Integrations
 APPROVED

mohammad
 8/4/2021 3:46:49 PM

Quant Time: Aug 04 02:16:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 02:14:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	40702	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	181255	0.400	ng	0.00
13) Acenaphthene-d10	14.408	164	92736	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	175143	0.400	ng	0.00
29) Chrysene-d12	21.365	240	149266	0.400	ng	# 0.00
35) Perylene-d12	23.707	264	146090	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	37890	0.381	ng	0.00
5) Phenol-d6	6.951	99	44042	0.366	ng	0.00
8) Nitrobenzene-d5	8.924	82	33749	0.290	ng	0.00
11) 2-Methylnaphthalene-d10	12.158	152	90067	0.331	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	9621	0.286	ng	0.00
15) 2-Fluorobiphenyl	13.038	172	122309	0.331	ng	0.00
27) Fluoranthene-d10	19.207	212	145931	0.320	ng	0.00
31) Terphenyl-d14	19.807	244	129010	0.349	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.355	88	1088	0.083	ng	97
3) n-Nitrosodimethylamine	3.742	42	1985	0.073	ng	# 98
6) bis(2-Chloroethyl)ether	7.218	93	11987	0.110	ng	99
9) Naphthalene	10.622	128	49933	0.105	ng	100
10) Hexachlorobutadiene	10.914	225	8436	0.102	ng	# 100
12) 2-Methylnaphthalene	12.234	142	32402	0.106	ng	100
16) Acenaphthylene	14.129	152	33036	0.086	ng	99
17) Acenaphthene	14.472	154	26002	0.097	ng	100
18) Fluorene	15.461	166	30828	0.097	ng	100
20) 4,6-Dinitro-2-methylph...	15.550	198	333	0.031	ng	# 42
21) 4-Bromophenyl-phenylether	16.360	248	9677	0.094	ng	95
22) Hexachlorobenzene	16.470	284	11688	0.099	ng	100
23) Atrazine	16.628	200	5543	0.088	ng	98
24) Pentachlorophenol	16.811	266	1710	0.047	ng	99
25) Phenanthrene	17.200	178	51774	0.099	ng	99
26) Anthracene	17.297	178	39647	0.091	ng	100
28) Fluoranthene	19.232	202	53421	0.099	ng	100
30) Pyrene	19.599	202	50626	0.102	ng	100
32) Benzo(a)anthracene	21.355	228	41720	0.091	ng	99
33) Chrysene	21.408	228	49848	0.101	ng	99
34) Bis(2-ethylhexyl)phtha...	21.302	149	13586	0.074	ng	99
36) Indeno(1,2,3-cd)pyrene	26.106	276	45955	0.089	ng	96
37) Benzo(b)fluoranthene	22.998	252	47934	0.094	ng	98
38) Benzo(k)fluoranthene	23.046	252	53257m	0.101	ng	
39) Benzo(a)pyrene	23.604	252	38611	0.092	ng	96
40) Dibenzo(a,h)anthracene	26.127	278	37828	0.087	ng	# 88
41) Benzo(g,h,i)perylene	26.835	276	40517	0.090	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015780.D
Acq On : 03 Aug 2021 22:09
Operator : CG/JU
Sample : M2940-08
Misc : LOQ-WATER-0.1ng
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM


Quant Time: Aug 04 02:16:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 02:14:12 2021
Response via : Initial Calibration





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.790 min Scan# 511
 Delta R.T. -0.000 min
 Lab File: BN015780.D
 Acq: 03 Aug 2021 22:09




Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT3-2021




Tgt Ion: 152 Resp: 40702
 Ion Ratio Lower Upper
 152 100
 150 154.0 123.5 185.3
 115 58.3 46.8 70.2

Manual Integrations
 APPROVED



mohammad
 8/4/2021 3:46:49 PM




#2
 1,4-Dioxane
 Concen: 0.083 ng
 RT: 3.355 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN015780.D
 Acq: 03 Aug 2021 22:09



Tgt Ion: 88 Resp: 1088
 Ion Ratio Lower Upper
 88 100
 43 26.7 23.1 34.7
 58 79.9 62.2 93.4



Abundance Scan 69 (3.715 min): BN015760.D\data.ms (-63)







#3
n-Nitrosodimethylamine
Concen: 0.073 ng
RT: 3.742 min Scan# 72
Delta R.T. 0.027 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion: 42 Resp: 1985
Ion Ratio Lower Upper
42 100
74 145.0 114.4 171.6
44 0.0 3.6 5.4#

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM




#4
2-Fluorophenol
Concen: 0.381 ng
RT: 5.383 min Scan# 250
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion: 112 Resp: 37890
Ion Ratio Lower Upper
112 100
64 53.1 42.2 63.4
63 28.0 22.2 33.2








#5
Phenol-d6
Concen: 0.366 ng
RT: 6.951 min Scan# 420
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion: 99 Resp: 44042

Ion	Ratio	Lower	Upper
99	100		
42	16.1	13.2	19.8
71	29.7	23.8	35.8





#6
bis(2-Chloroethyl)ether
Concen: 0.110 ng
RT: 7.218 min Scan# 449
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09



Tgt Ion: 93 Resp: 11987


Ion	Ratio	Lower	Upper
93	100		
63	74.3	58.8	88.2
95	33.7	26.6	39.8



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021


Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Tgt Ion:	136	Resp:	181255
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	4.8	3.9	5.9
68	4.0	3.3	4.9

Manual Integrations
APPROVED



mohammad
8/4/2021 3:46:49 PM




#8
Nitrobenzene-d5
Concen: 0.290 ng
RT: 8.924 min Scan# 616
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:	82	Resp:	33749
Ion	Ratio	Lower	Upper
82	100		
128	32.9	26.2	39.4
54	56.5	45.1	67.7






#9
Naphthalene
Concen: 0.105 ng
RT: 10.622 min Scan# 750
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:	128	Resp:	49933
Ion	Ratio	Lower	Upper
128	100		
129	11.2	8.8	13.2
127	12.8	10.2	15.2




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED



mohammad
8/4/2021 3:46:49 PM



#10
Hexachlorobutadiene
Concen: 0.102 ng
RT: 10.914 min Scan# 773
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09



Tgt Ion:	225	Resp:	8436
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.4	51.5	77.3









#11
2-Methylnaphthalene-d10
Concen: 0.331 ng
RT: 12.158 min Scan# 966
Delta R.T. -0.005 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:152 Resp: 90067
Ion Ratio Lower Upper
152 100
151 19.1 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM



#12
2-Methylnaphthalene
Concen: 0.106 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09


Tgt Ion:142 Resp: 32402
Ion Ratio Lower Upper
142 100
141 88.0 70.5 105.7
115 34.1 27.4 41.0





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:164 Resp: 92736
Ion Ratio Lower Upper
164 100
162 103.7 84.2 126.2
160 48.1 39.8 59.6




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM



#14
2,4,6-Tribromophenol
Concen: 0.286 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09


Tgt Ion:330 Resp: 9621
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.8 28.2 42.2





#15
2-Fluorobiphenyl
Concen: 0.331 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:172 Resp: 122309
Ion Ratio Lower Upper
172 100
171 34.7 27.8 41.8
170 23.3 18.7 28.1




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM



#16
Acenaphthylene
Concen: 0.086 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09


Tgt Ion:152 Resp: 33036
Ion Ratio Lower Upper
152 100
151 19.3 15.7 23.5
153 13.0 10.5 15.7





#17
Acenaphthene
Concen: 0.097 ng
RT: 14.472 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:154 Resp: 26002
Ion Ratio Lower Upper
154 100
153 113.0 90.5 135.7
152 56.1 44.4 66.6




Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM



#18
Fluorene
Concen: 0.097 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:166 Resp: 30828
Ion Ratio Lower Upper
166 100
165 97.7 78.2 117.2
167 13.4 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:188 Resp: 175143
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.8 7.7 11.5

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM



#20
4,6-Dinitro-2-methylphenol
Concen: 0.031 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.012 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09


Tgt Ion:198 Resp: 333
Ion Ratio Lower Upper
198 100
182 37.6 11.1 16.7#
77 0.0 0.0 0.0





#21
4-Bromophenyl-phenylether
Concen: 0.094 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Tgt Ion:248 Resp: 9677
Ion Ratio Lower Upper
248 100
250 97.9 75.8 113.6
141 59.2 52.8 79.2

Manual Integrations
APPROVED



mohammad
8/4/2021 3:46:49 PM




#22
Hexachlorobenzene
Concen: 0.099 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:284 Resp: 11688
Ion Ratio Lower Upper
284 100
142 37.1 29.4 44.2
249 29.9 23.8 35.6





#23
Atrazine
Concen: 0.088 ng
RT: 16.628 min Scan# 1371
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:	200	Resp:	5543
Ion	Ratio	Lower	Upper
200	100		
173	29.5	25.0	37.6
215	46.6	36.3	54.5




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM



#24
Pentachlorophenol
Concen: 0.047 ng
RT: 16.811 min Scan# 1386
Delta R.T. -0.012 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:	266	Resp:	1710
Ion	Ratio	Lower	Upper
266	100		
264	62.6	49.7	74.5
268	66.3	51.8	77.6









#25
Phenanthrene
Concen: 0.099 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.012 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:178 Resp: 51774
Ion Ratio Lower Upper
178 100
176 19.0 15.1 22.7
179 16.4 12.2 18.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM




#26
Anthracene
Concen: 0.091 ng
RT: 17.297 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:178 Resp: 39647
Ion Ratio Lower Upper
178 100
176 18.5 14.6 22.0
179 15.4 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.320 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09





Tgt Ion:212 Resp: 145931
Ion Ratio Lower Upper
212 100
106 13.8 10.8 16.2
104 7.6 6.0 9.0



#28
Fluoranthene
Concen: 0.099 ng
RT: 19.232 min Scan# 1730
Delta R.T. -0.005 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:202 Resp: 53421
Ion Ratio Lower Upper
202 100
101 11.5 9.0 13.6
203 17.2 13.8 20.8




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED




mohammad
8/4/2021 3:46:49 PM

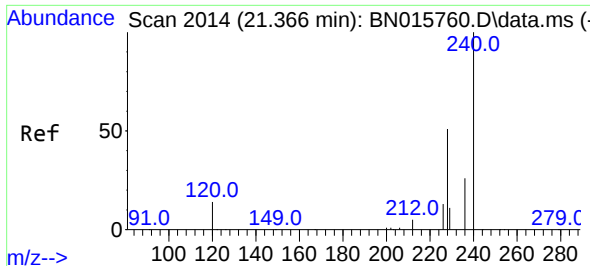


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.365 min Scan# 2014
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09





Tgt Ion:240 Resp: 149266
Ion Ratio Lower Upper
240 100
120 11.0 11.4 17.0#
236 26.3 21.2 31.8



#30
Pyrene
Concen: 0.102 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:202 Resp: 50626
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.6 13.9 20.9



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021


Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM



#31
Terphenyl-d14
Concen: 0.349 ng
RT: 19.807 min Scan# 1846
Delta R.T. -0.005 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:244 Resp: 129010
Ion Ratio Lower Upper
244 100
212 7.7 5.9 8.9
122 13.8 9.7 14.5




Manual Integrations
APPROVED


mohammad
8/4/2021 3:46:49 PM




#32
Benzo(a)anthracene
Concen: 0.091 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:228 Resp: 41720
Ion Ratio Lower Upper
228 100
226 26.0 21.2 31.8
229 20.0 15.6 23.4









#33
Chrysene
Concen: 0.101 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09





Tgt Ion:228 Resp: 49848
Ion Ratio Lower Upper
228 100
226 28.3 23.3 34.9
229 20.2 15.7 23.5



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.074 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09



Tgt Ion:149 Resp: 13586
Ion Ratio Lower Upper
149 100
167 27.2 21.2 31.8
279 4.1 3.2 4.8



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021


Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM



#35
Perylene-d12
Concen: 0.400 ng
RT: 23.707 min Scan# 2492
Delta R.T. -0.007 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:264 Resp: 146090
Ion Ratio Lower Upper
264 100
260 24.5 19.5 29.3
265 23.3 19.2 28.8




Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.089 ng
RT: 26.106 min Scan# 3193
Delta R.T. -0.007 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:276 Resp: 45955
Ion Ratio Lower Upper
276 100
138 28.7 19.6 29.4
277 25.1 20.0 30.0








#37
Benzo(b)fluoranthene
Concen: 0.094 ng
RT: 22.998 min Scan# 2285
Delta R.T. -0.004 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09





Tgt Ion:252 Resp: 47934
Ion Ratio Lower Upper
252 100
253 23.2 17.7 26.5
125 11.1 8.2 12.4



#38
Benzo(k)fluoranthene
Concen: 0.101 ng m
RT: 23.046 min Scan# 2299
Delta R.T. -0.004 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09



Tgt Ion:252 Resp: 53257
Ion Ratio Lower Upper
252 100
253 23.7 17.8 26.6
125 15.5 8.3 12.5#




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED



mohammad
8/4/2021 3:46:49 PM



#39
Benzo(a)pyrene
Concen: 0.092 ng
RT: 23.604 min Scan# 2462
Delta R.T. -0.004 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:252 Resp: 38611
Ion Ratio Lower Upper
252 100
253 24.2 17.8 26.8
125 13.2 9.0 13.6




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED



mohammad
8/4/2021 3:46:49 PM




#40
Dibenzo(a,h)anthracene
Concen: 0.087 ng
RT: 26.127 min Scan# 3199
Delta R.T. -0.004 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09




Tgt Ion:278 Resp: 37828
Ion Ratio Lower Upper
278 100
139 28.3 13.1 19.7#
279 24.7 19.1 28.7





#41
Benzo(g,h,i)perylene
Concen: 0.090 ng
RT: 26.835 min Scan# 3406
Delta R.T. -0.010 min
Lab File: BN015780.D
Acq: 03 Aug 2021 22:09

Tgt Ion:	276	Resp:	40517
Ion Ratio	Lower	Upper	
276	100		
277	24.2	19.0	28.6
138	22.0	16.6	24.8



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED

mohammad
8/4/2021 3:46:49 PM