

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
 Data File : BN015770.D
 Acq On : 03 Aug 2021 16:03
 Operator : CG/JU
 Sample : PB137774BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB137774BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BN015770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.383	245	250	263	rBV	16493	60222	25.42%	2.703%
2	6.951	415	420	432	rBV	27874	61476	25.95%	2.759%
3	7.790	505	511	523	rBV	63346	135925	57.37%	6.101%
4	8.103	540	545	553	rBV	58579	115618	48.80%	5.190%
5	8.936	613	617	623	rBV	34394	74068	31.26%	3.325%
6	10.571	742	746	749	rBV	132545	236728	99.92%	10.626%
7	12.163	956	967	979	rBV	76152	122016	51.50%	5.477%
8	13.038	1083	1086	1089	rBV	153677	228541	96.47%	10.258%
9	14.408	1191	1194	1198	rBV	136825	236910	100.00%	10.634%
10	15.905	1309	1312	1322	rVB2	8192	15711	6.63%	0.705%
11	17.163	1412	1415	1418	rBV	127628	184769	77.99%	8.294%
12	19.207	1717	1725	1758	rBV	138840	200894	84.80%	9.018%
13	19.812	1840	1847	1869	rBV	142463	178806	75.47%	8.026%
14	20.017	1885	1887	1890	rBV3	1149	3210	1.35%	0.144%
15	21.365	2011	2014	2018	rBV	133143	196825	83.08%	8.835%
16	23.714	2480	2494	2528	rVB	87316	176102	74.33%	7.905%




Sum of corrected areas: 2227821

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015770.D
Acq On : 03 Aug 2021 16:03
Operator : CG/JU
Sample : PB137774BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137774BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

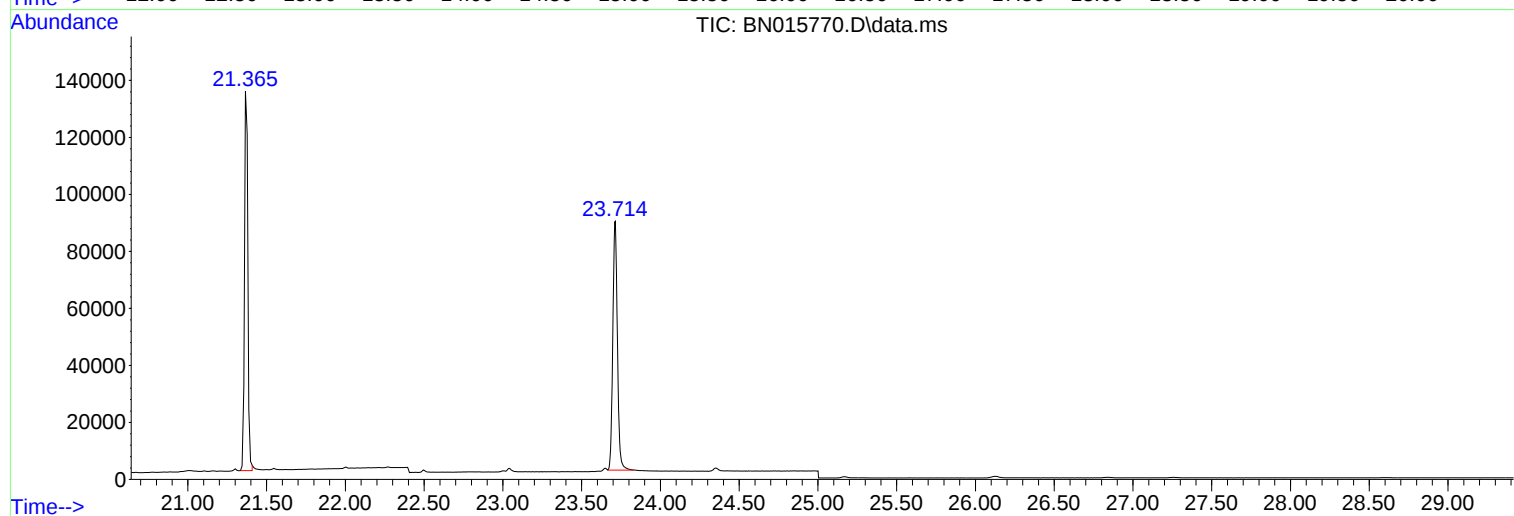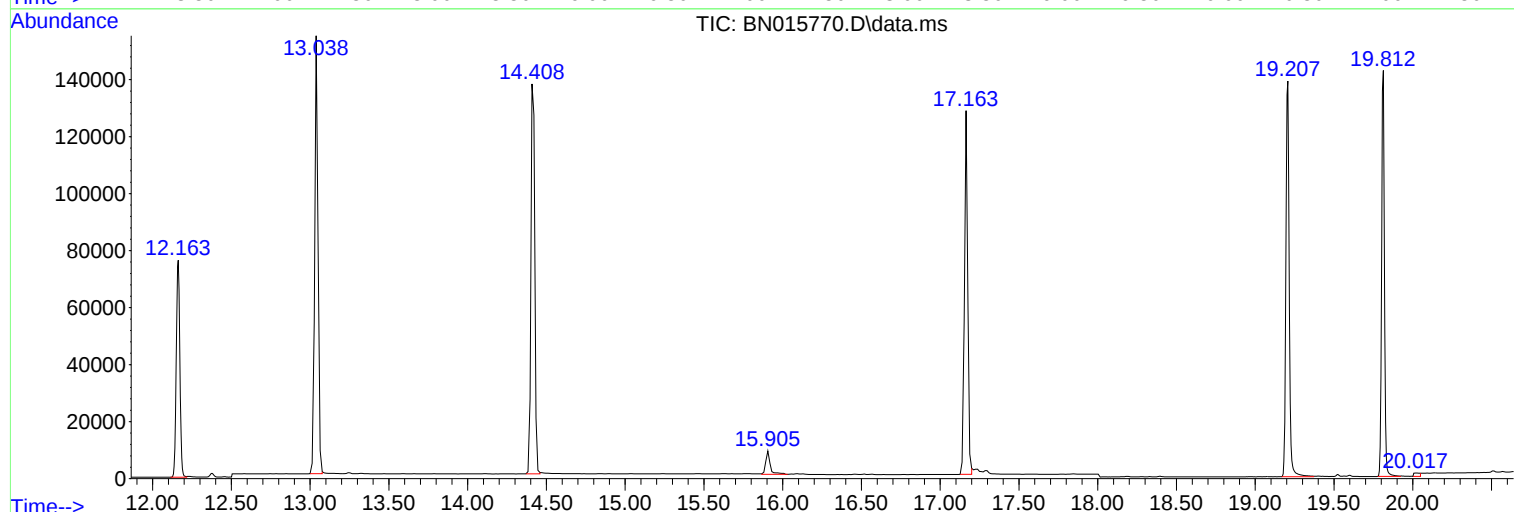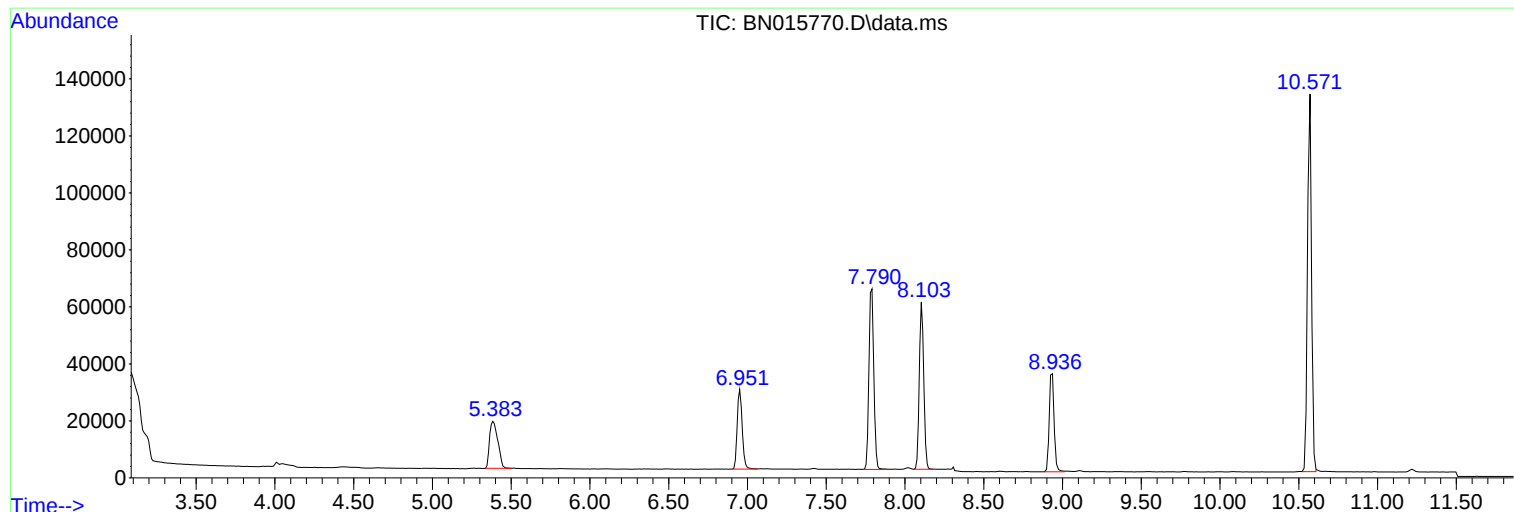

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015770.D
Acq On : 03 Aug 2021 16:03
Operator : CG/JU
Sample : PB137774BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137774BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015770.D
Acq On : 03 Aug 2021 16:03
Operator : CG/JU
Sample : PB137774BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137774BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------