


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
 Data File : BN015767.D
 Acq On : 03 Aug 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 14:09:59 2021

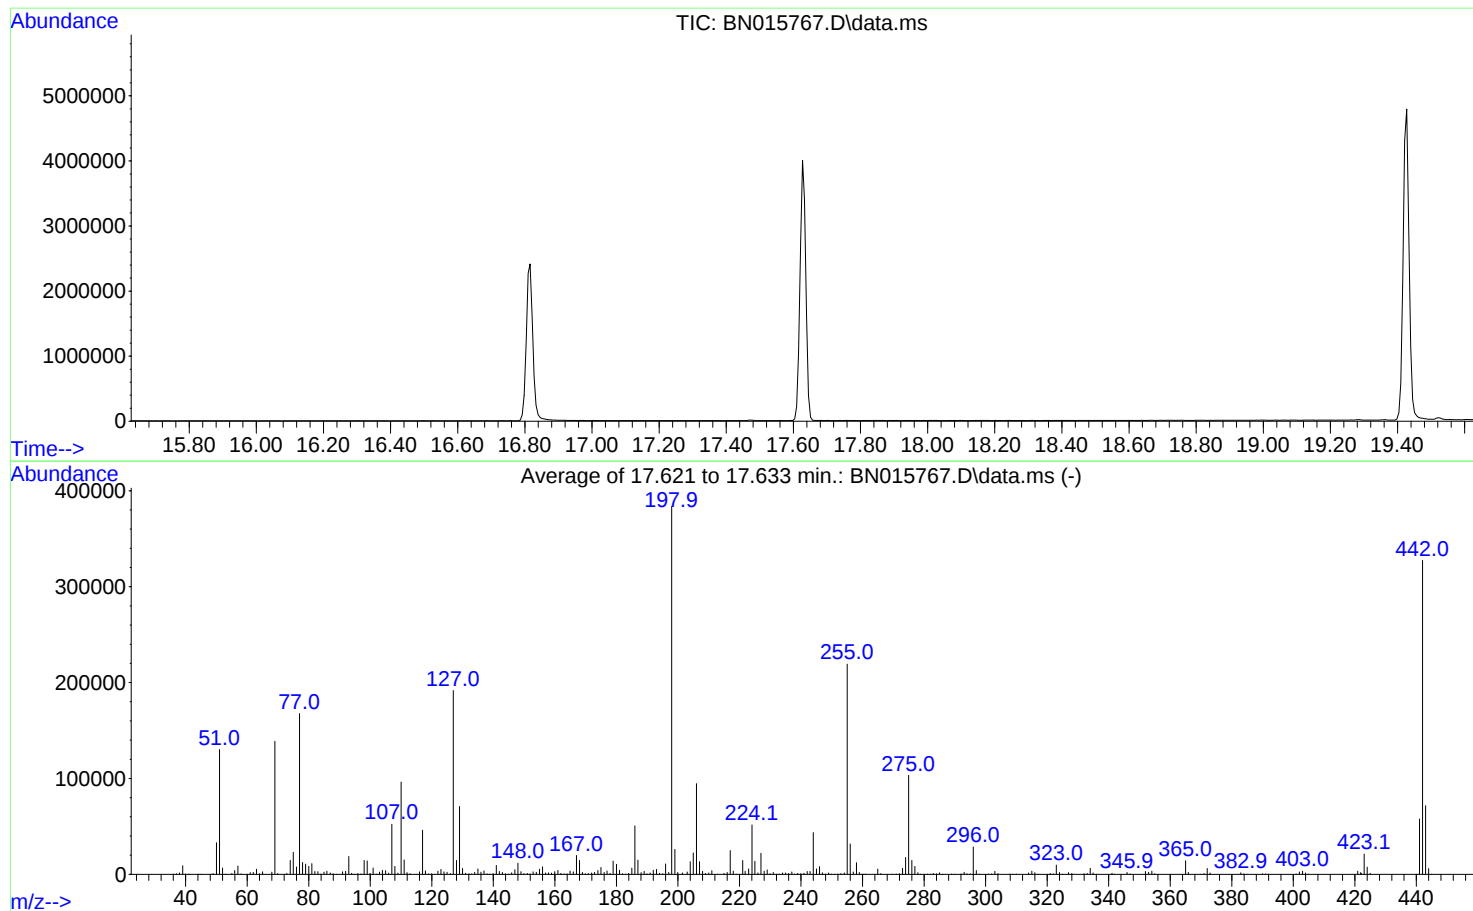




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	130099	PASS
68	69	0.00	2	1.7	2348	PASS
69	198	0.00	100	36.2	138856	PASS
70	69	0.00	2	0.6	802	PASS
127	198	10	80	50.0	191723	PASS
197	198	0.00	2	0.5	2006	PASS
198	198	100	100	100.0	383573	PASS
199	198	5	9	6.8	26085	PASS
275	198	10	60	26.9	103251	PASS
365	198	1	100	3.7	14267	PASS
441	198	0.01	100	15.0	57669	PASS
442	442	50	100	100.0	327275	PASS
443	442	15	24	21.8	71504	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
Data File : BN015767.D
Acq On : 03 Aug 2021 12:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 15:52:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 04:52:40 2021
Response via : Initial Calibration

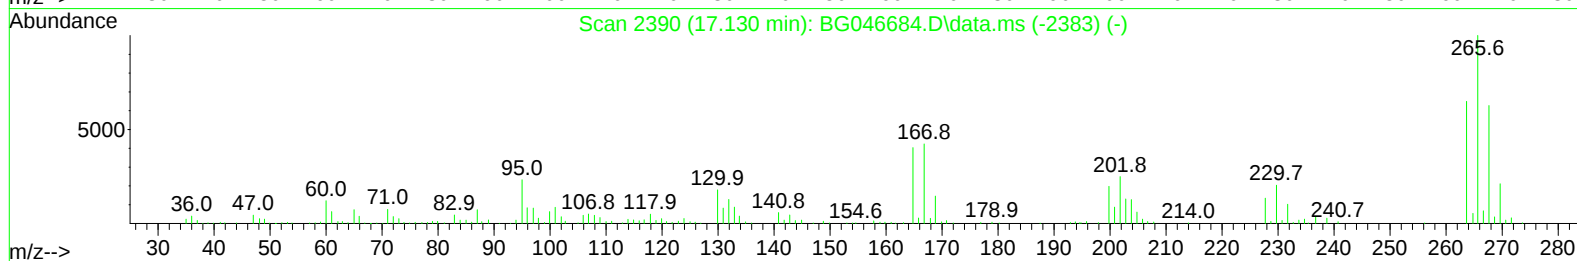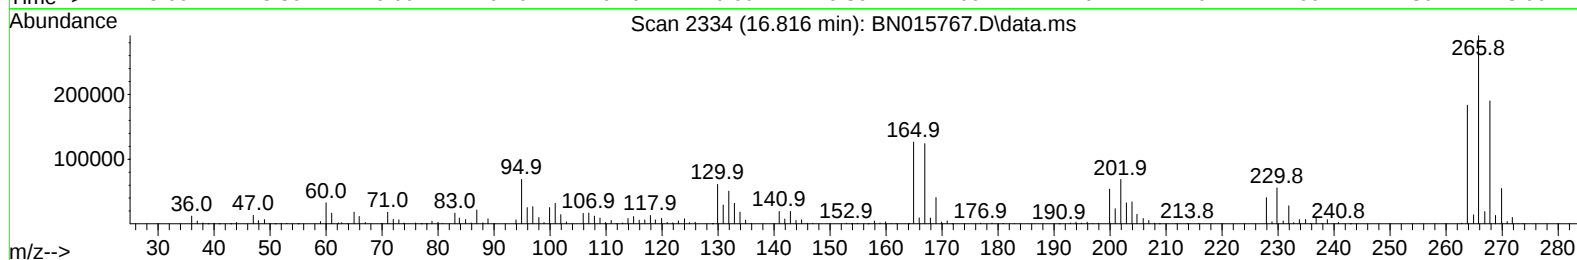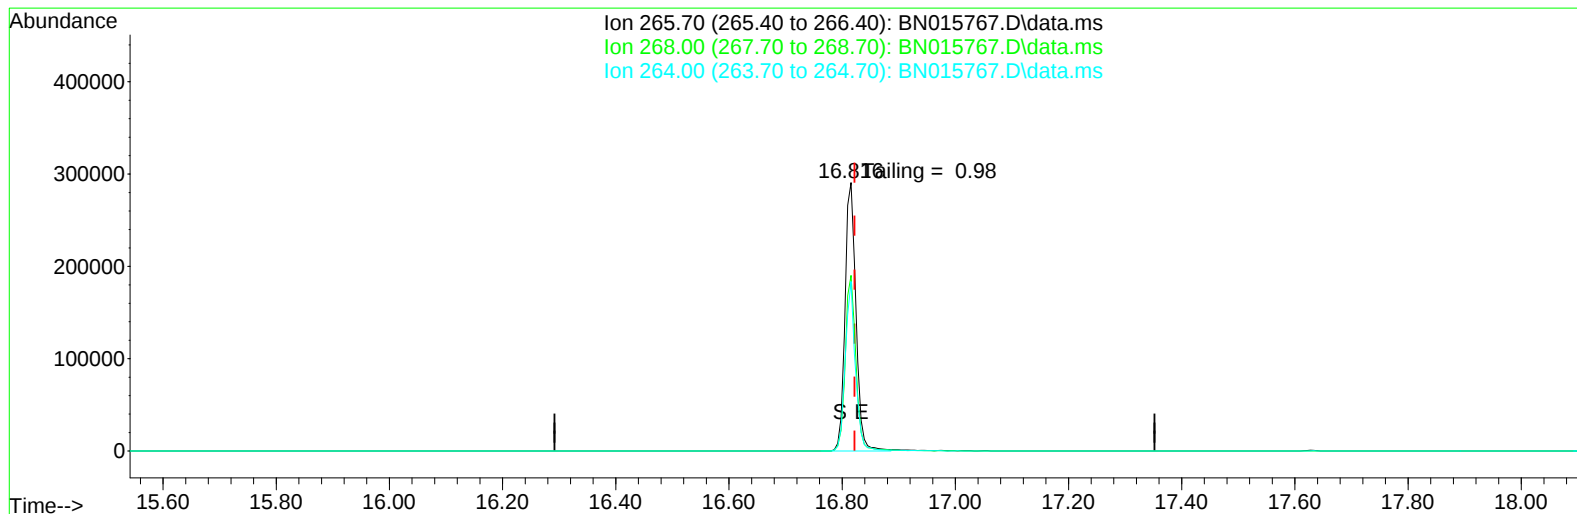

TIC: BN015767.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 19965.46 ng




response 391083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.40
264.00	61.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080321\
 Data File : BN015767.D
 Acq On : 03 Aug 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 15:52:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 04:52:40 2021
 Response via : Initial Calibration

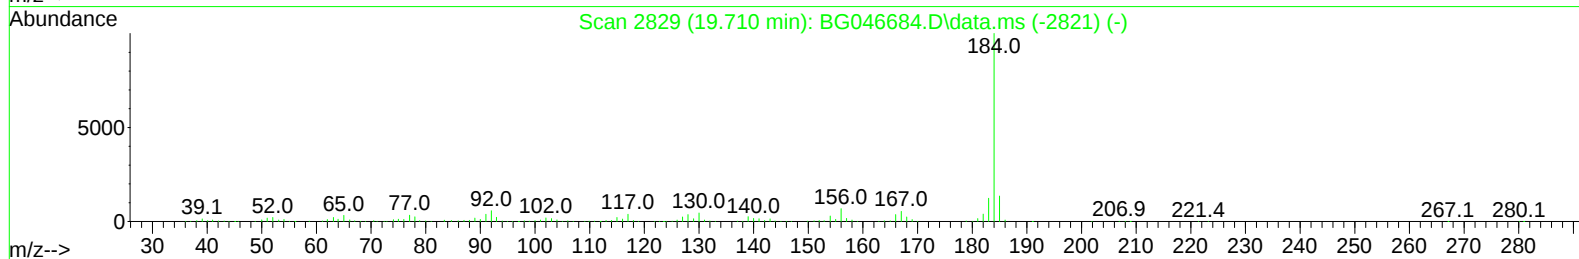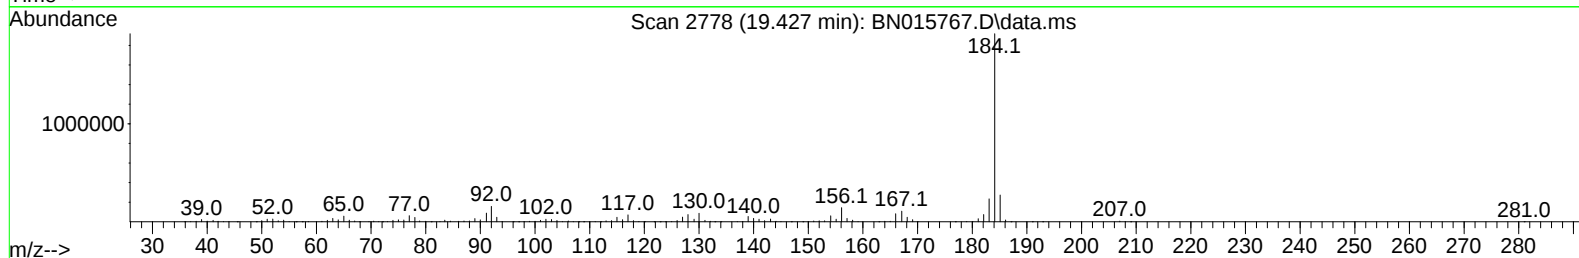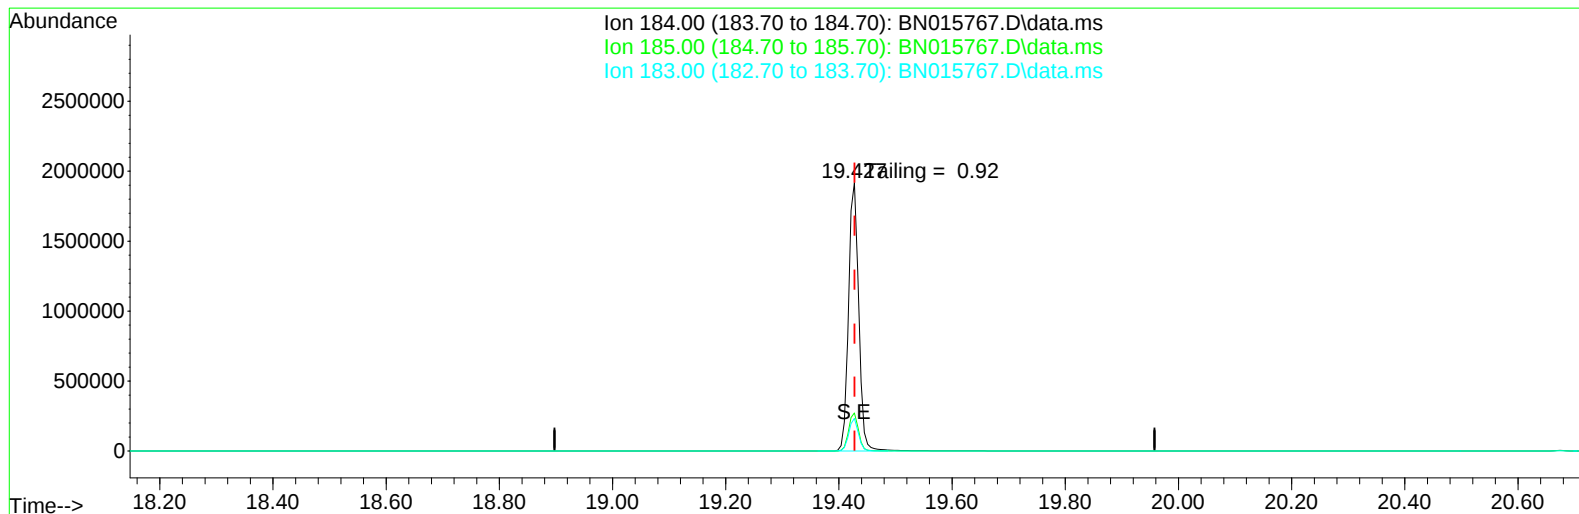

TIC: BN015767.D\data.ms

(77) Benzidine

19.427min (-0.000) 0.00 ng

response 2392373

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2021	BNA_N	<u>BN015767.D</u>
Compound Name	Response	Retention Time
DDT	1183507	20.67
DDD	9142	20.22
DDE	1544	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10686	1194193	0.89

Instrument :
BNA_N
ClientSampleId :
DFTPP