
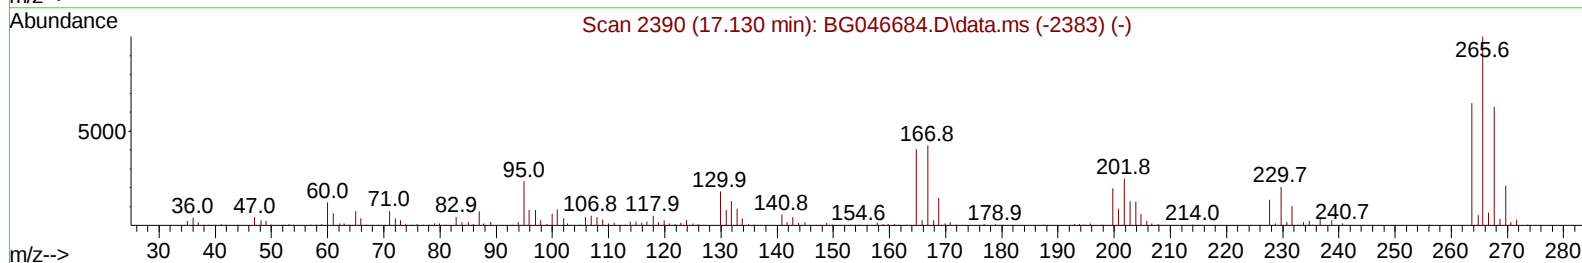
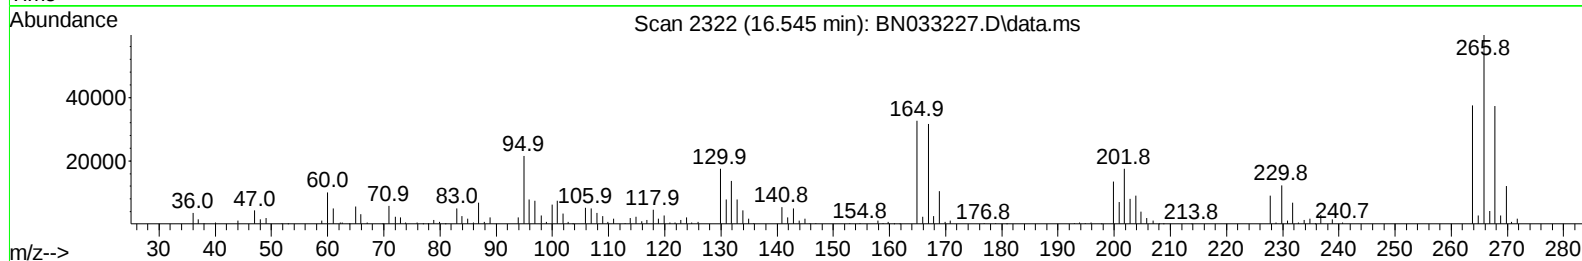


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033227.D
Acq On : 03 Aug 2024 07:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Aug 03 08:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 08:08:34 2024
Response via : Initial Calibration

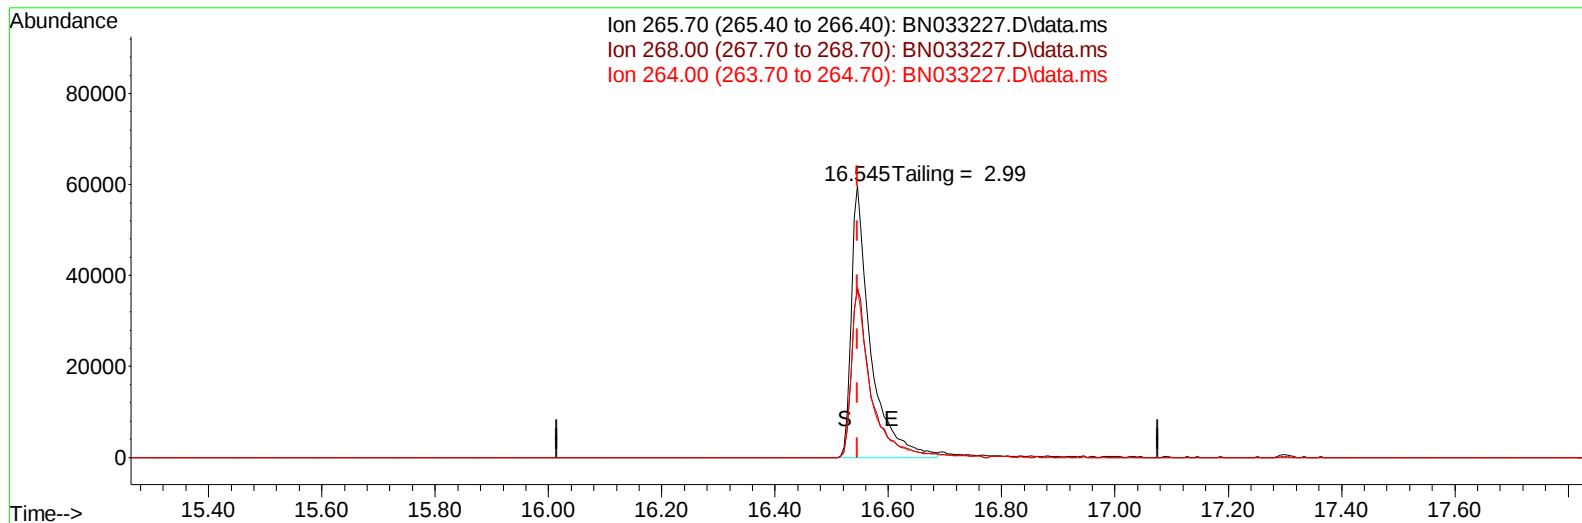




TIC: BN033227.D\data.ms

(70) Pentachlorophenol (C)**16.545min (0.000) 16263.43 ng****response 140905**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.48
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033227.D
Acq On : 03 Aug 2024 07:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Aug 03 08:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 08:08:34 2024
Response via : Initial Calibration

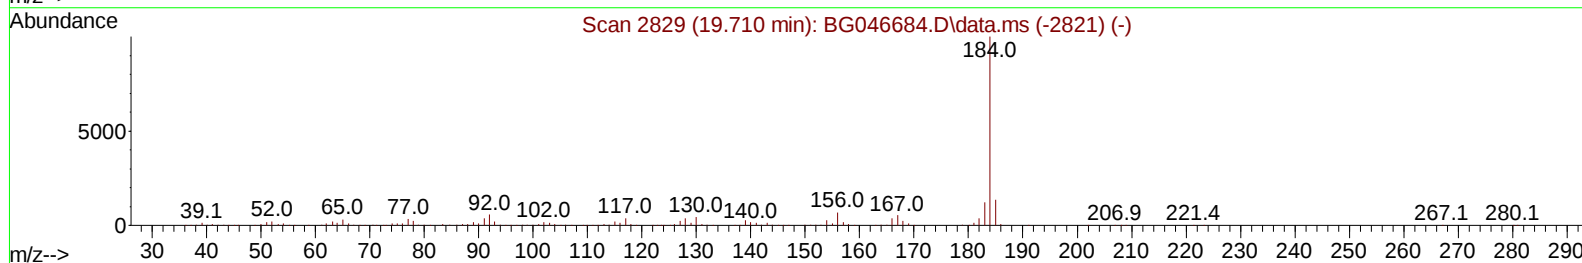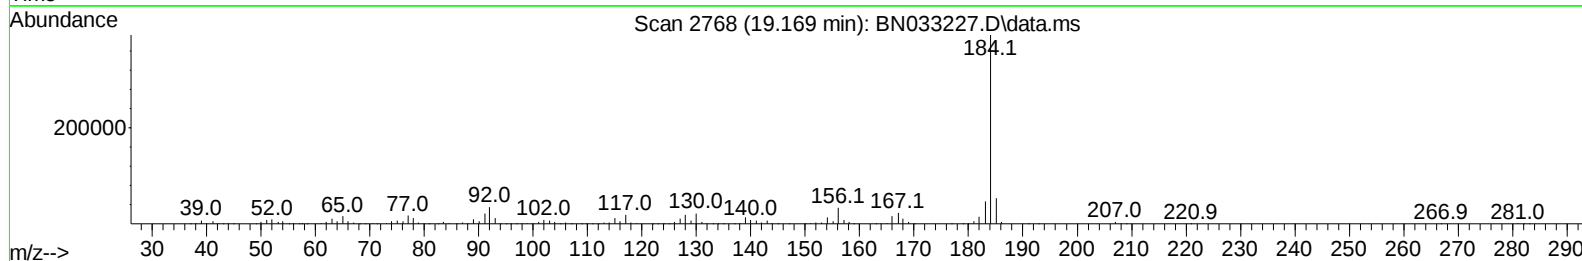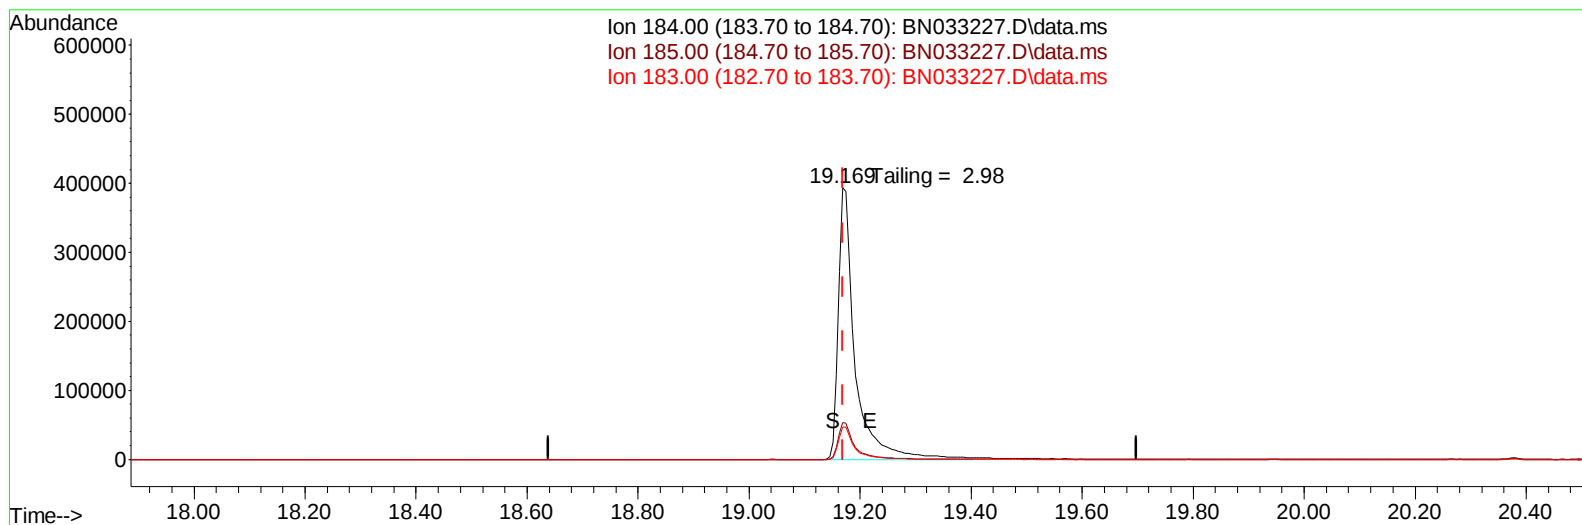

TIC: BN033227.D\data.ms

(77) Benzidine

19.169min (0.000) 0.00 ng

response 845092

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	11.93
0.00	0.00	0.00