
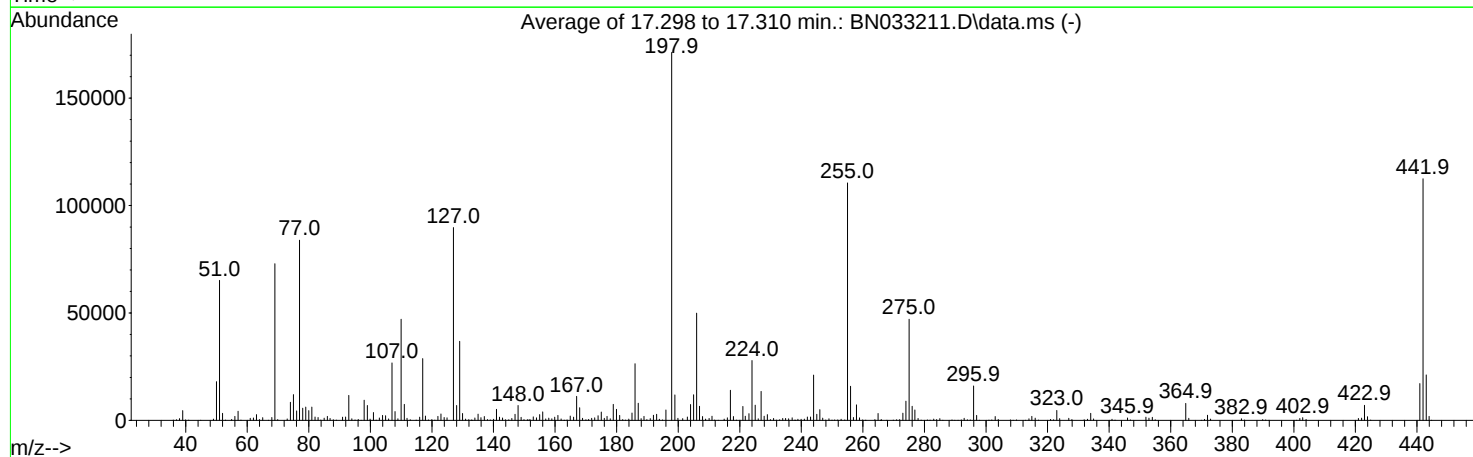


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033211.D
Acq On : 02 Aug 2024 20:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 02 22:49:47 2024

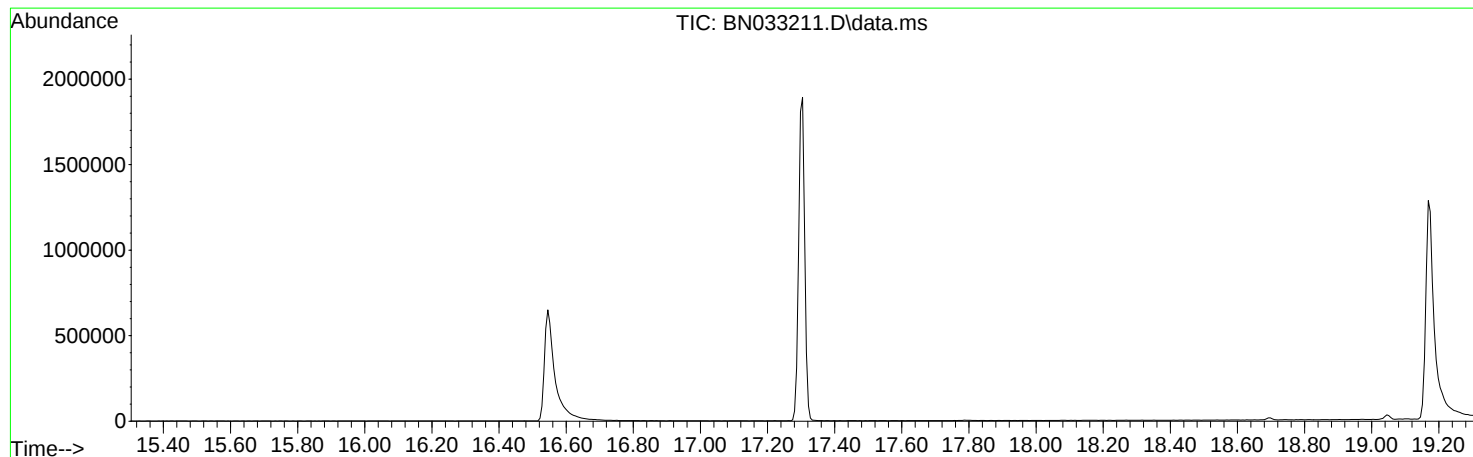

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	65157	PASS
68	69	0.00	2	1.8	1321	PASS
69	198	0.00	100	42.6	72904	PASS
70	69	0.00	2	0.5	400	PASS
127	198	10	80	52.4	89776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	171240	PASS
199	198	5	9	6.9	11880	PASS
275	198	10	60	27.5	47067	PASS
365	198	1	100	4.6	7902	PASS
441	198	0.01	100	10.0	17147	PASS
442	442	50	100	100.0	112451	PASS
443	442	15	24	18.8	21149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/3/2024	BNA_N	<u>BN033211.D</u>
Compound Name	Response	Retention Time
DDT	446251	20.38
DDD	73948	19.945
DDE	2159	19.427
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
76107	522358	14.57

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033211.D
Acq On : 02 Aug 2024 20:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:10:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 06:10:42 2024
Response via : Initial Calibration

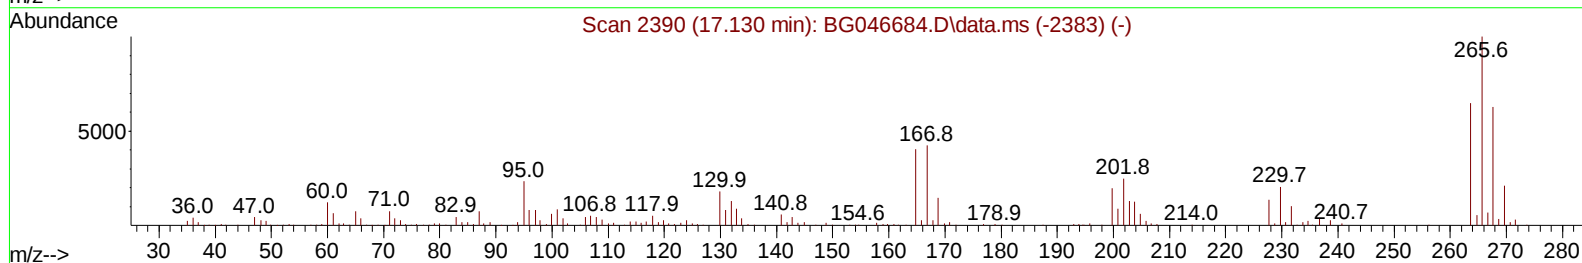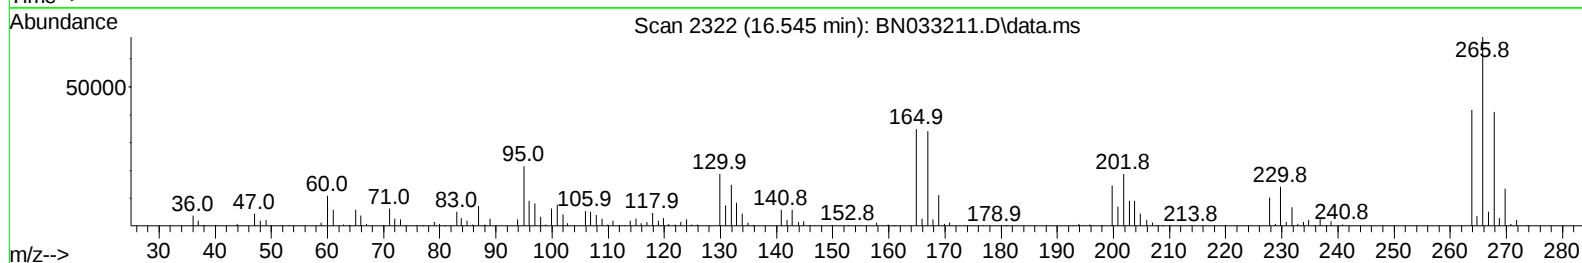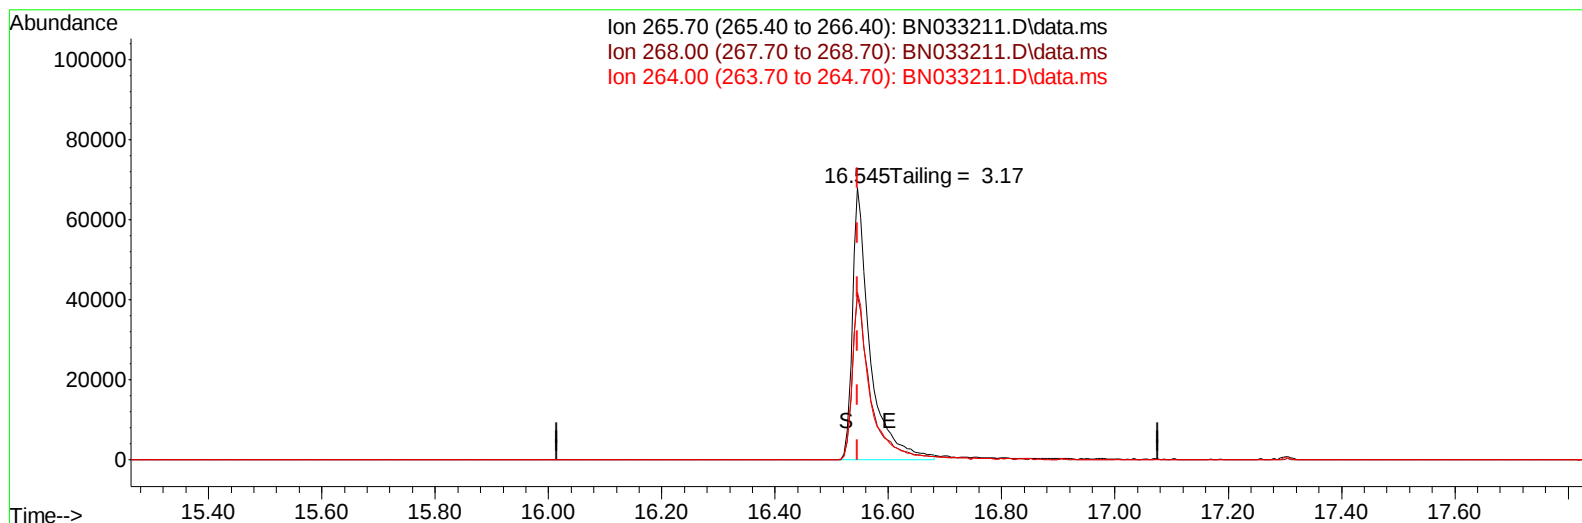

TIC: BN033211.D\data.ms

(70) Pentachlorophenol (C)

16.545min (0.000) 16191.87 ng




response 147655

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.60
264.00	61.60	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033211.D
Acq On : 02 Aug 2024 20:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:10:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 06:10:42 2024
Response via : Initial Calibration

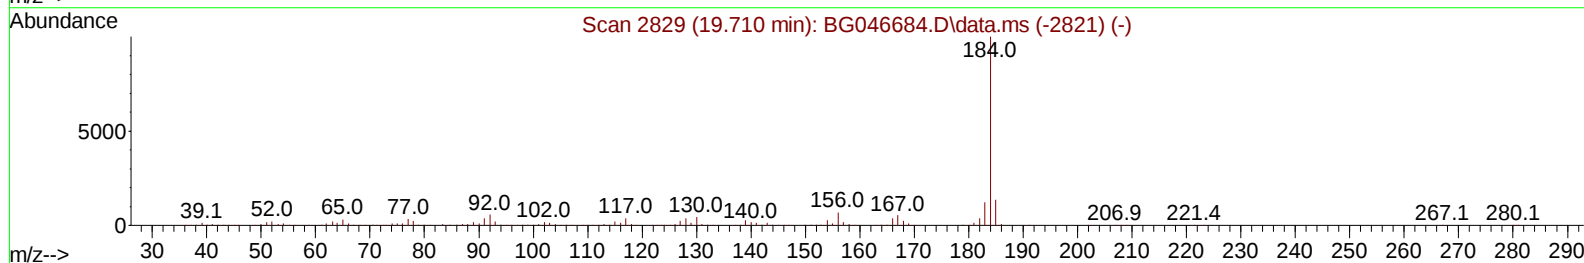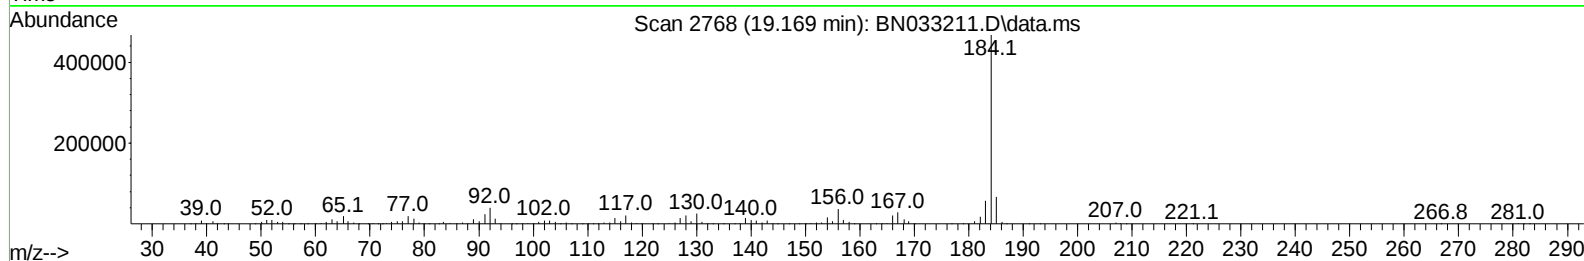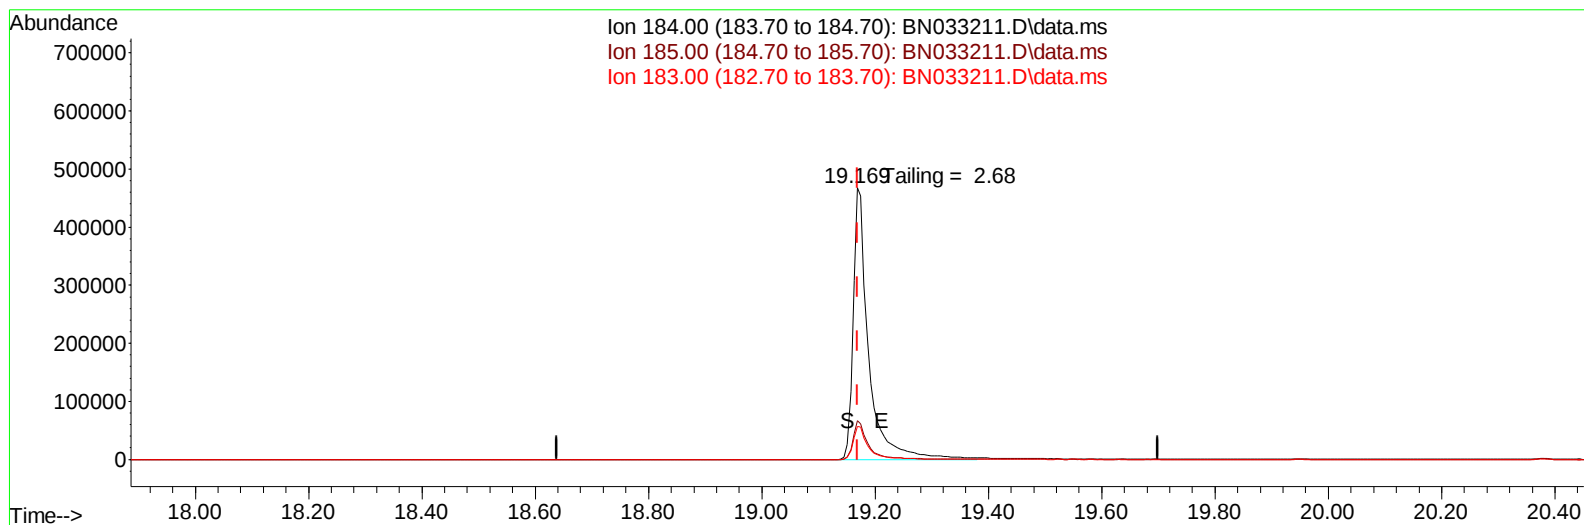

TIC: BN033211.D\data.ms

(77) Benzidine

19.169min (0.000) 0.00 ng

response 895092

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	12.27
0.00	0.00	0.00