
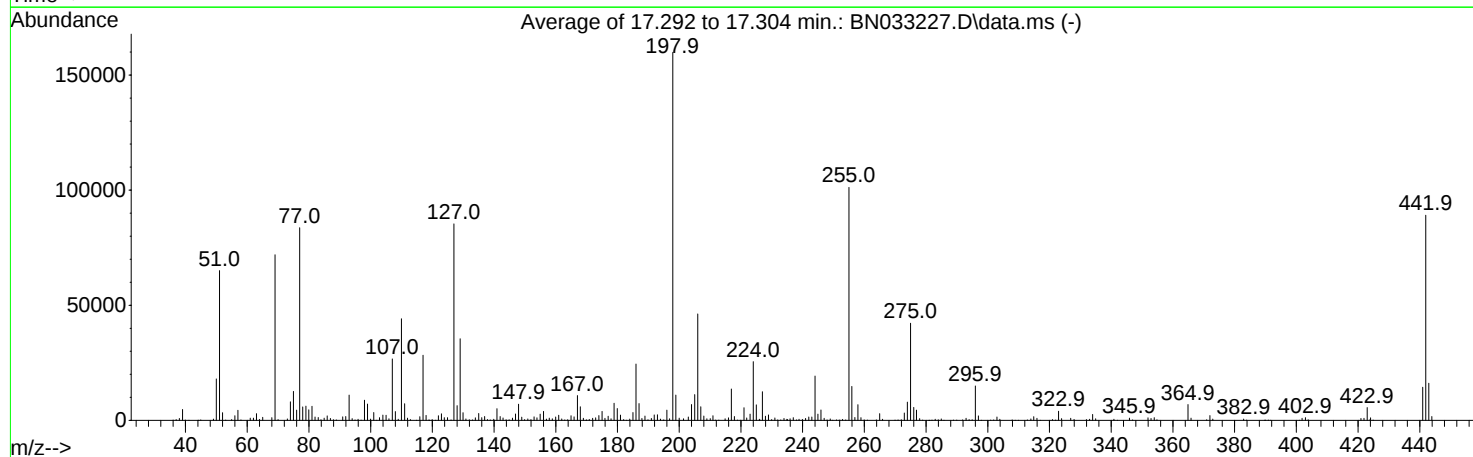


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033227.D
Acq On : 03 Aug 2024 07:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 02 22:49:47 2024

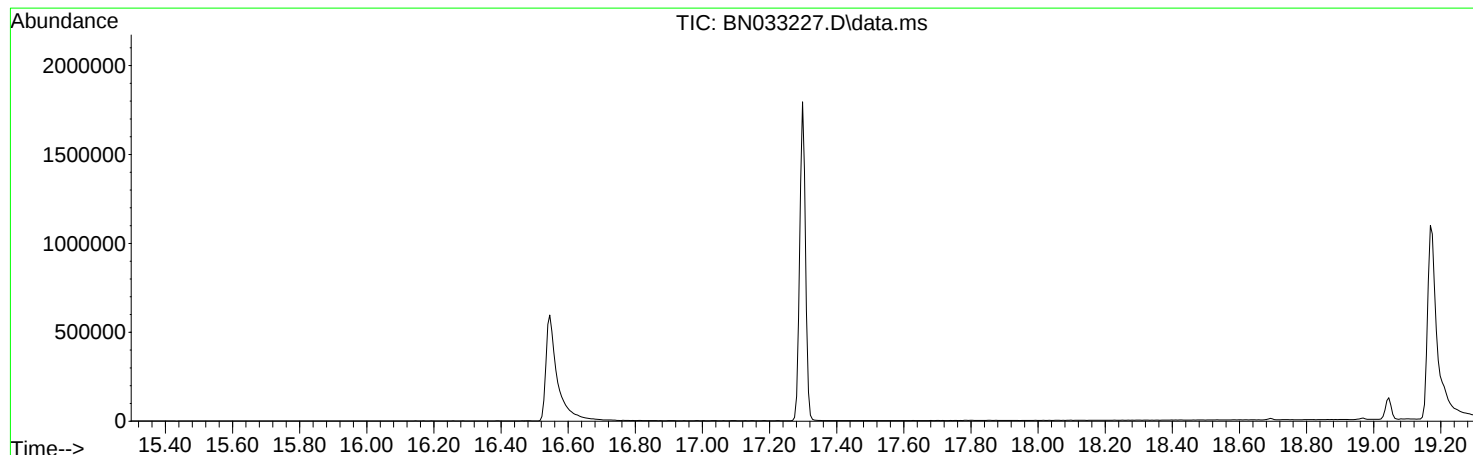

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	65075	PASS
68	69	0.00	2	1.7	1203	PASS
69	198	0.00	100	45.0	71917	PASS
70	69	0.00	2	0.5	343	PASS
127	198	10	80	53.4	85360	PASS
197	198	0.00	2	0.4	710	PASS
198	198	100	100	100.0	159787	PASS
199	198	5	9	6.9	11013	PASS
275	198	10	60	26.4	42229	PASS
365	198	1	100	4.3	6906	PASS
441	198	0.01	100	9.0	14409	PASS
442	442	50	100	100.0	89128	PASS
443	442	15	24	18.1	16097	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/3/2024	BNA_N	<u>BN033227.D</u>
Compound Name	Response	Retention Time
DDT	447194	20.38
DDD	59146	19.945
DDE	2418	19.427
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61564	508758	12.10

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033227.D
Acq On : 03 Aug 2024 07:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 08:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 08:08:34 2024
Response via : Initial Calibration

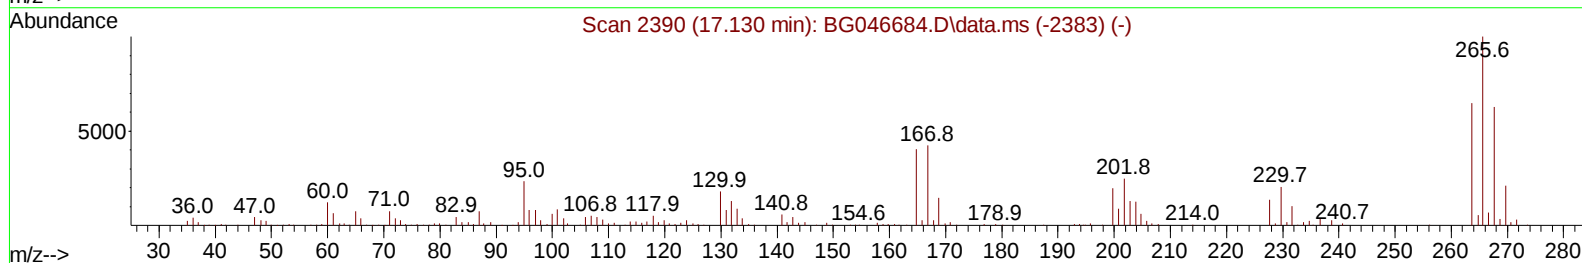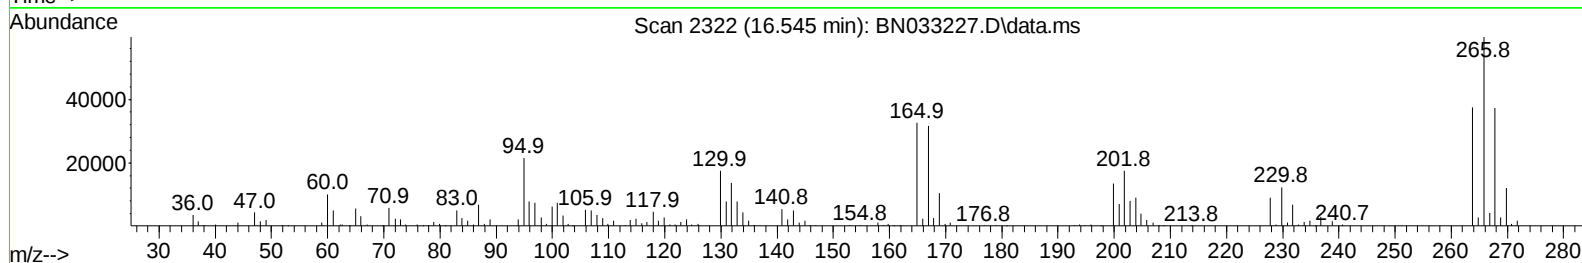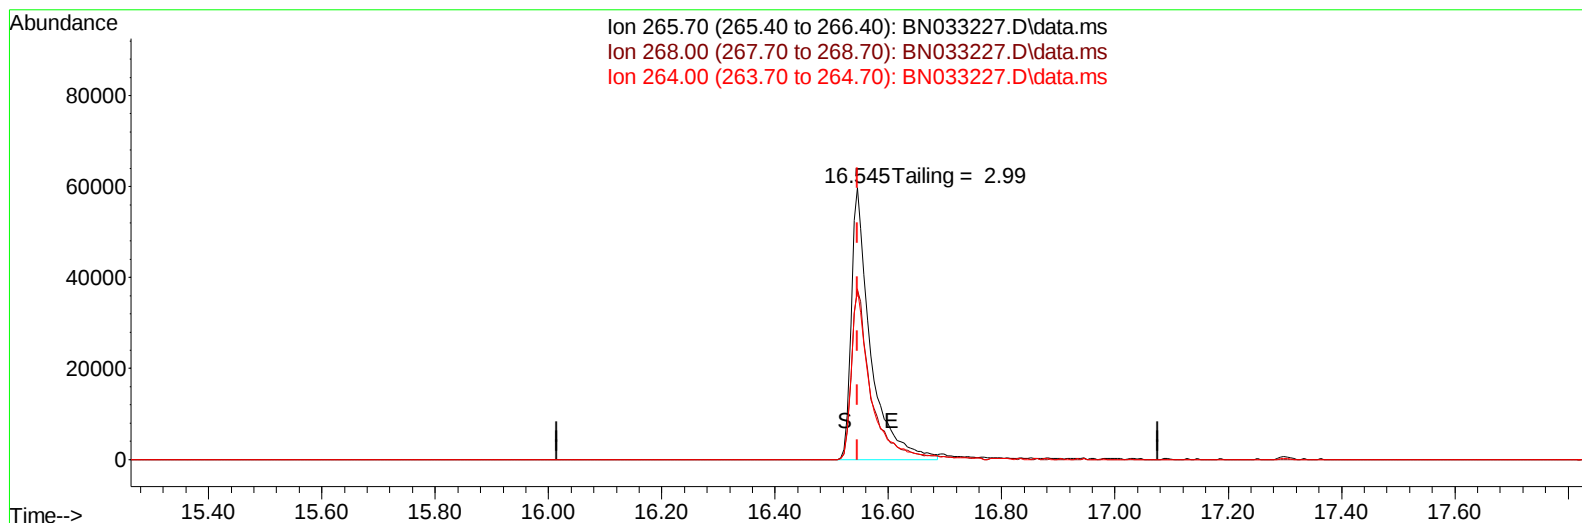

TIC: BN033227.D\data.ms

(70) Pentachloropheno1 (C)

16.545min (0.000) 16263.43 ng




response 140905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.48
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033227.D
Acq On : 03 Aug 2024 07:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 08:08:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 08:08:34 2024
Response via : Initial Calibration

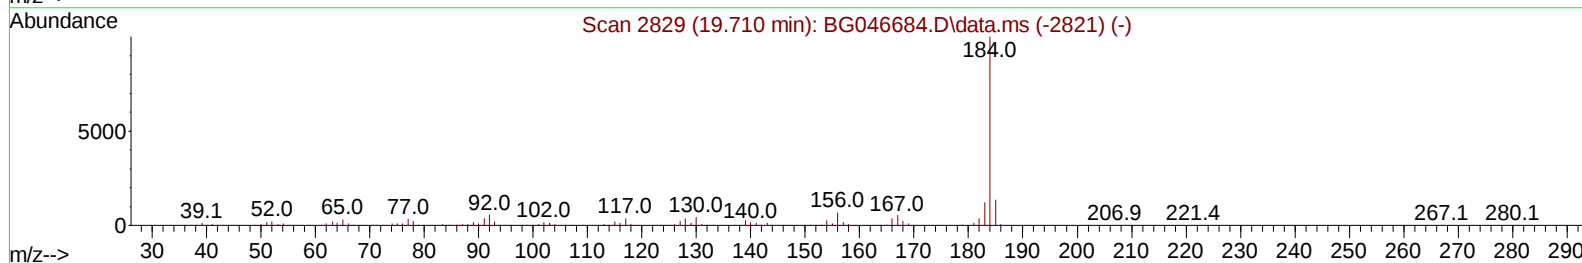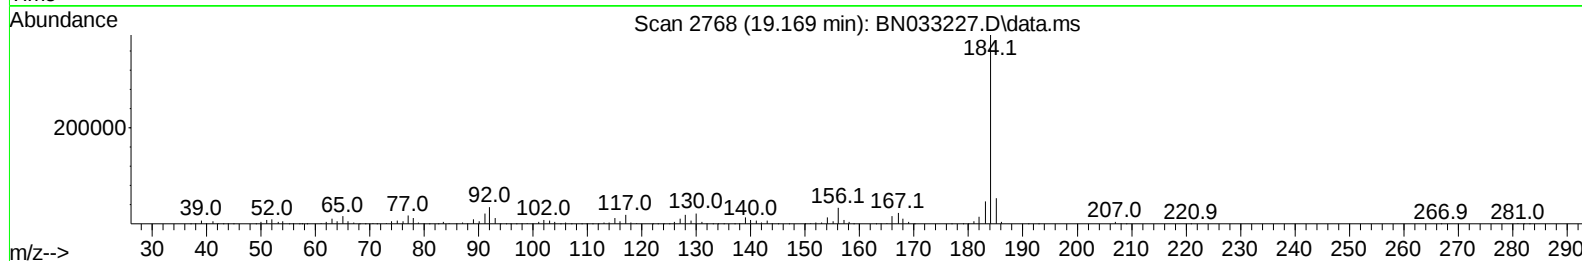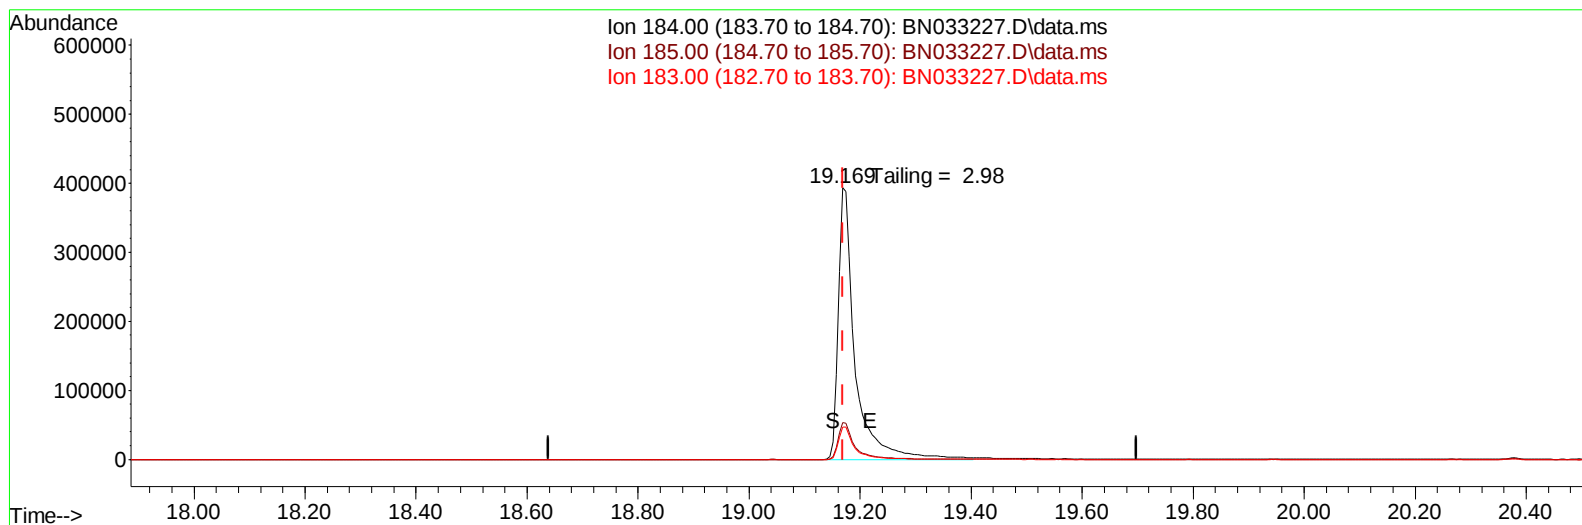

TIC: BN033227.D\data.ms

(77) Benzidine

19.169min (0.000) 0.00 ng

response 845092

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	11.93
0.00	0.00	0.00