
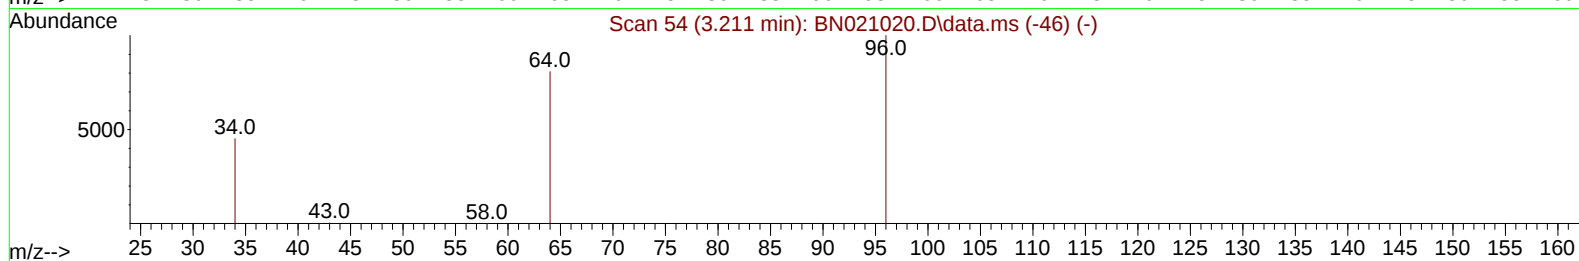
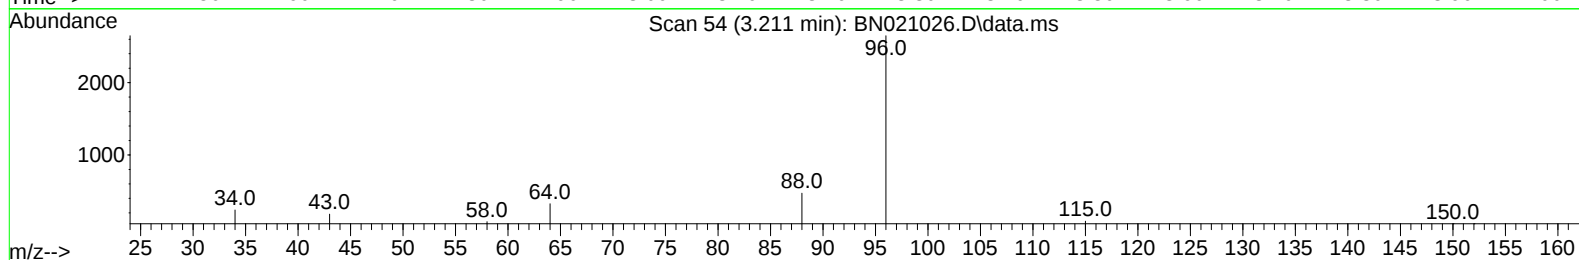


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021026.D
Acq On : 05 Aug 2022 14:39
Operator : CG/JU
Sample : N4026-04MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Aug 06 00:28:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

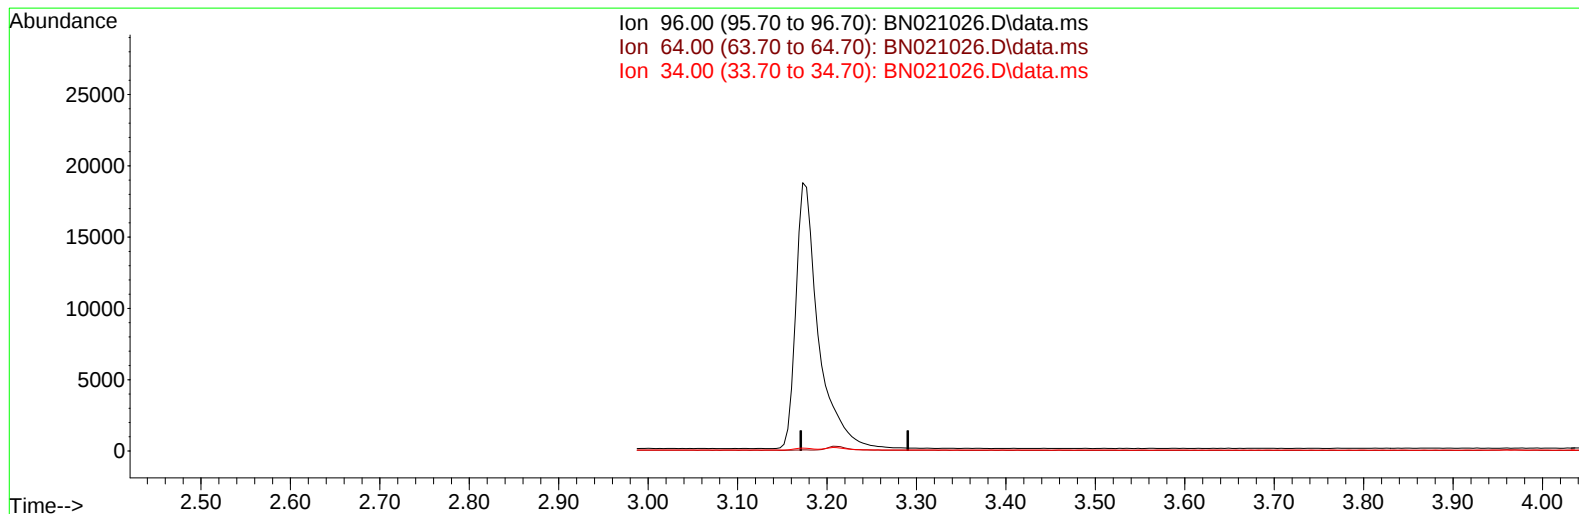

TIC: BN021026.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.211min (-3.211) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	68.40	0.00#
34.00	42.60	0.00#
0.00	0.00	0.00