

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020990.D
 Acq On : 04 Aug 2022 15:35
 Operator : CG/JU
 Sample : N3900-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:21:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	2570	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.596	136	8173	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164	4735	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.205	188	9356	0.400	ng/ul	0.00
17) Chrysene-d12	21.424	240	7581	0.400	ng/ul	0.00
23) Perylene-d12	23.762	264	8394	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	15174	4.615	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	3778	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	9748	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.612	202	1364	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.610	252	2926	0.083	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020990.D
Acq On : 04 Aug 2022 15:35
Operator : CG/JU
Sample : N3900-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 05 01:21:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration




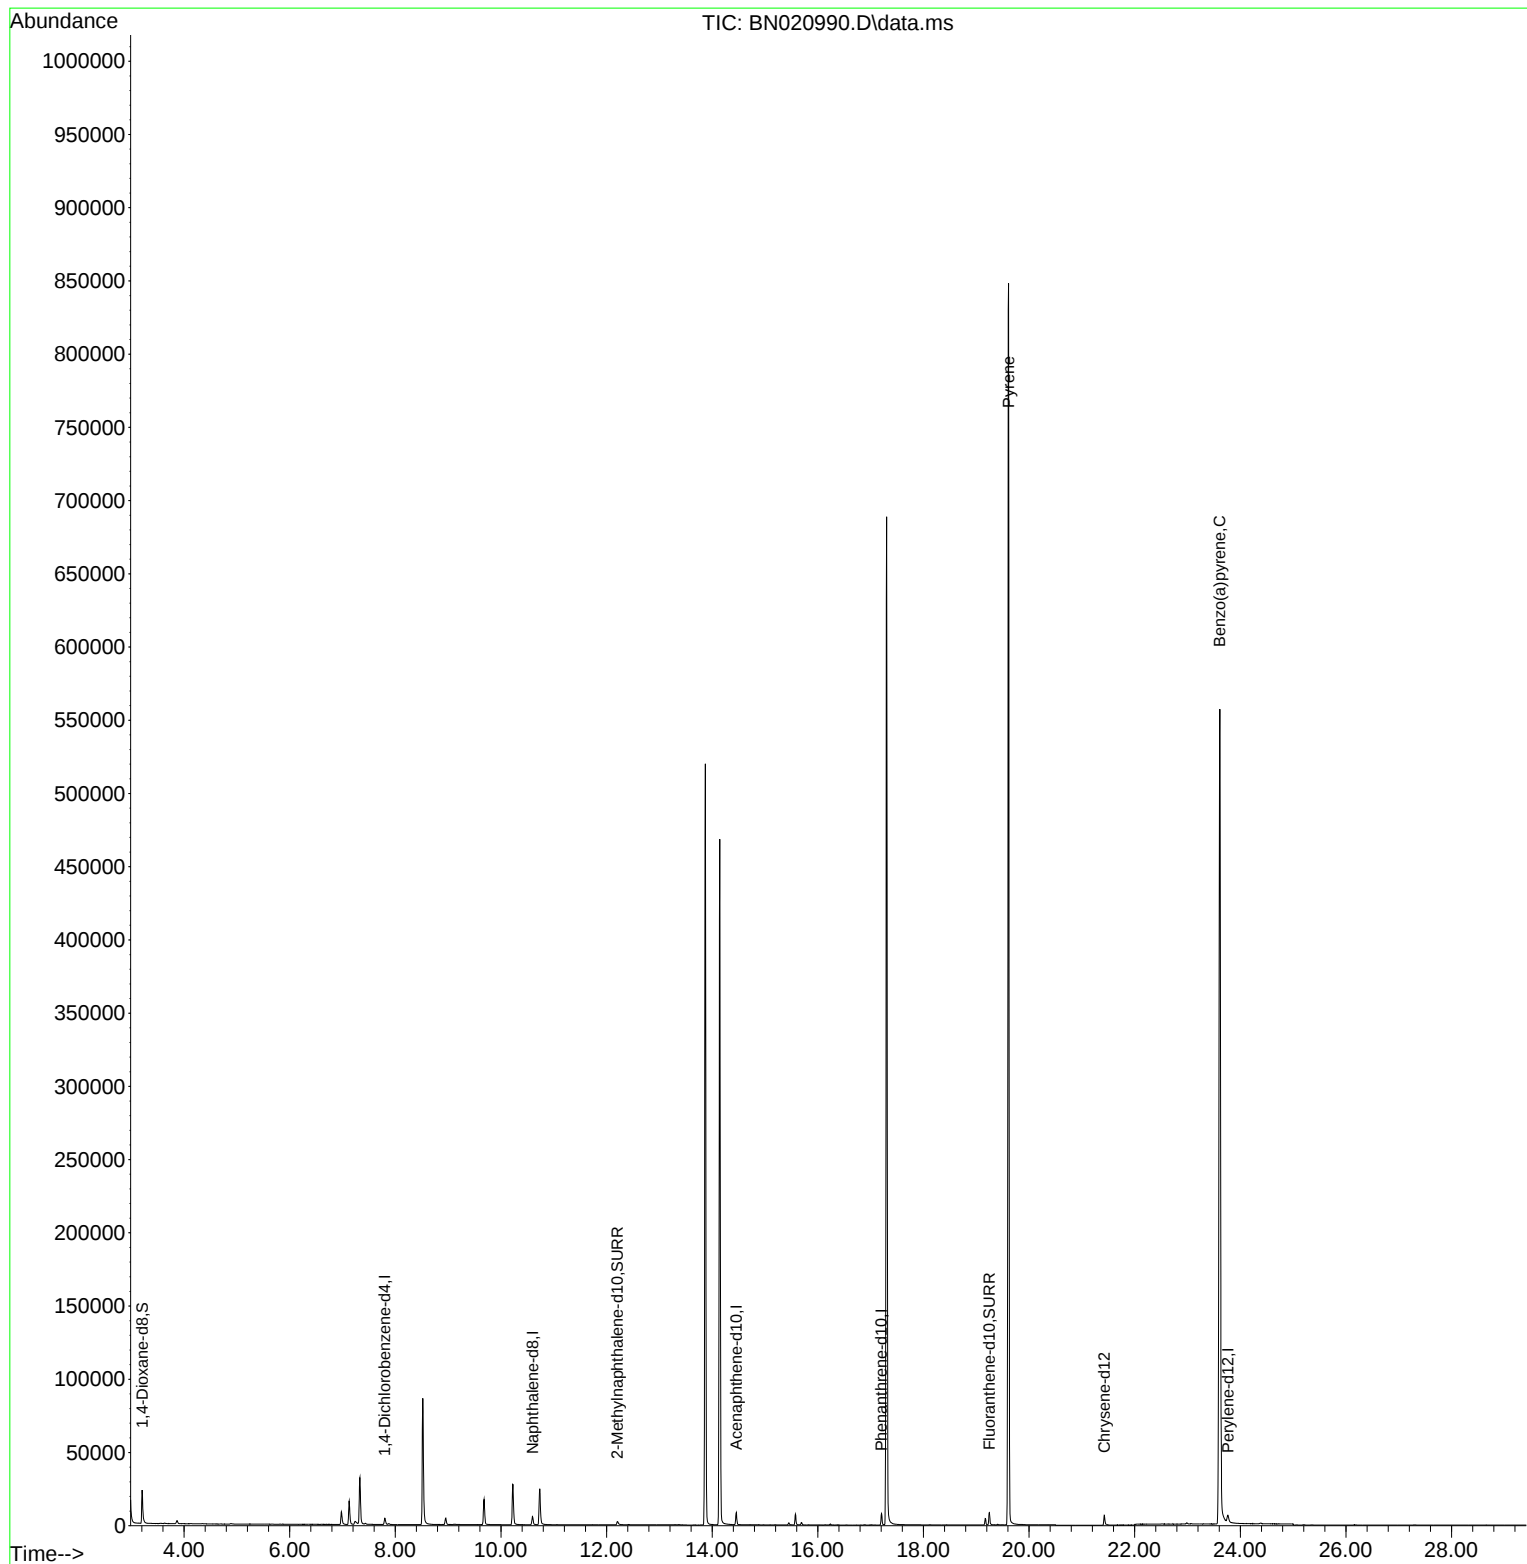


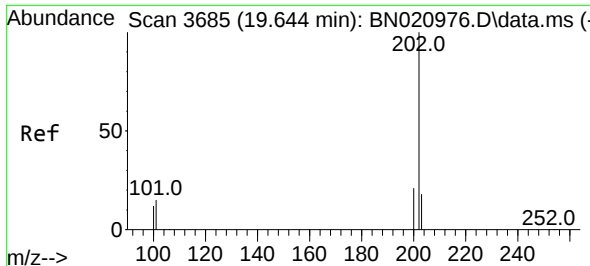

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.612 min Scan# 30
Delta R.T. -0.032 min
Lab File: BN020990.D
Acq: 04 Aug 2022 15:35

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1364
Ion Ratio Lower Upper
202 100
101 176.3 11.3 16.9#
100 1224.3 9.0 13.4#

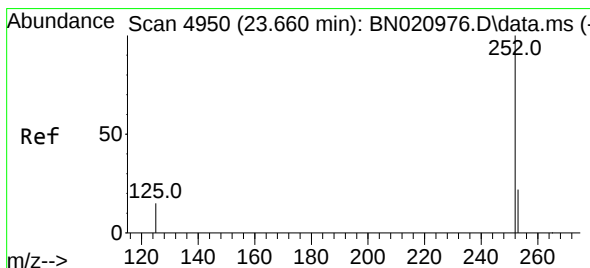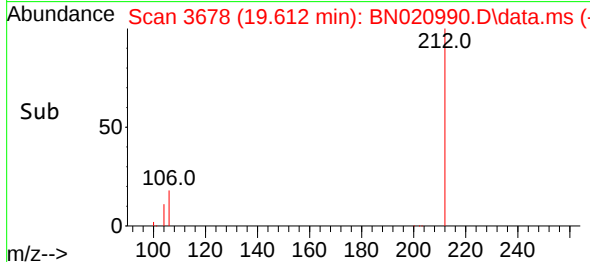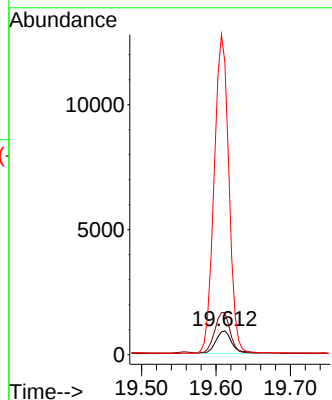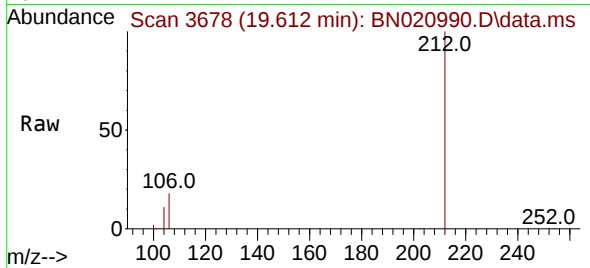

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.610 min Scan# 4933
Delta R.T. -0.050 min
Lab File: BN020990.D
Acq: 04 Aug 2022 15:35

Tgt Ion:252 Resp: 2926
Ion Ratio Lower Upper
252 100
253 44.3 22.1 33.1#
125 35.6 14.7 22.1#

