

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020992.D
 Acq On : 04 Aug 2022 16:51
 Operator : CG/JU
 Sample : N3900-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:21:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.806	152	3223	0.400	ng/ul	0.00
4) Naphthalene-d8	10.601	136	9699	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.456	164	5311	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.209	188	11753	0.400	ng/ul	0.00
17) Chrysene-d12	21.426	240	9241	0.400	ng/ul	0.00
23) Perylene-d12	23.767	264	9860	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	14425	3.498	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	4397	0.309	ng/ul	0.00
18) Fluoranthene-d10	19.248	212	11941	0.418	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.611	202	1710	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.609	252	3488	0.084	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020992.D
Acq On : 04 Aug 2022 16:51
Operator : CG/JU
Sample : N3900-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 05 01:21:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

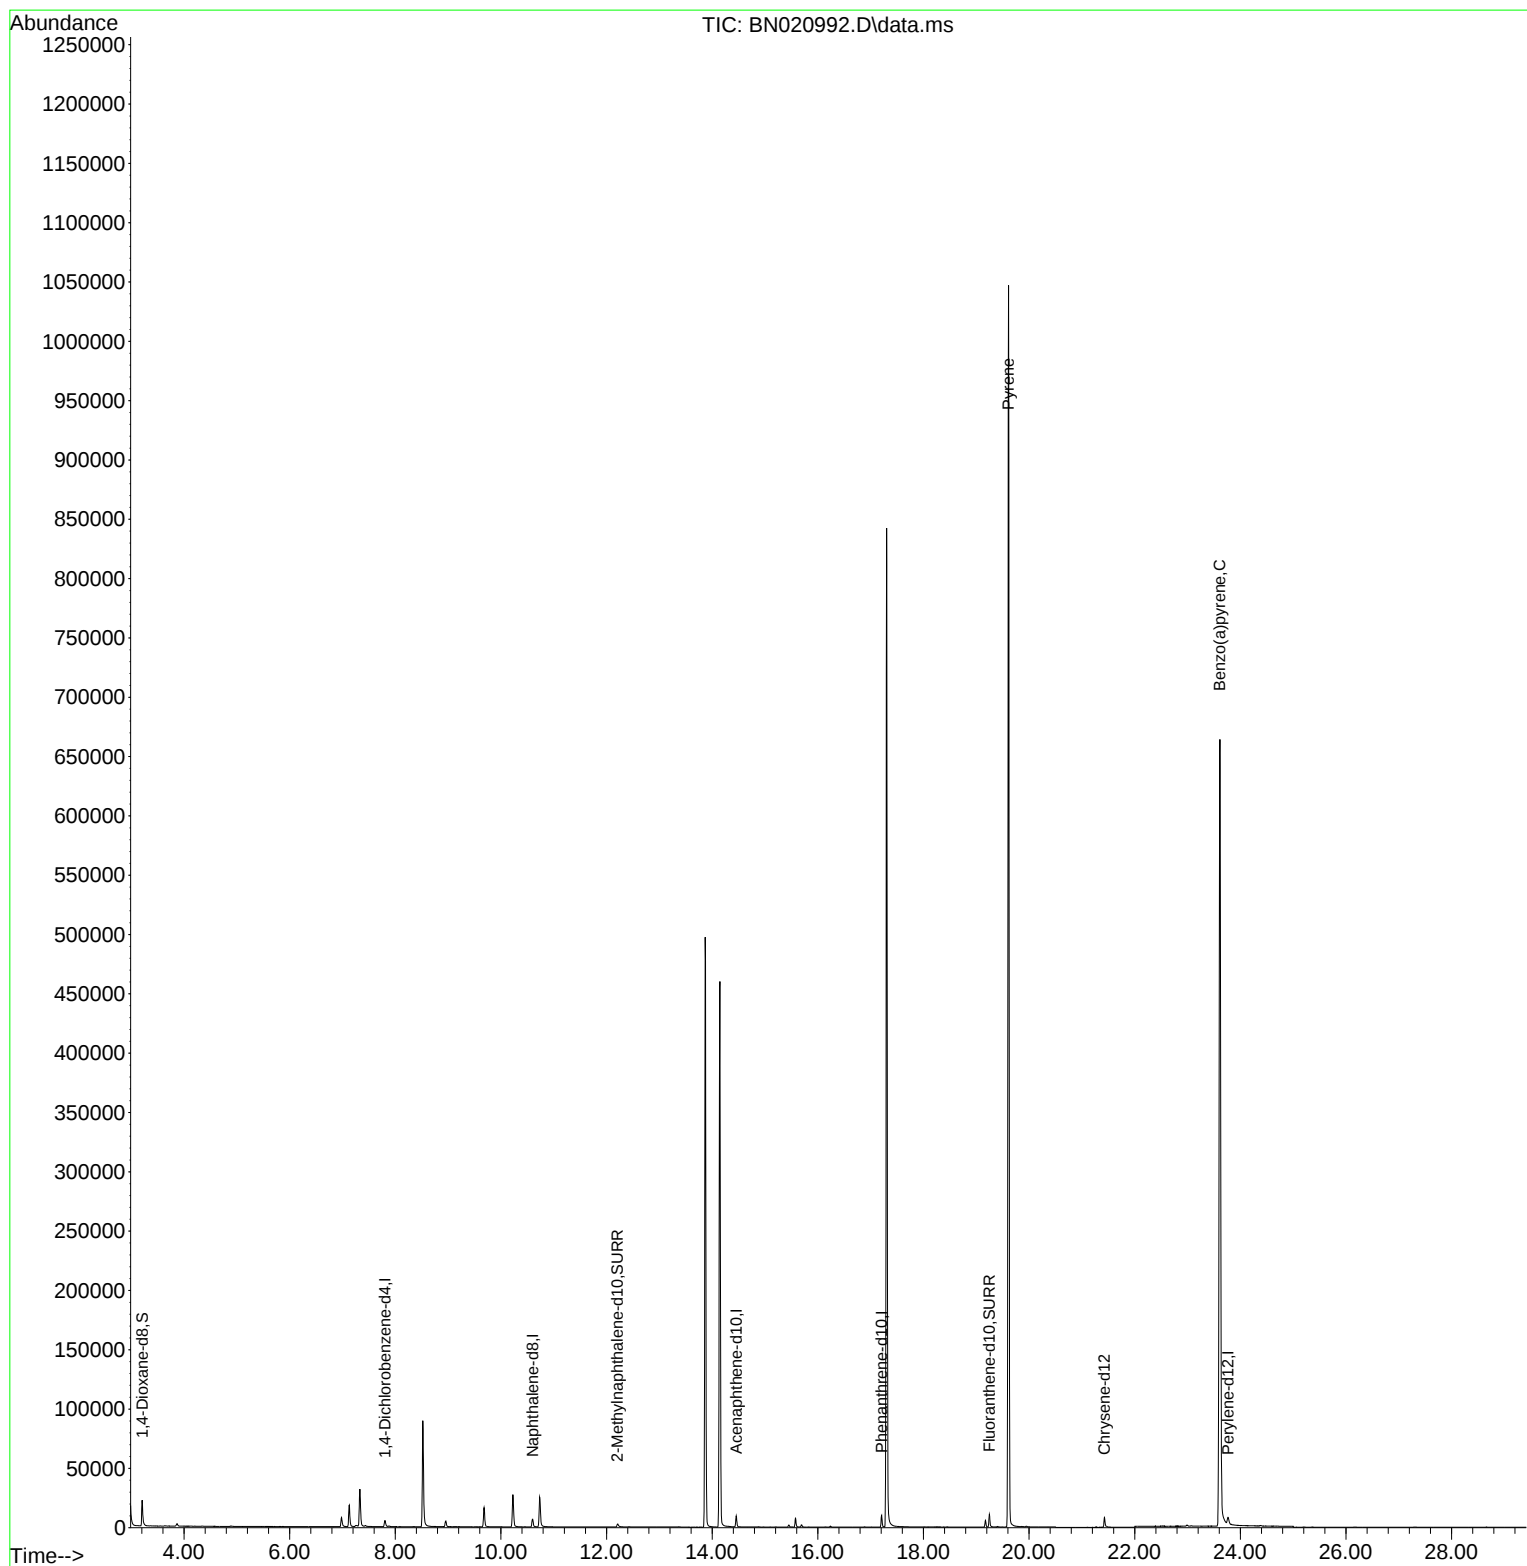



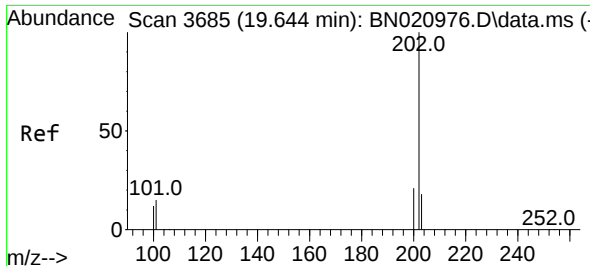


#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.611 min Scan# 30
Delta R.T. -0.033 min
Lab File: BN020992.D
Acq: 04 Aug 2022 16:51

Instrument :
BNA_N
ClientSampleId :

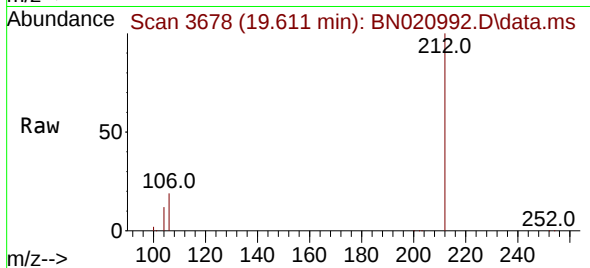

Tgt Ion:202 Resp: 1710
Ion Ratio Lower Upper
202 100
101 179.4 11.3 16.9#
100 1312.4 9.0 13.4#

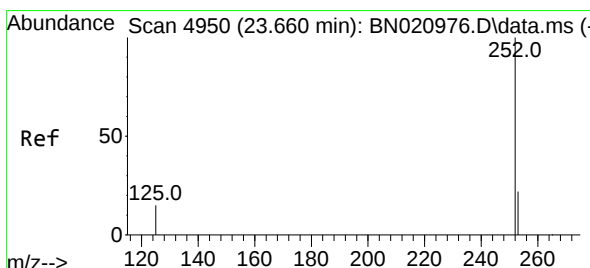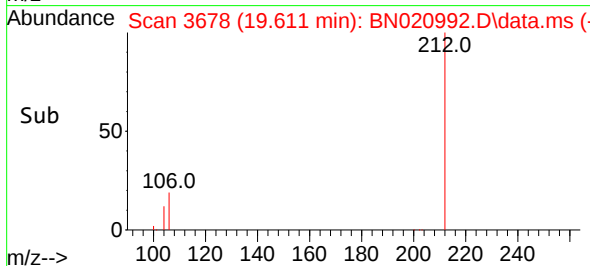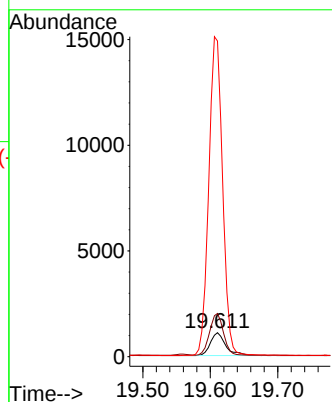

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.609 min Scan# 4933
Delta R.T. -0.051 min
Lab File: BN020992.D
Acq: 04 Aug 2022 16:51

Tgt Ion:252 Resp: 3488
Ion Ratio Lower Upper
252 100
253 42.8 22.1 33.1#
125 34.0 14.7 22.1#

