

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020994.D
 Acq On : 04 Aug 2022 18:07
 Operator : CG/JU
 Sample : PB146574BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:22:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2853	0.400	ng/ul	0.00
4) Naphthalene-d8	10.602	136	11369	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	6817	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.210	188	13431	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	9826	0.400	ng/ul	0.00
23) Perylene-d12	23.763	264	11363	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	23960	6.564	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	4856	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	10751	0.354	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.612	202	1514	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.605	252	3365	0.070	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020994.D
Acq On : 04 Aug 2022 18:07
Operator : CG/JU
Sample : PB146574BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 05 01:22:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

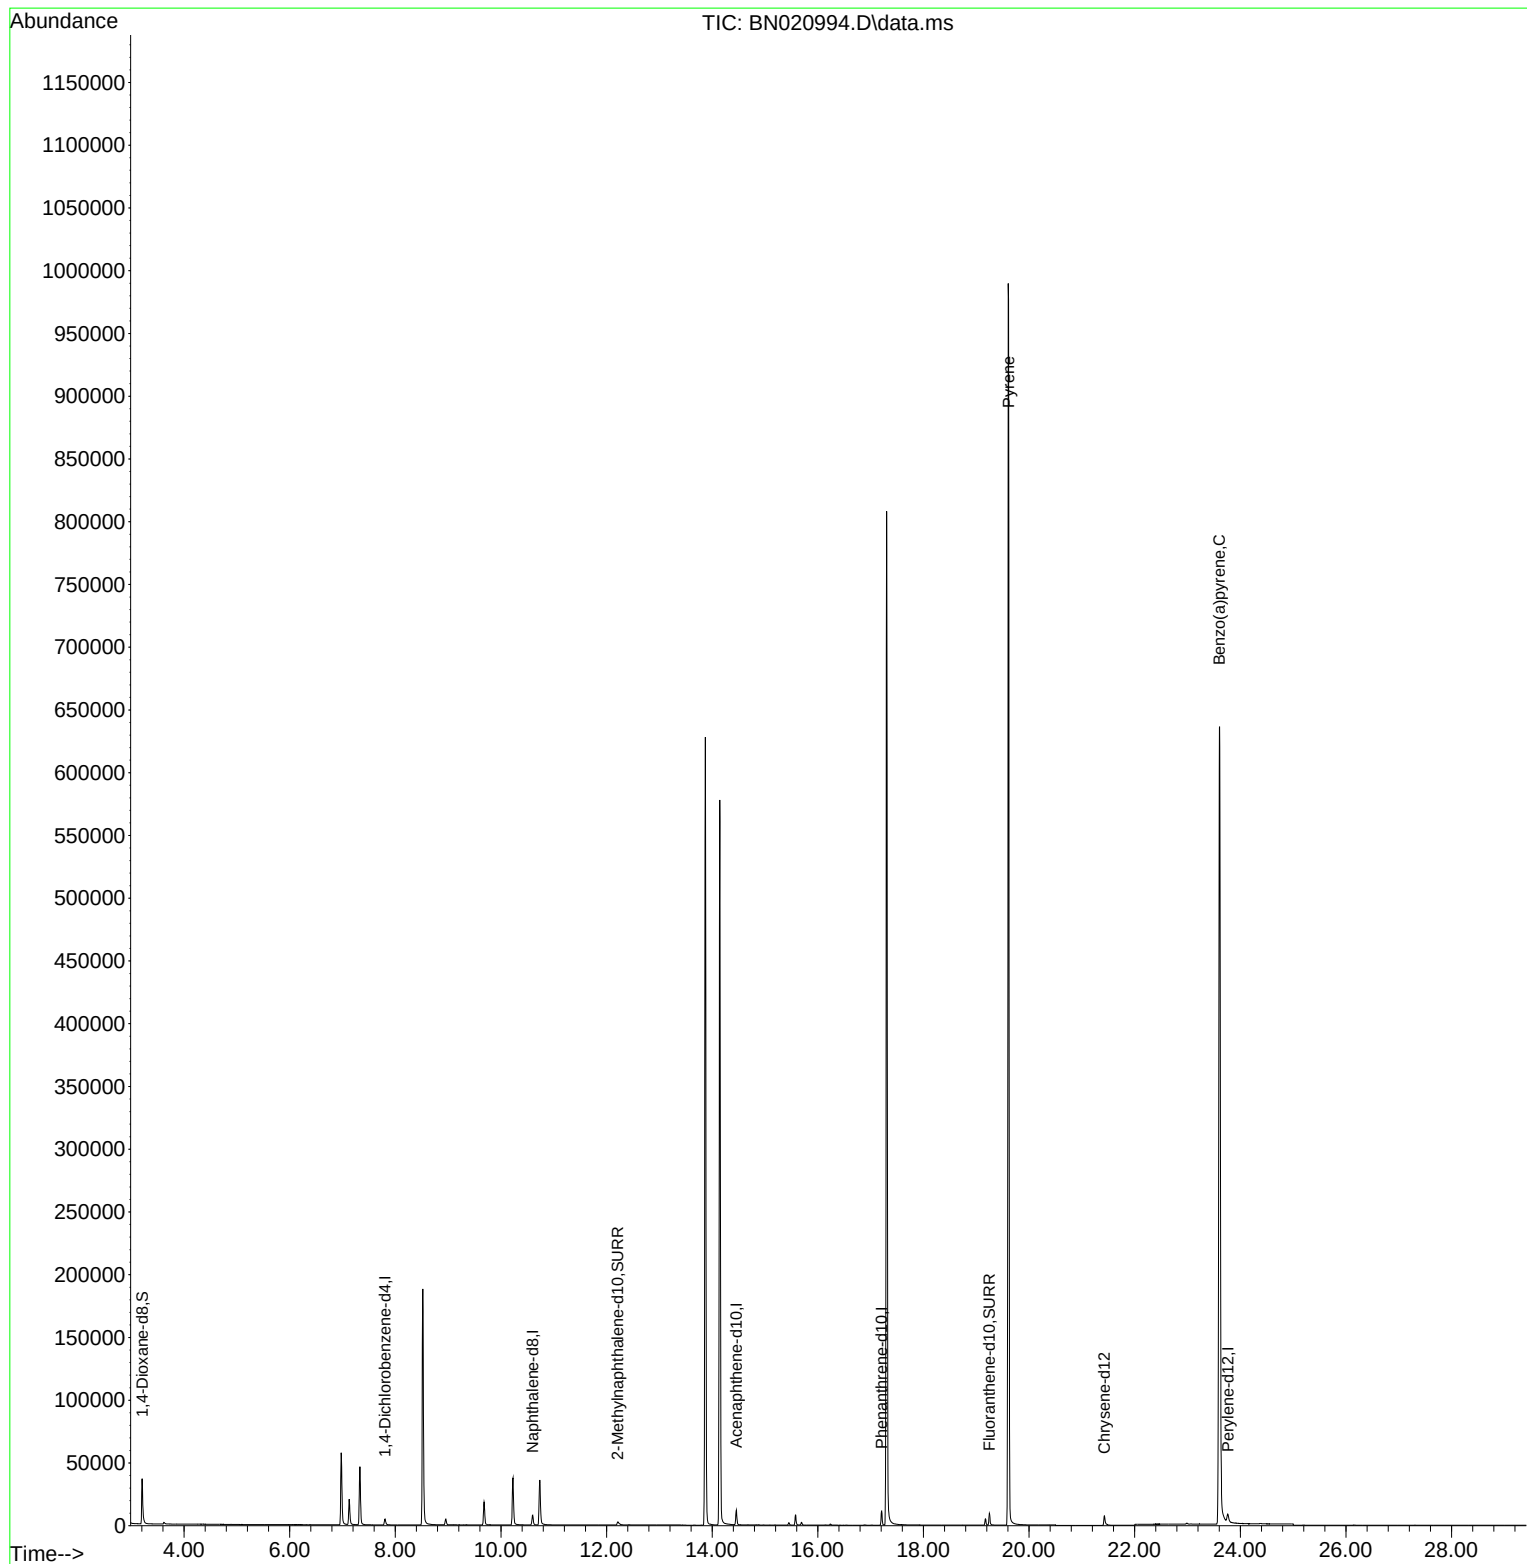



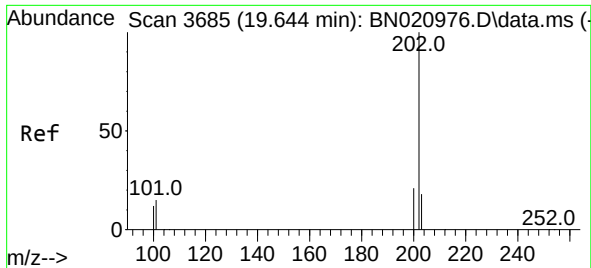


#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.612 min Scan# 3099
Delta R.T. -0.032 min
Lab File: BN020994.D
Acq: 04 Aug 2022 18:07

Instrument :
BNA_N
ClientSampleId :

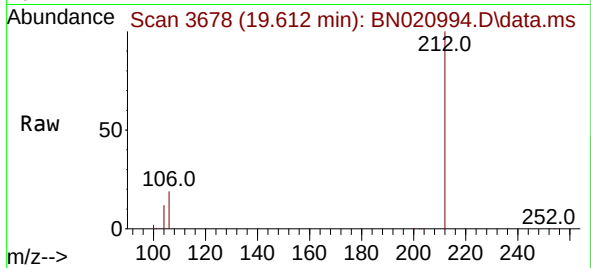

Tgt Ion:202 Resp: 1514
Ion Ratio Lower Upper
202 100
101 175.7 11.3 16.9#
100 1278.3 9.0 13.4#

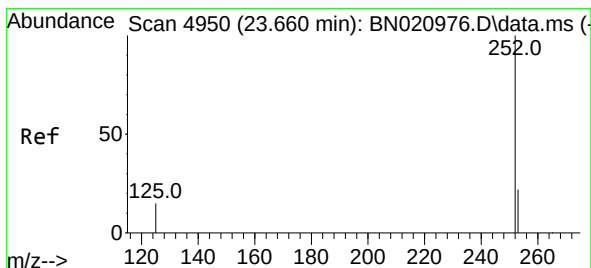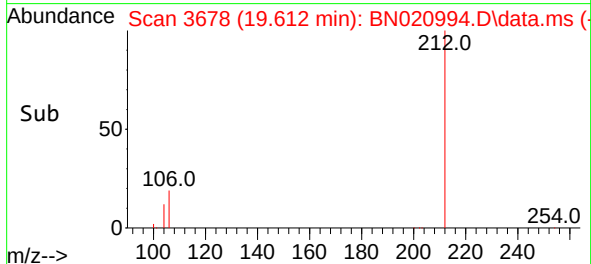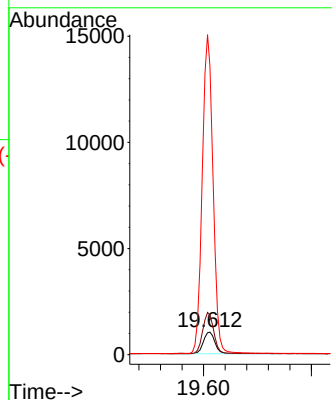

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.605 min Scan# 4931
Delta R.T. -0.055 min
Lab File: BN020994.D
Acq: 04 Aug 2022 18:07

Tgt Ion:252 Resp: 3365
Ion Ratio Lower Upper
252 100
253 41.8 22.1 33.1#
125 34.2 14.7 22.1#

