

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020995.D
 Acq On : 04 Aug 2022 18:45
 Operator : CG/JU
 Sample : PB146568BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:22:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2357	0.400	ng/ul	0.00
4) Naphthalene-d8	10.600	136	7355	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.455	164	4303	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.208	188	8300	0.400	ng/ul	0.00
17) Chrysene-d12	21.430	240	6094	0.400	ng/ul	0.01
23) Perylene-d12	23.769	264	7055	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	17756	5.888	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152	3485	0.323	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	7561	0.402	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.450	166	1233	0.068	ng/ul#	16
20) Pyrene	19.610	202	1071	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.611	252	2363	0.079	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020995.D
Acq On : 04 Aug 2022 18:45
Operator : CG/JU
Sample : PB146568BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 05 01:22:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

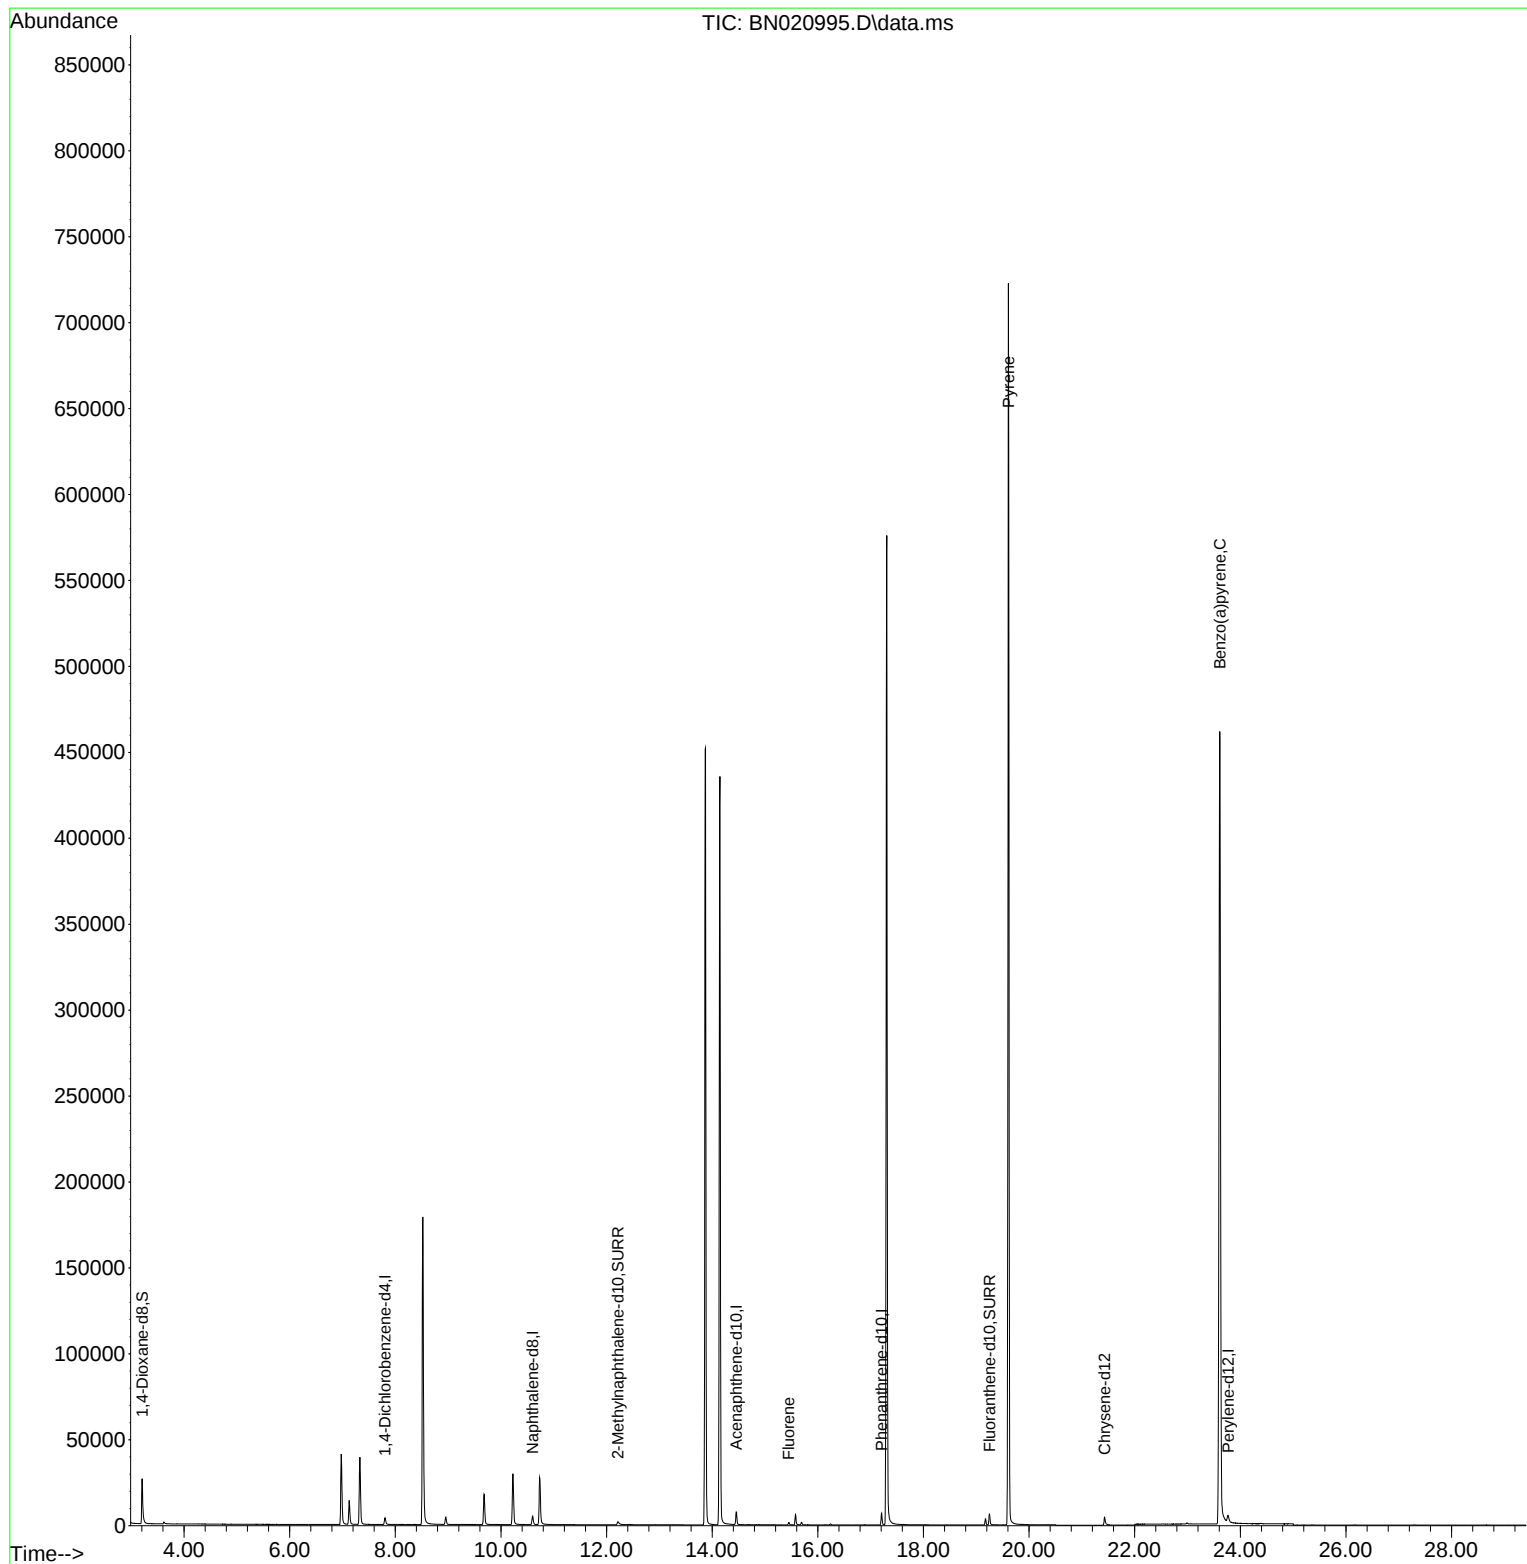



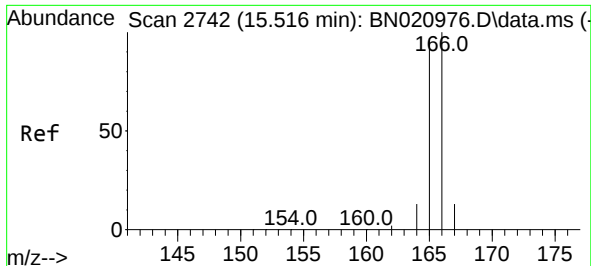


#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.450 min Scan# 21
Delta R.T. -0.066 min
Lab File: BN020995.D
Acq: 04 Aug 2022 18:45

Instrument :
BNA_N
ClientSampleId :



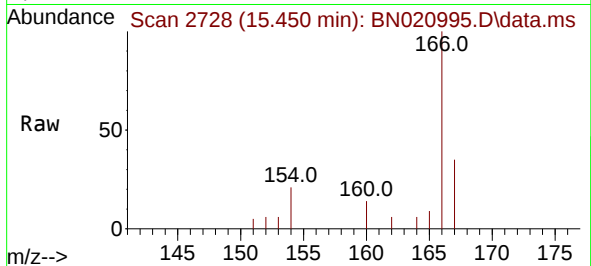



Tgt Ion:166 Resp: 1233
Ion Ratio Lower Upper
166 100
165 9.5 78.6 117.8#
167 35.1 11.8 17.6#

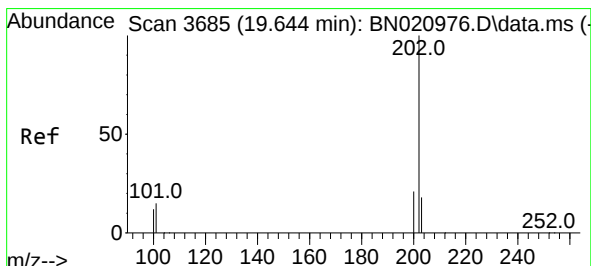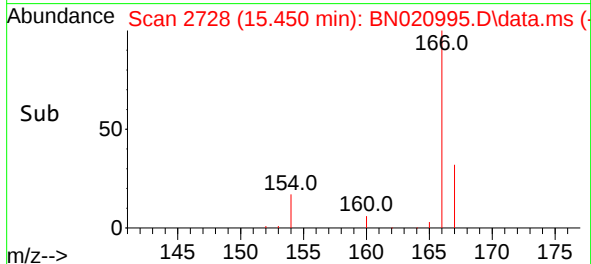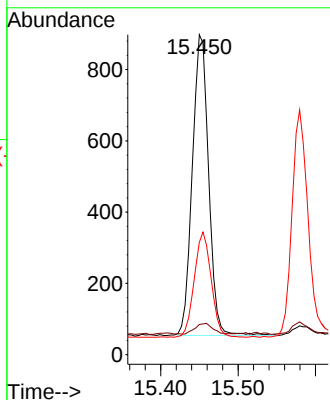

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.610 min Scan# 3678
Delta R.T. -0.034 min
Lab File: BN020995.D
Acq: 04 Aug 2022 18:45


Tgt Ion:202 Resp: 1071
Ion Ratio Lower Upper
202 100
101 180.4 11.3 16.9#
100 1317.2 9.0 13.4#

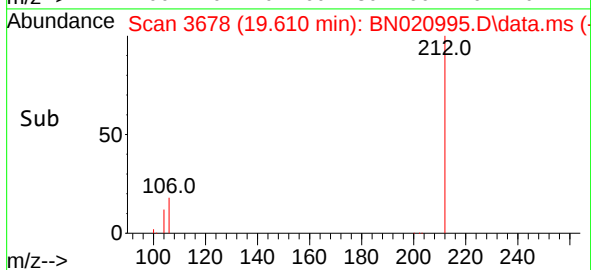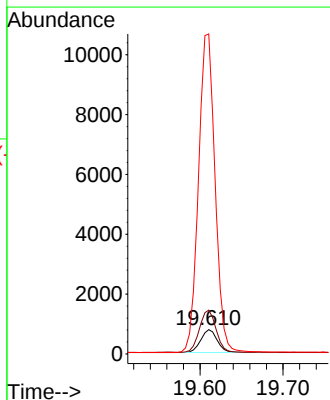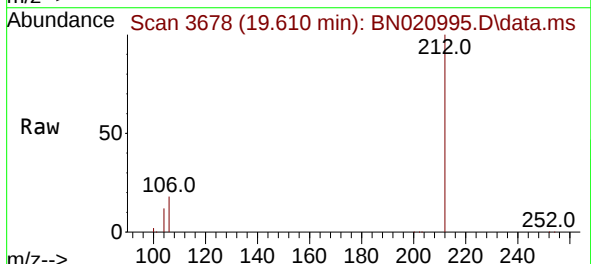

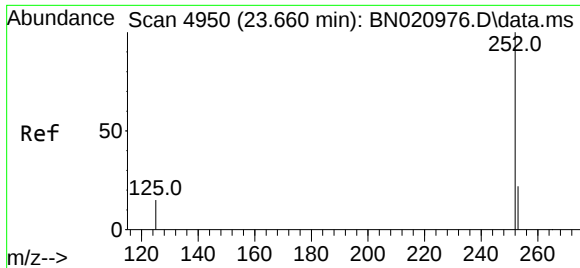

#26
 Benzo(a)pyrene
 Concen: 0.079 ng/ul
 RT: 23.611 min Scan# 4933
 Delta R.T. -0.049 min
 Lab File: BN020995.D
 Acq: 04 Aug 2022 18:45

Instrument :
 BNA_N
 ClientSampleId :

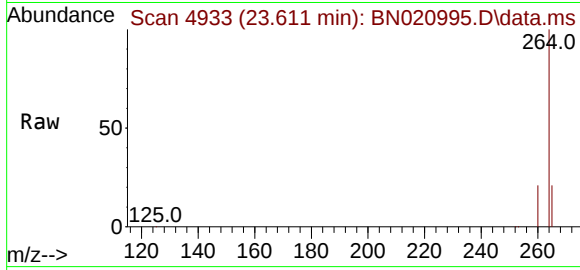

Tgt Ion:	252	Resp:	2363
Ion	Ratio	Lower	Upper
252	100		
253	45.2	22.1	33.1#
125	35.8	14.7	22.1#

