

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021002.D
 Acq On : 04 Aug 2022 23:11
 Operator : CG/JU
 Sample : N3900-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:22:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2856	0.400	ng/ul	0.00
4) Naphthalene-d8	10.596	136	9087	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164	5348	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.206	188	10549	0.400	ng/ul	0.00
17) Chrysene-d12	21.415	240	8717	0.400	ng/ul	0.00
23) Perylene-d12	23.751	264	9700	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	12655	3.464	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	3785	0.284	ng/ul	0.00
18) Fluoranthene-d10	19.245	212	9998	0.371	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	1615	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.593	252	3278	0.080	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021002.D
Acq On : 04 Aug 2022 23:11
Operator : CG/JU
Sample : N3900-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 05 01:22:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

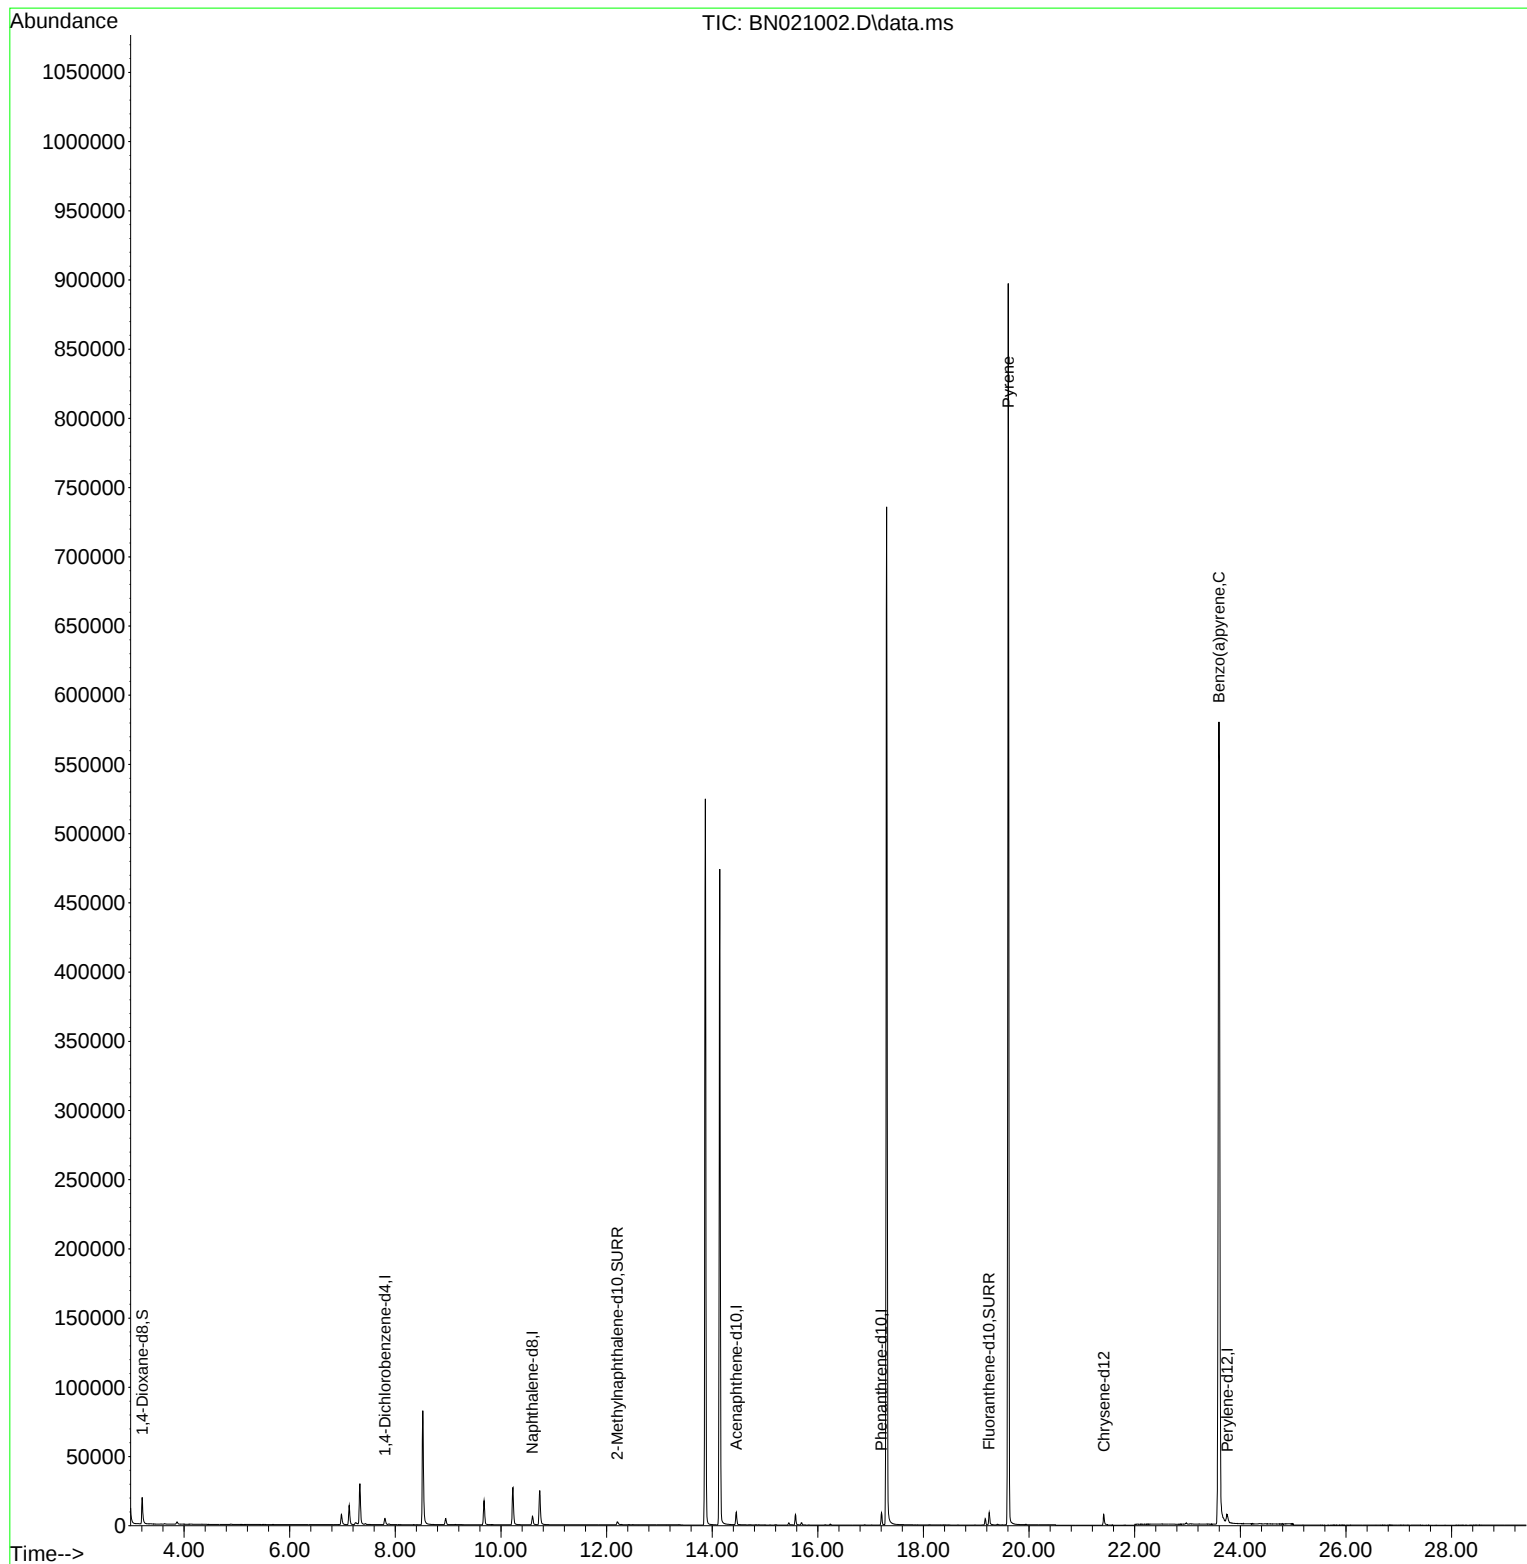



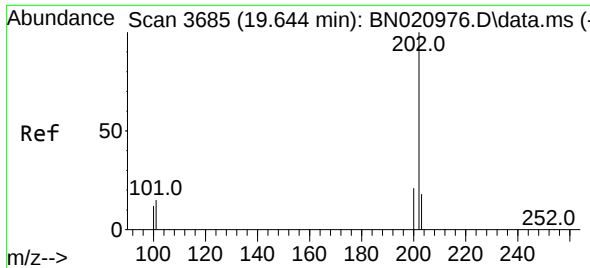


#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.607 min Scan# 3677
Delta R.T. -0.037 min
Lab File: BN021002.D
Acq: 04 Aug 2022 23:11

Instrument :
BNA_N
ClientSampleId :

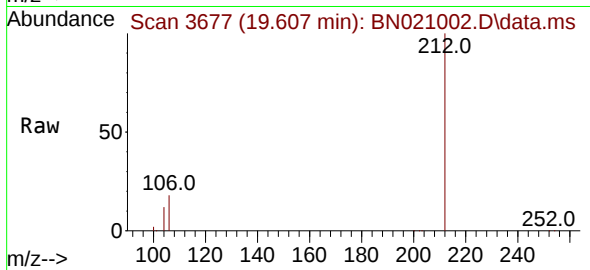

Tgt Ion:202 Resp: 1615
Ion Ratio Lower Upper
202 100
101 179.7 11.3 16.9#
100 1301.5 9.0 13.4#

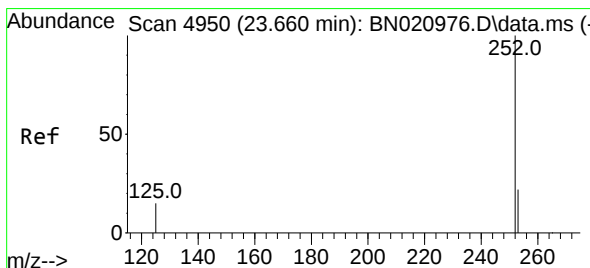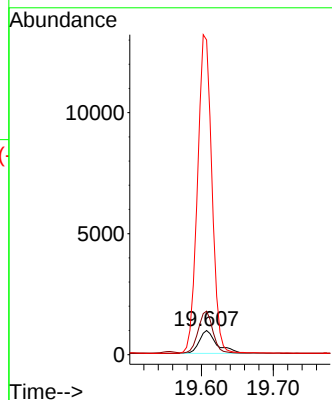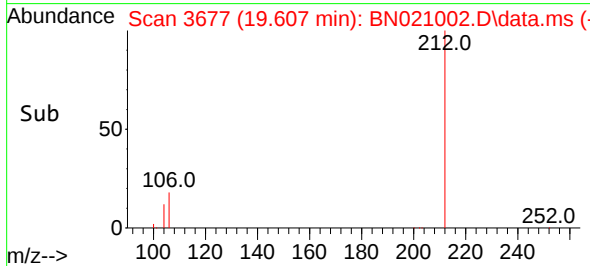

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.593 min Scan# 4927
Delta R.T. -0.067 min
Lab File: BN021002.D
Acq: 04 Aug 2022 23:11

Tgt Ion:252 Resp: 3278
Ion Ratio Lower Upper
252 100
253 42.8 22.1 33.1#
125 36.1 14.7 22.1#

