

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021003.D
 Acq On : 04 Aug 2022 23:48
 Operator : CG/JU
 Sample : N3900-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 05 01:22:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	2772	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.596	136	8815	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164	4850	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.205	188	9774	0.400	ng/ul	0.00
17) Chrysene-d12	21.415	240	8481	0.400	ng/ul	0.00
23) Perylene-d12	23.751	264	11192	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	17301	4.879	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	3805	0.295	ng/ul	0.00
18) Fluoranthene-d10	19.245	212	10388	0.397	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	1381	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.599	252	3658	0.077	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021003.D
Acq On : 04 Aug 2022 23:48
Operator : CG/JU
Sample : N3900-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 05 01:22:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration




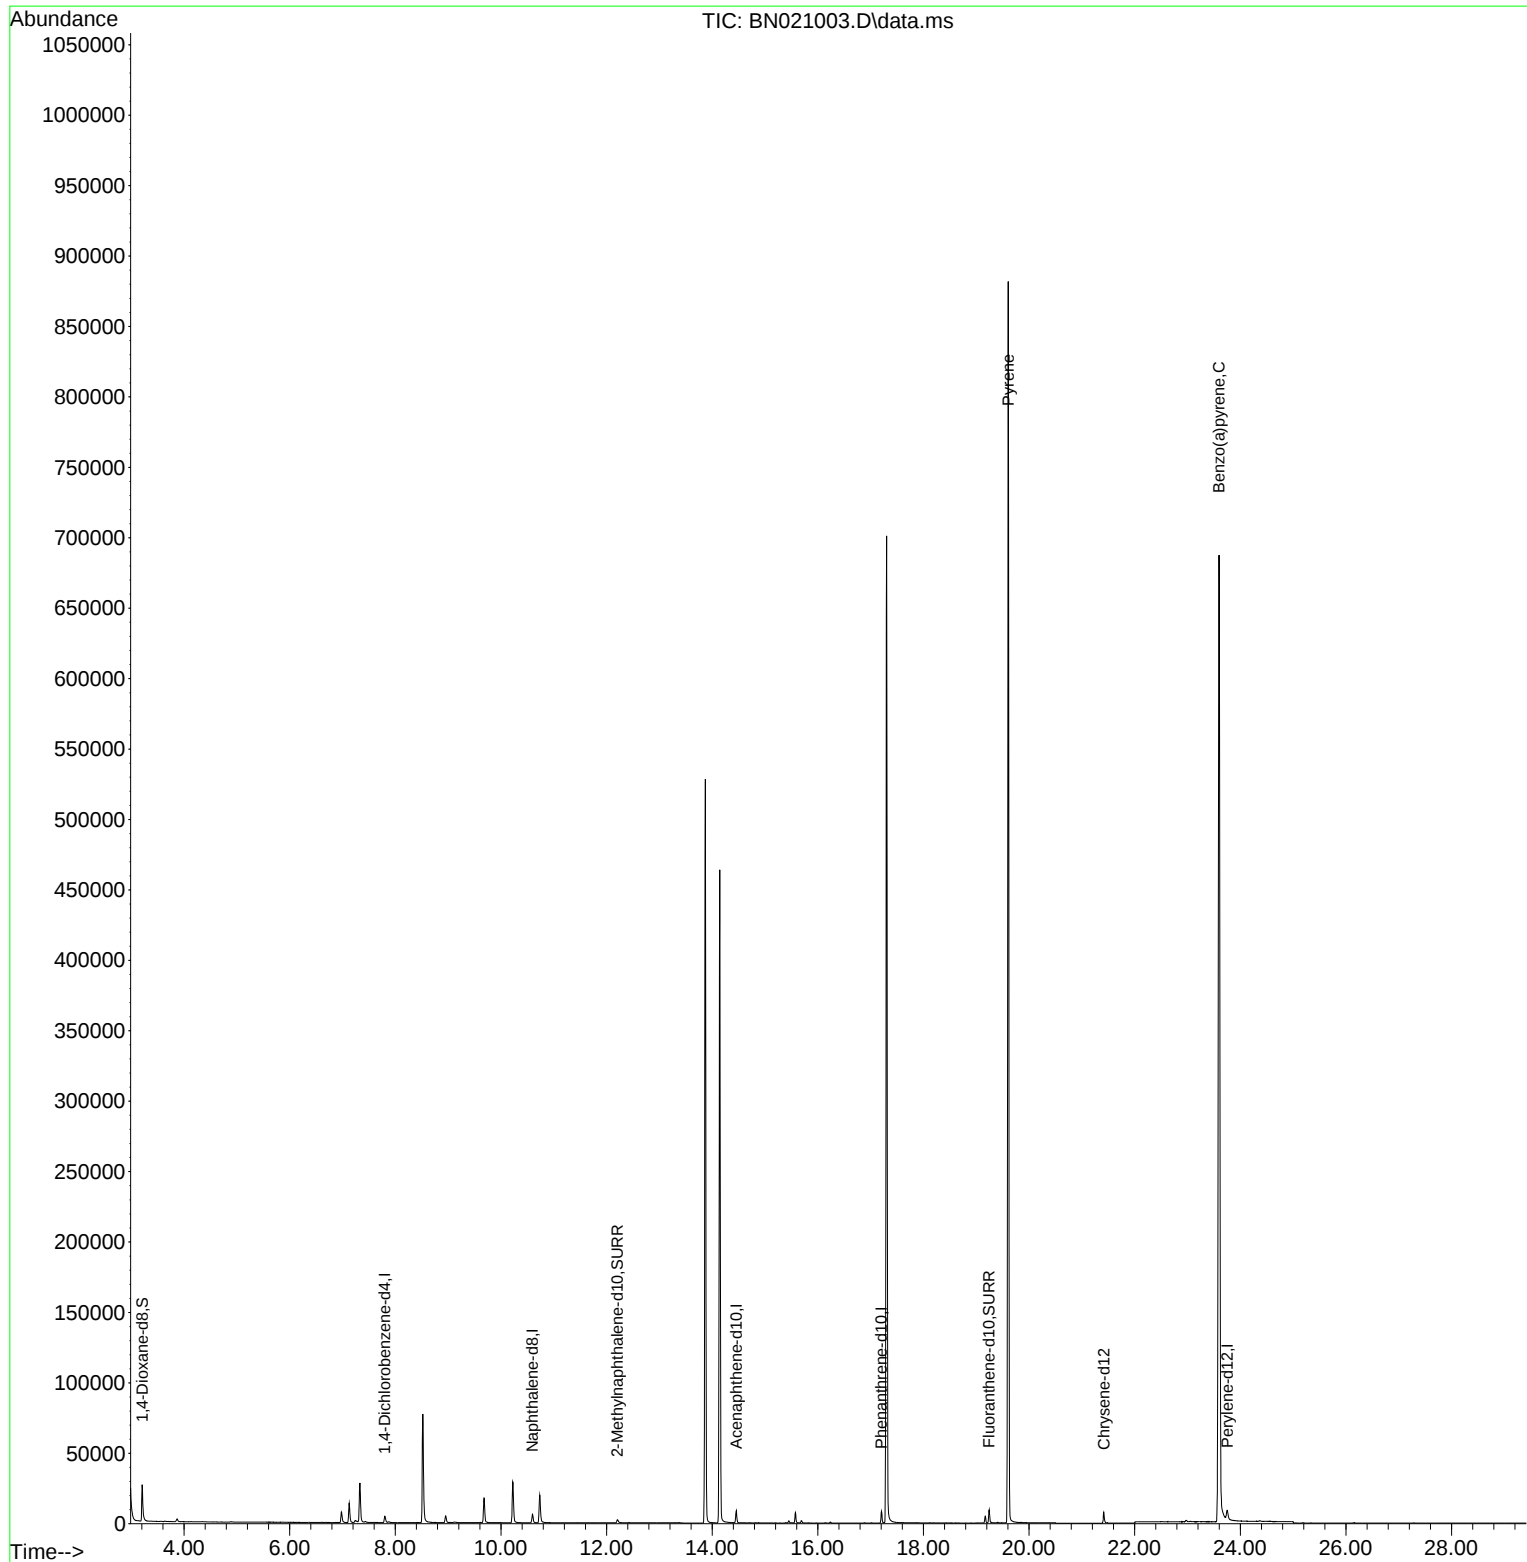


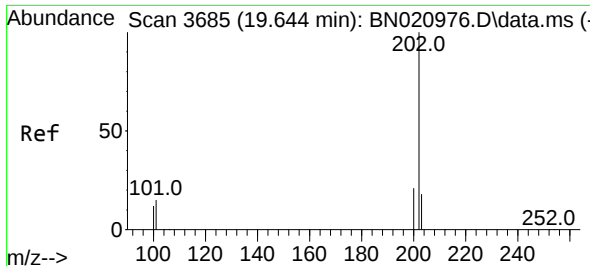

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.607 min Scan# 30
Delta R.T. -0.037 min
Lab File: BN021003.D
Acq: 04 Aug 2022 23:48

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1381
Ion Ratio Lower Upper
202 100
101 179.4 11.3 16.9#
100 1297.1 9.0 13.4#

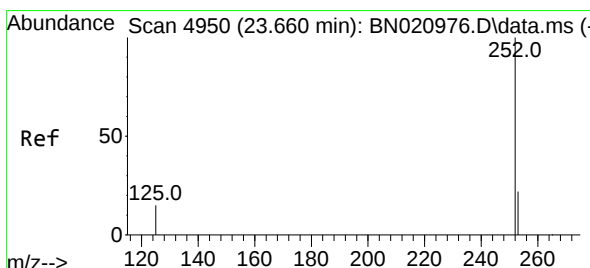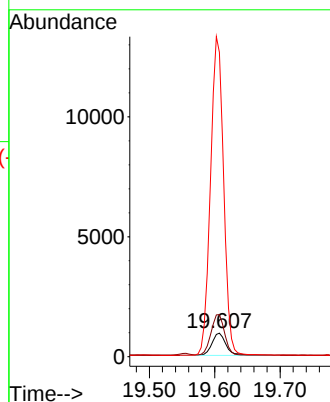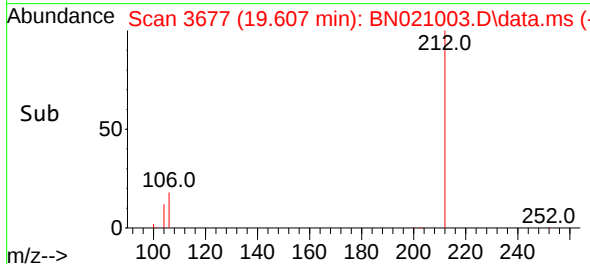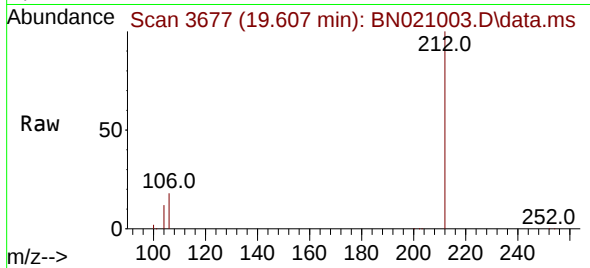

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.599 min Scan# 4929
Delta R.T. -0.061 min
Lab File: BN021003.D
Acq: 04 Aug 2022 23:48

Tgt Ion:252 Resp: 3658
Ion Ratio Lower Upper
252 100
253 44.1 22.1 33.1#
125 34.1 14.7 22.1#

