

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021031.D
 Acq On : 05 Aug 2022 17:47
 Operator : CG/JU
 Sample : N3951-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 06 00:28:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	2779	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.592	136	9141	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.454	164	5280	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.202	188	10560	0.400	ng/ul	0.00
17) Chrysene-d12	21.417	240	8717	0.400	ng/ul	0.00
23) Perylene-d12	23.749	264	9194	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.208	96	12963	3.646	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.204	152	4310	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.246	212	10615	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.608	202	1662	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.597	252	3190	0.082	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021031.D
Acq On : 05 Aug 2022 17:47
Operator : CG/JU
Sample : N3951-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 06 00:28:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

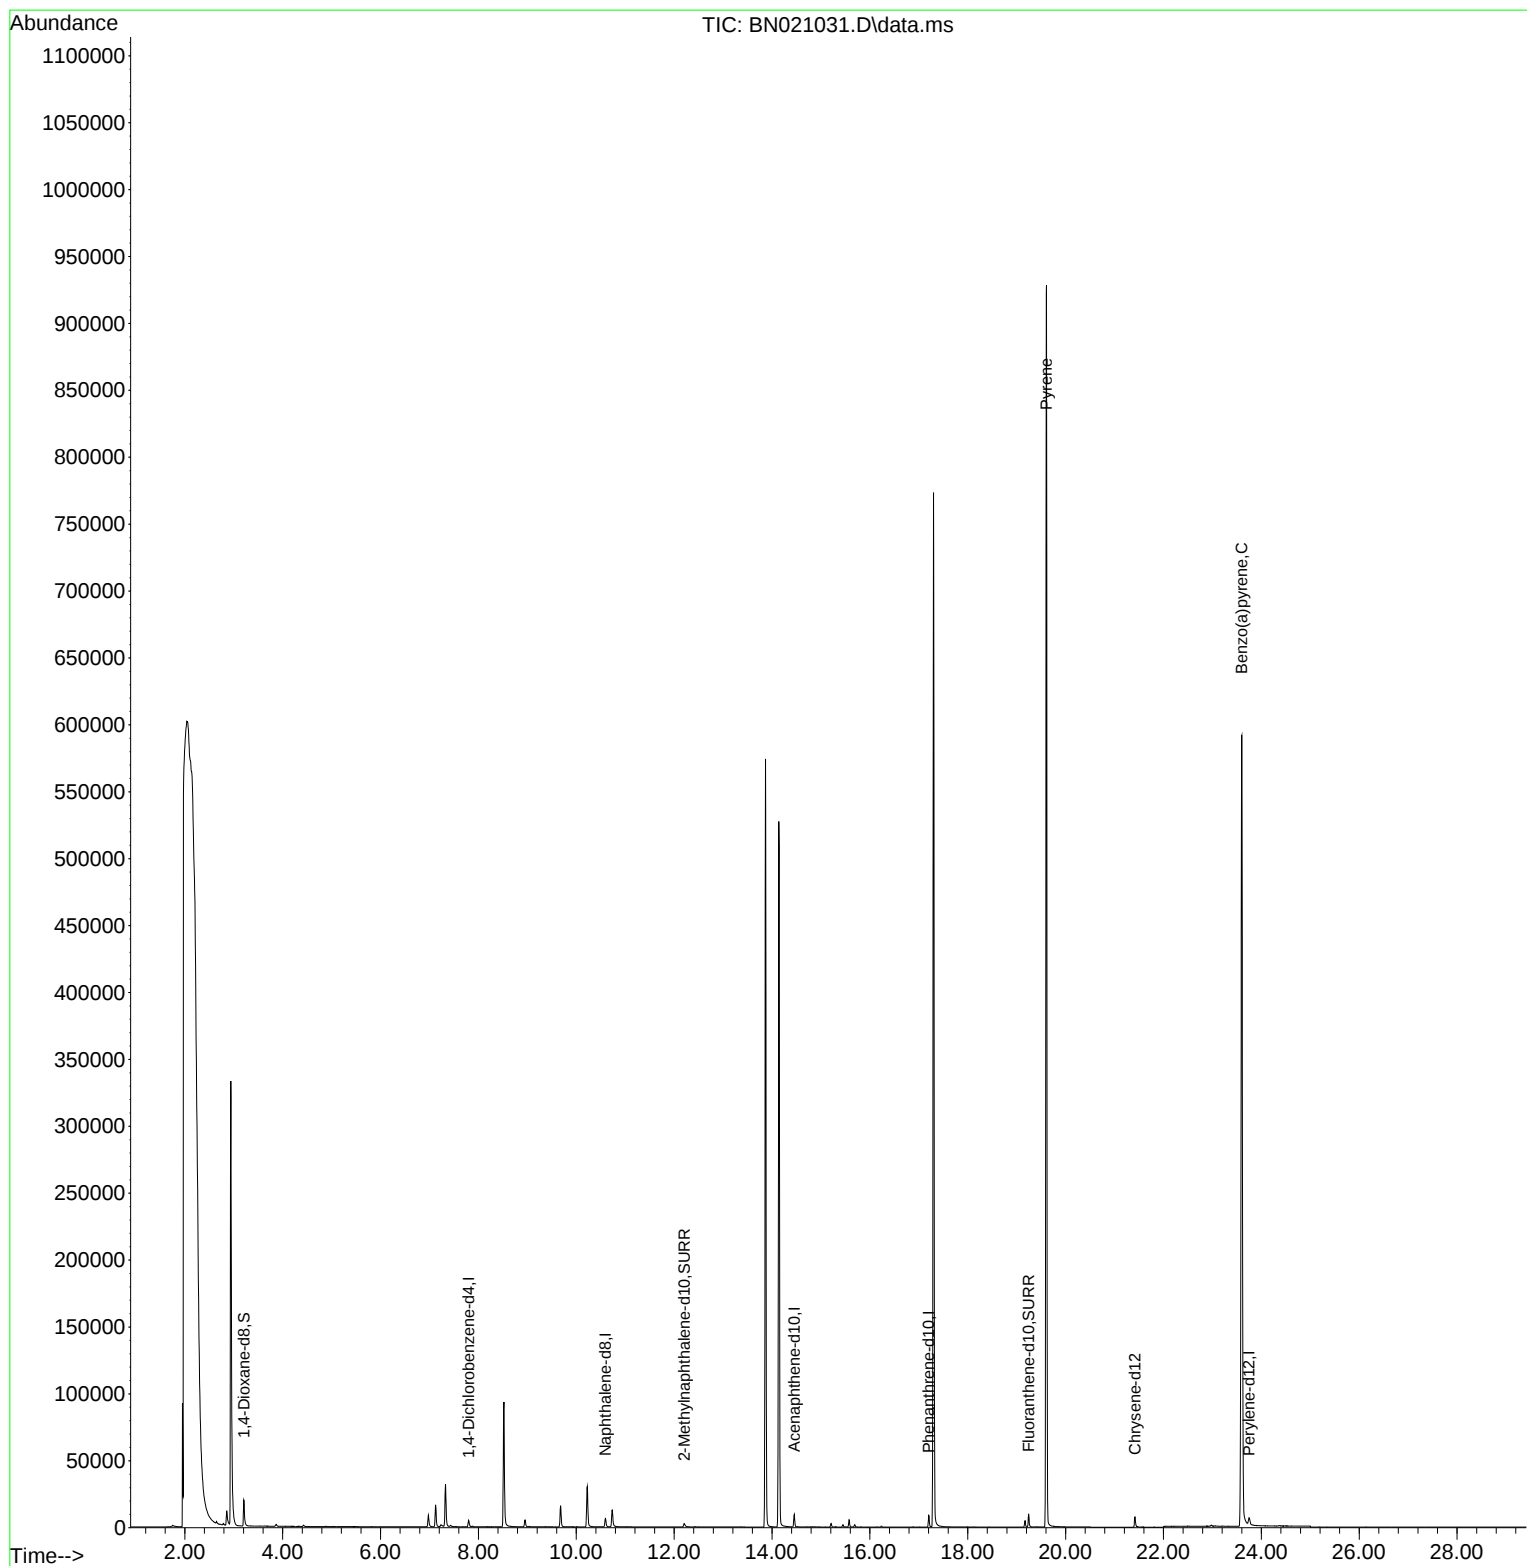



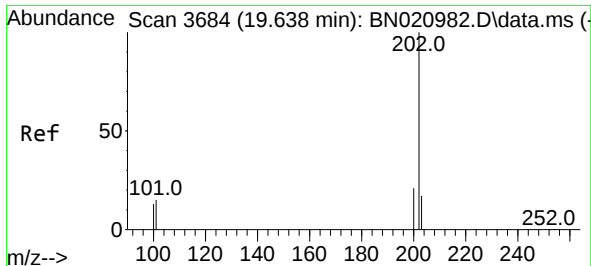


#20
Pyrene
Concen: 0.042 ng/u1
RT: 19.608 min Scan# 41
Delta R.T. -0.036 min
Lab File: BN021031.D
Acq: 05 Aug 2022 17:47


Instrument :
BNA_N
ClientSampleId :

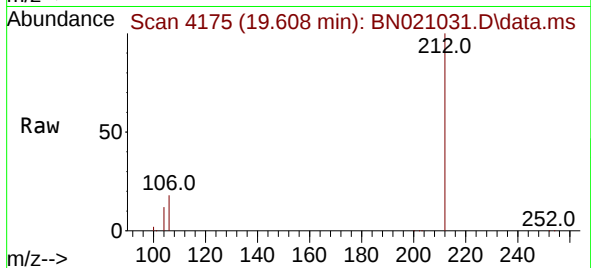

Tgt Ion:202 Resp: 1662
Ion Ratio Lower Upper
202 100
101 172.4 11.3 16.9#
100 1224.0 9.0 13.4#

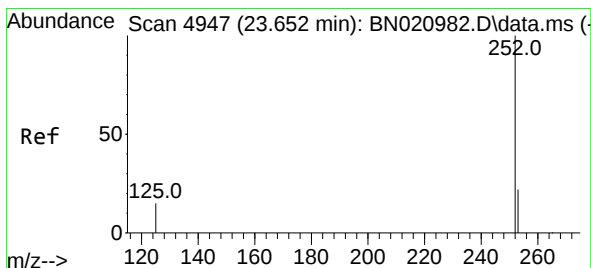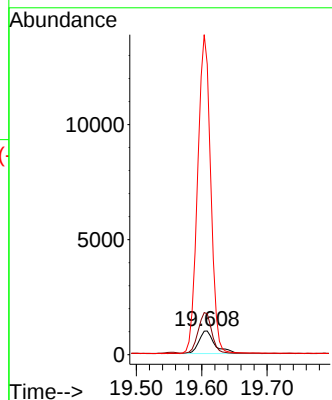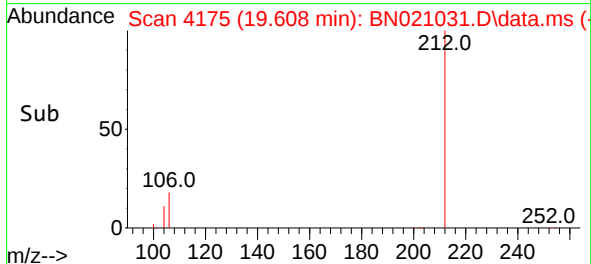

#26
Benzo(a)pyrene
Concen: 0.082 ng/u1
RT: 23.597 min Scan# 5426
Delta R.T. -0.063 min
Lab File: BN021031.D
Acq: 05 Aug 2022 17:47

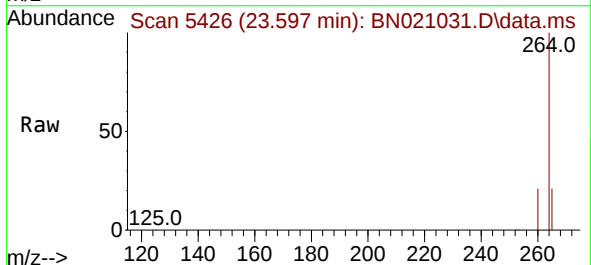

Tgt Ion:252 Resp: 3190
Ion Ratio Lower Upper
252 100
253 43.3 22.1 33.1#
125 33.3 14.7 22.1#

