

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021034.D
 Acq On : 05 Aug 2022 19:40
 Operator : CG/JU
 Sample : N3952-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 06 00:28:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	2599	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.596	136	8481	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.452	164	4728	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.205	188	9319	0.400	ng/ul	0.00
17) Chrysene-d12	21.415	240	7627	0.400	ng/ul	0.00
23) Perylene-d12	23.751	264	8058	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	11671	3.510	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	4102	0.330	ng/ul	0.00
18) Fluoranthene-d10	19.245	212	9894	0.420	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	1597	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.599	252	2947	0.087	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021034.D
Acq On : 05 Aug 2022 19:40
Operator : CG/JU
Sample : N3952-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 06 00:28:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

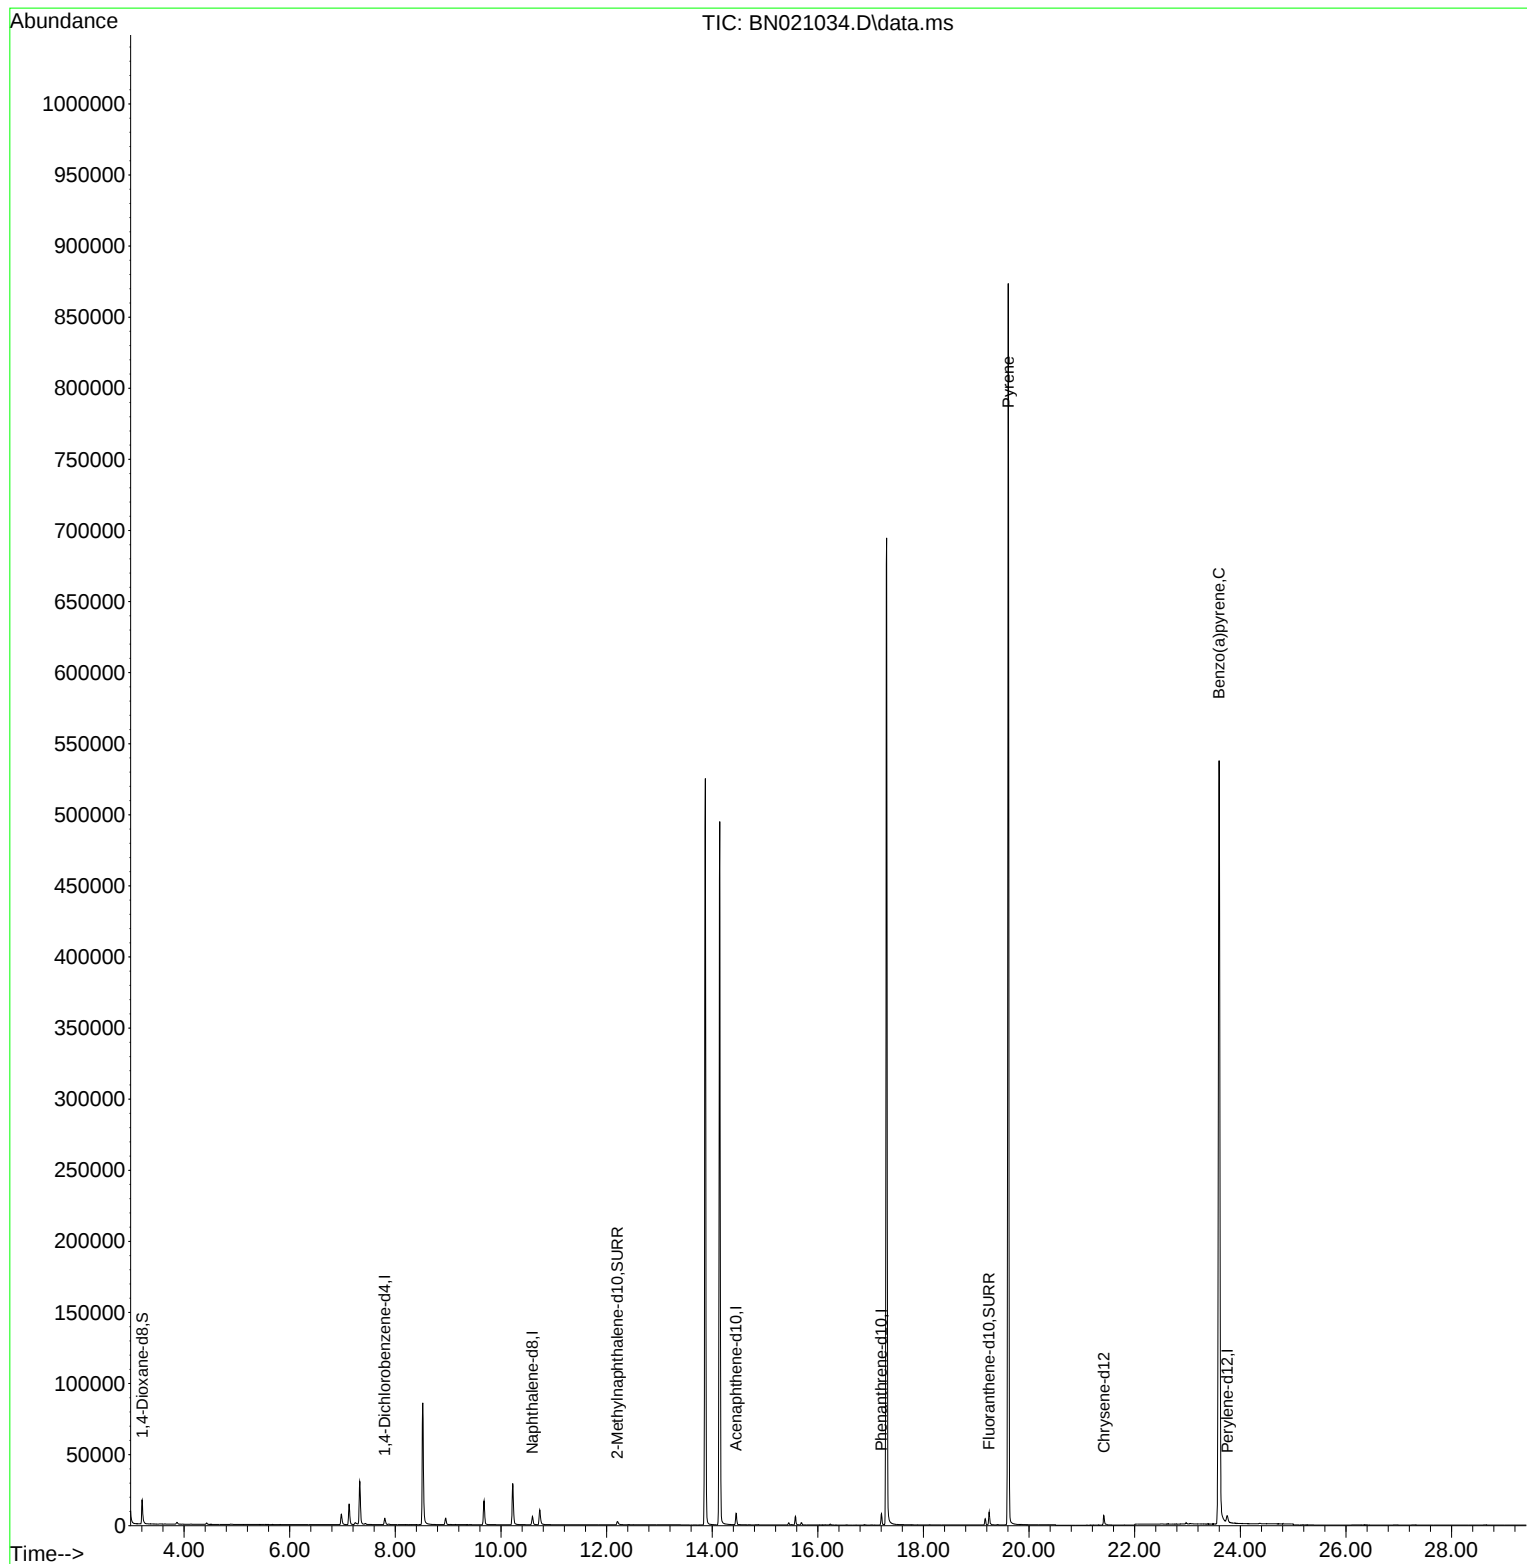

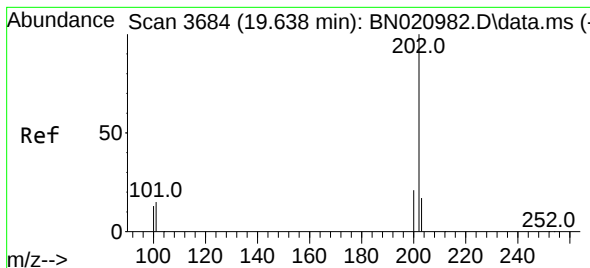

#20

Pyrene

Concen: 0.046 ng/ul

RT: 19.607 min Scan# 30

Delta R.T. -0.037 min

Lab File: BN021034.D

Acq: 05 Aug 2022 19:40





Instrument :

BNA_N

ClientSampleId :

Tgt Ion:202 Resp: 1597

Ion	Ratio	Lower	Upper
202	100		
101	172.5	11.3	16.9#
100	1226.8	9.0	13.4#

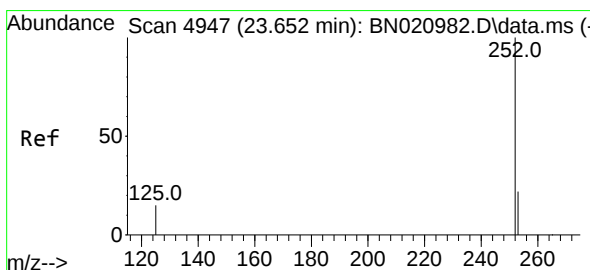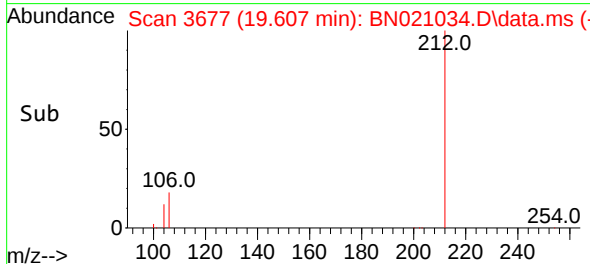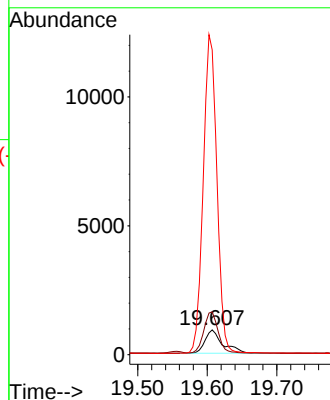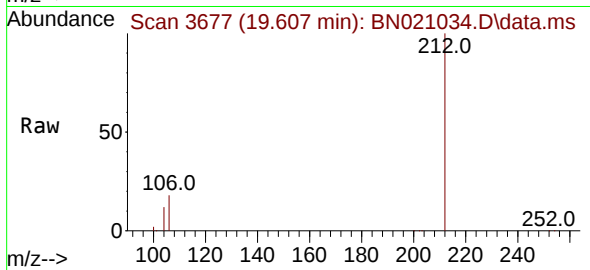

#26

Benzo(a)pyrene

Concen: 0.087 ng/ul

RT: 23.599 min Scan# 4929

Delta R.T. -0.061 min

Lab File: BN021034.D

Acq: 05 Aug 2022 19:40

Tgt Ion:252 Resp: 2947

Ion	Ratio	Lower	Upper
252	100		
253	47.3	22.1	33.1#
125	35.1	14.7	22.1#

