

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020988.D
 Acq On : 04 Aug 2022 14:20
 Operator : CG/JU
 Sample : N3900-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C88

Quant Time: Aug 05 01:21:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2934	0.400	ng/ul	0.00
4) Naphthalene-d8	10.596	136	8997	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164	5592	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.205	188	13535	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	10160	0.400	ng/ul	0.00
23) Perylene-d12	23.763	264	10847	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	18202	4.849	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.202	152	3768	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	12507	0.399	ng/ul	0.00
Target Compounds						
8) 1-Methylnaphthalene	12.494	142	1257	0.075	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020988.D
Acq On : 04 Aug 2022 14:20
Operator : CG/JU
Sample : N3900-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C88


Quant Time: Aug 05 01:21:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

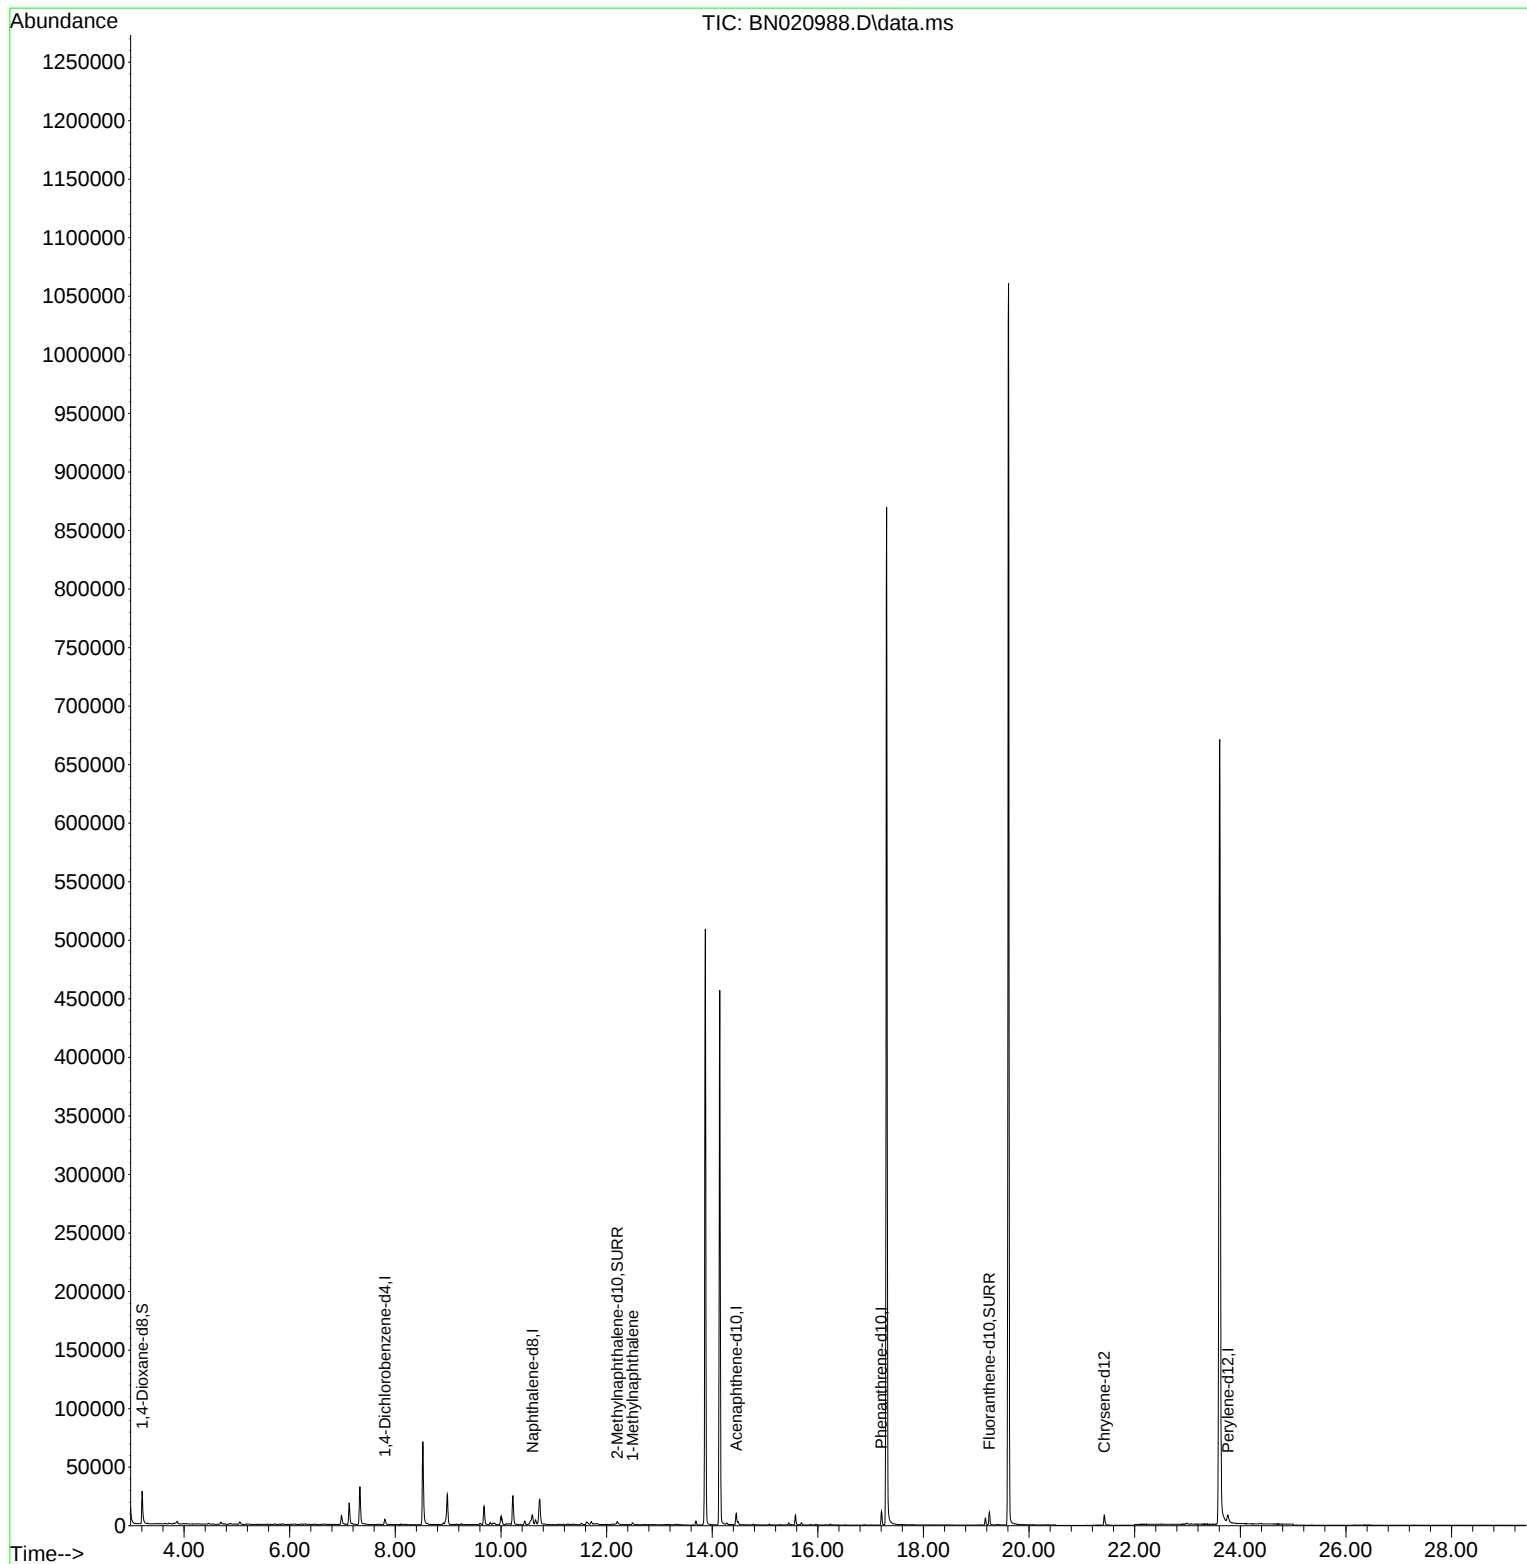

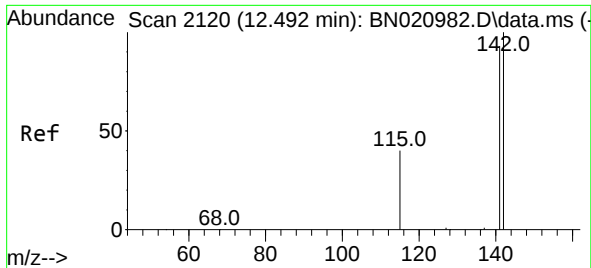

#8
 1-Methylnaphthalene
 Concen: 0.075 ng/ul
 RT: 12.494 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BN020988.D
 Acq: 04 Aug 2022 14:20

Instrument :
 BNA_N
 ClientSampleId :
 C0C88

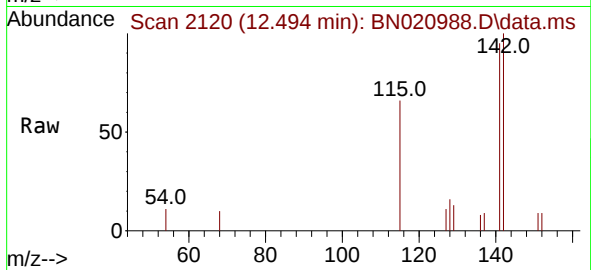

Tgt Ion:142 Resp: 1257
 Ion Ratio Lower Upper
 142 100
 141 94.2 73.9 110.9

