

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN020991.D
 Acq On : 04 Aug 2022 16:13
 Operator : CG/JU
 Sample : N3900-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0CB3

Quant Time: Aug 05 01:21:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	2433	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.596	136	7796	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164	4711	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.206	188	9298	0.400	ng/ul	0.00
17) Chrysene-d12	21.430	240	7375	0.400	ng/ul	0.01
23) Perylene-d12	23.768	264	8104	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	11991	3.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.202	152	4147	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	9912	0.435	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.646	128	552	0.023	ng/ul#	68
7) 2-Methylnaphthalene	12.274	142	666	0.046	ng/ul	99
8) 1-Methylnaphthalene	12.494	142	426	0.029	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN020991.D
Acq On : 04 Aug 2022 16:13
Operator : CG/JU
Sample : N3900-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0CB3

Quant Time: Aug 05 01:21:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

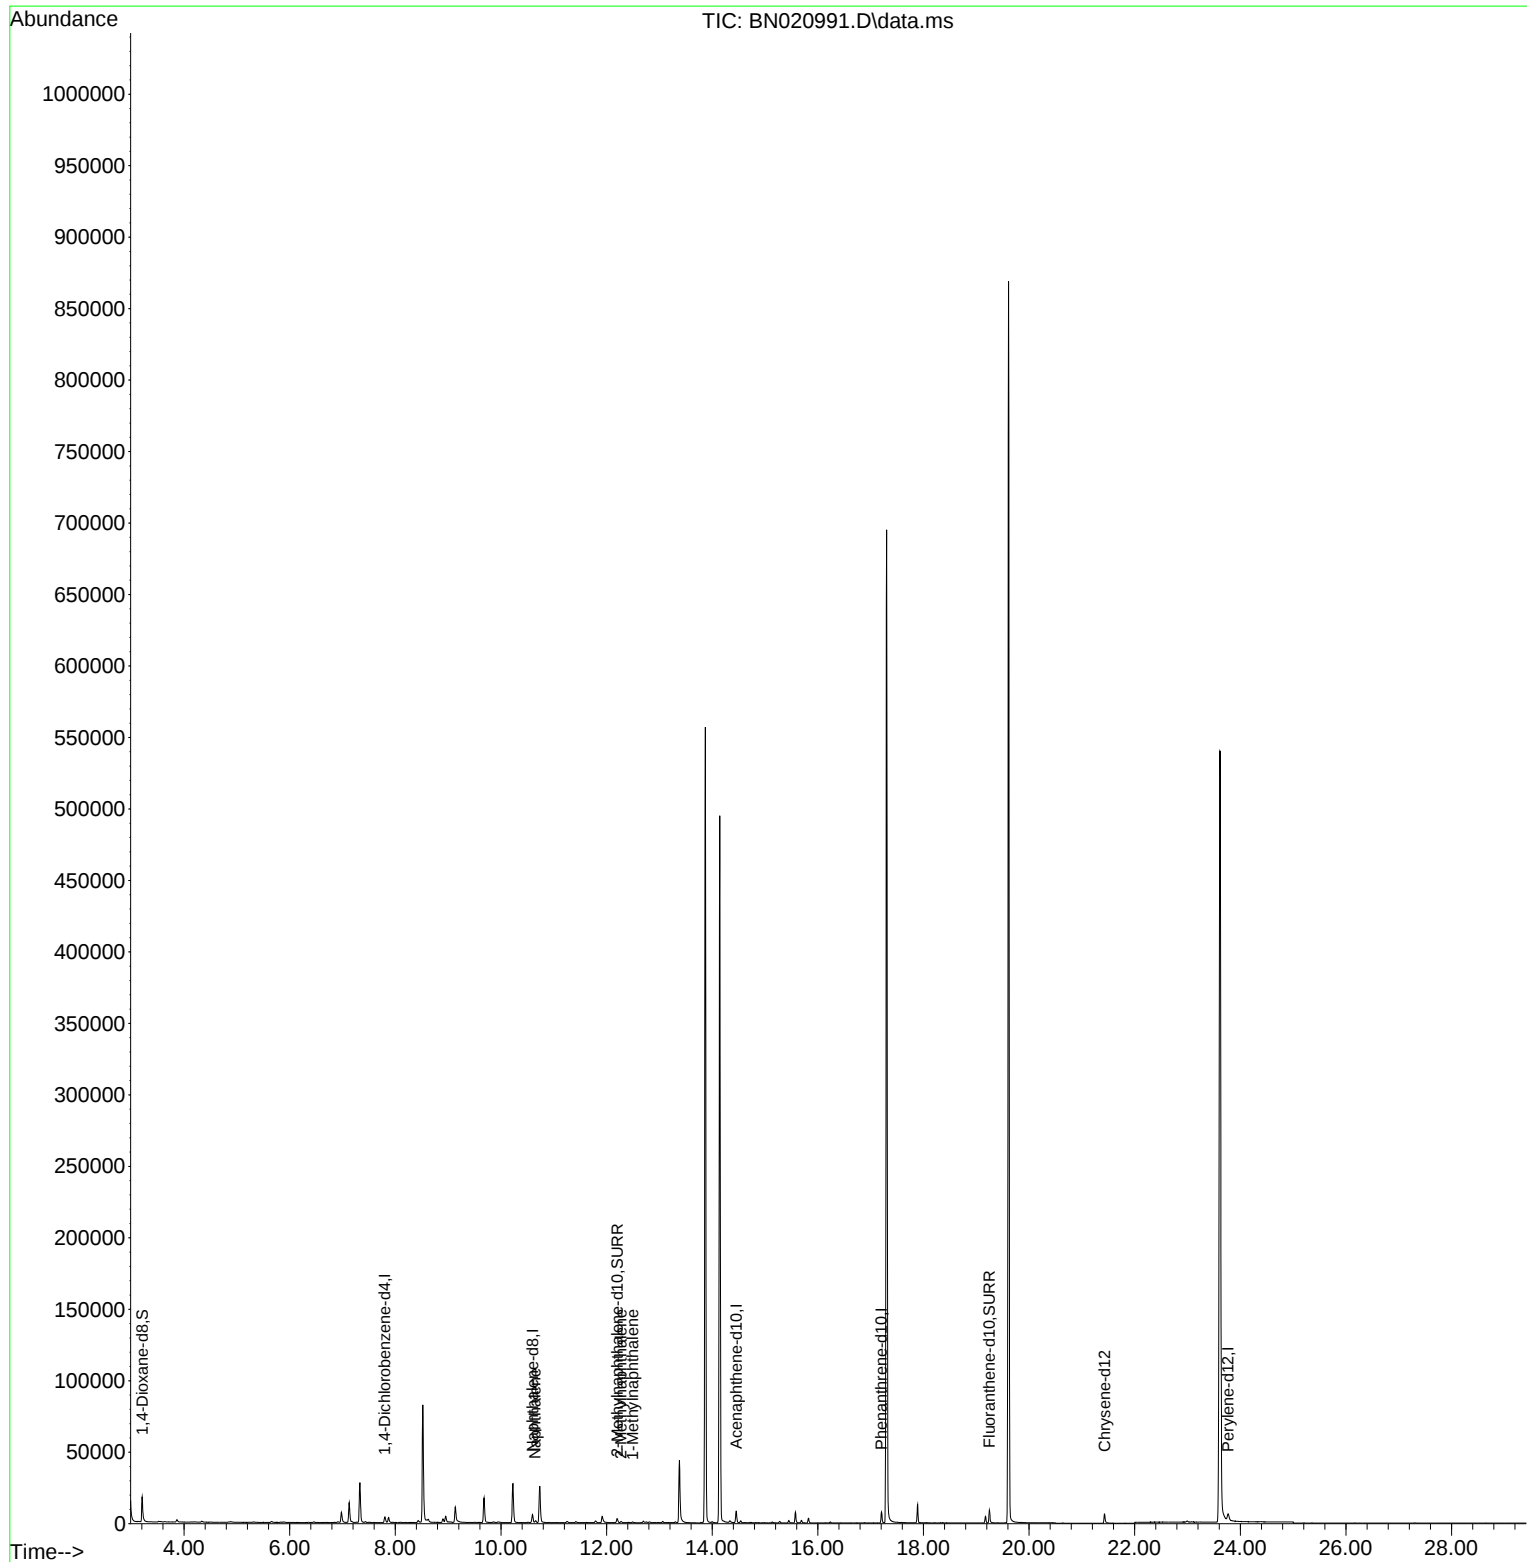

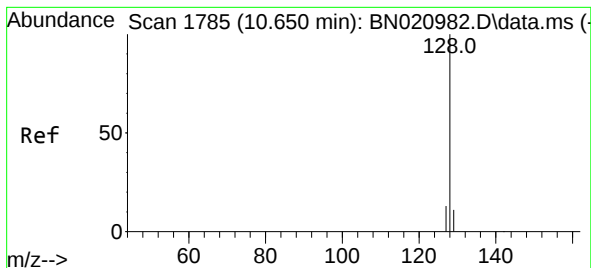

#5

Naphthalene

Concen: 0.023 ng/ul

RT: 10.646 min Scan# 1784

Delta R.T. -0.005 min

Lab File: BN020991.D

Acq: 04 Aug 2022 16:13

Instrument :

BNA_N

ClientSampleId :

C0CB3





Tgt Ion:128 Resp: 552

Ion Ratio Lower Upper

128 100

129 27.9 9.8 14.6#

127 25.0 11.6 17.4#

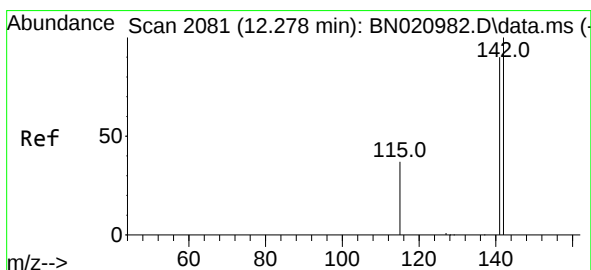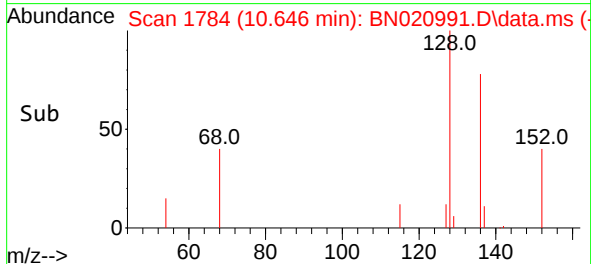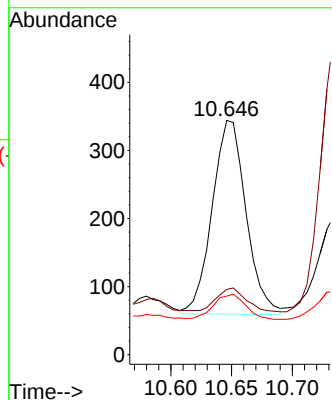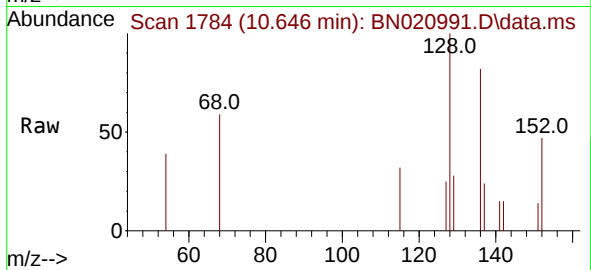

#7

2-Methylnaphthalene

Concen: 0.046 ng/ul

RT: 12.274 min Scan# 2080

Delta R.T. -0.005 min

Lab File: BN020991.D




Acq: 04 Aug 2022 16:13


Tgt Ion:142 Resp: 666

Ion Ratio Lower Upper

142 100

141 90.8 72.2 108.2

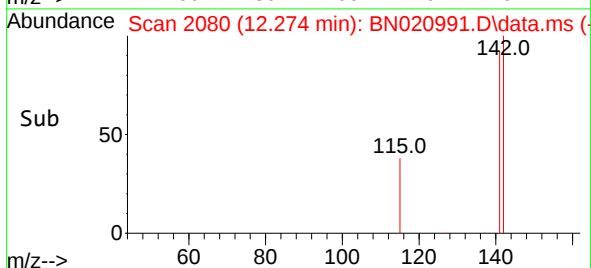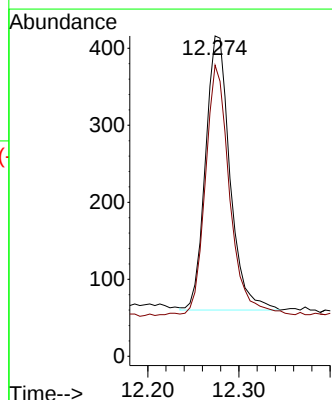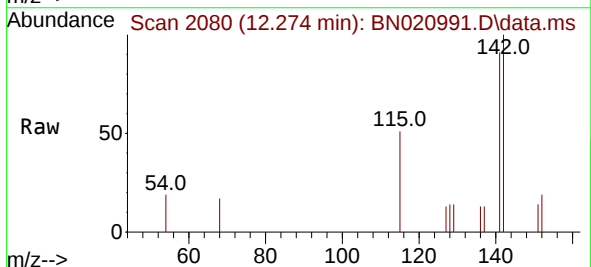

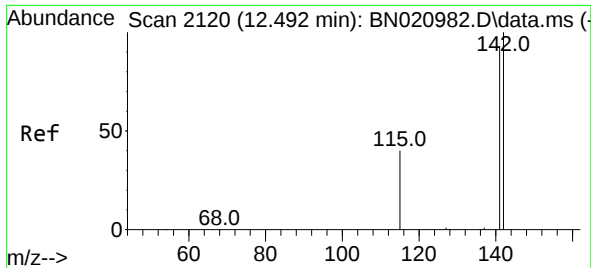

#8
 1-Methylnaphthalene
 Concen: 0.029 ng/ul
 RT: 12.494 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BN020991.D
 Acq: 04 Aug 2022 16:13

Instrument :
 BNA_N
 ClientSampleId :
 C0CB3

Tgt Ion:142 Resp: 426
 Ion Ratio Lower Upper
 142 100
 141 90.8 73.9 110.9

