

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021004.D
 Acq On : 05 Aug 2022 00:26
 Operator : CG/JU
 Sample : N4026-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJG8

Quant Time: Aug 05 01:22:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	3814	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.595	136	11139	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.455	164	6995	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.204	188	13640	0.400	ng/ul	0.00
17) Chrysene-d12	21.416	240	8111	0.400	ng/ul	0.00
23) Perylene-d12	23.751	264	8905	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	20340	4.169	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	4733	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.248	212	11304	0.451	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.244	88	2186	0.435	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021004.D
Acq On : 05 Aug 2022 00:26
Operator : CG/JU
Sample : N4026-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJG8


Quant Time: Aug 05 01:22:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

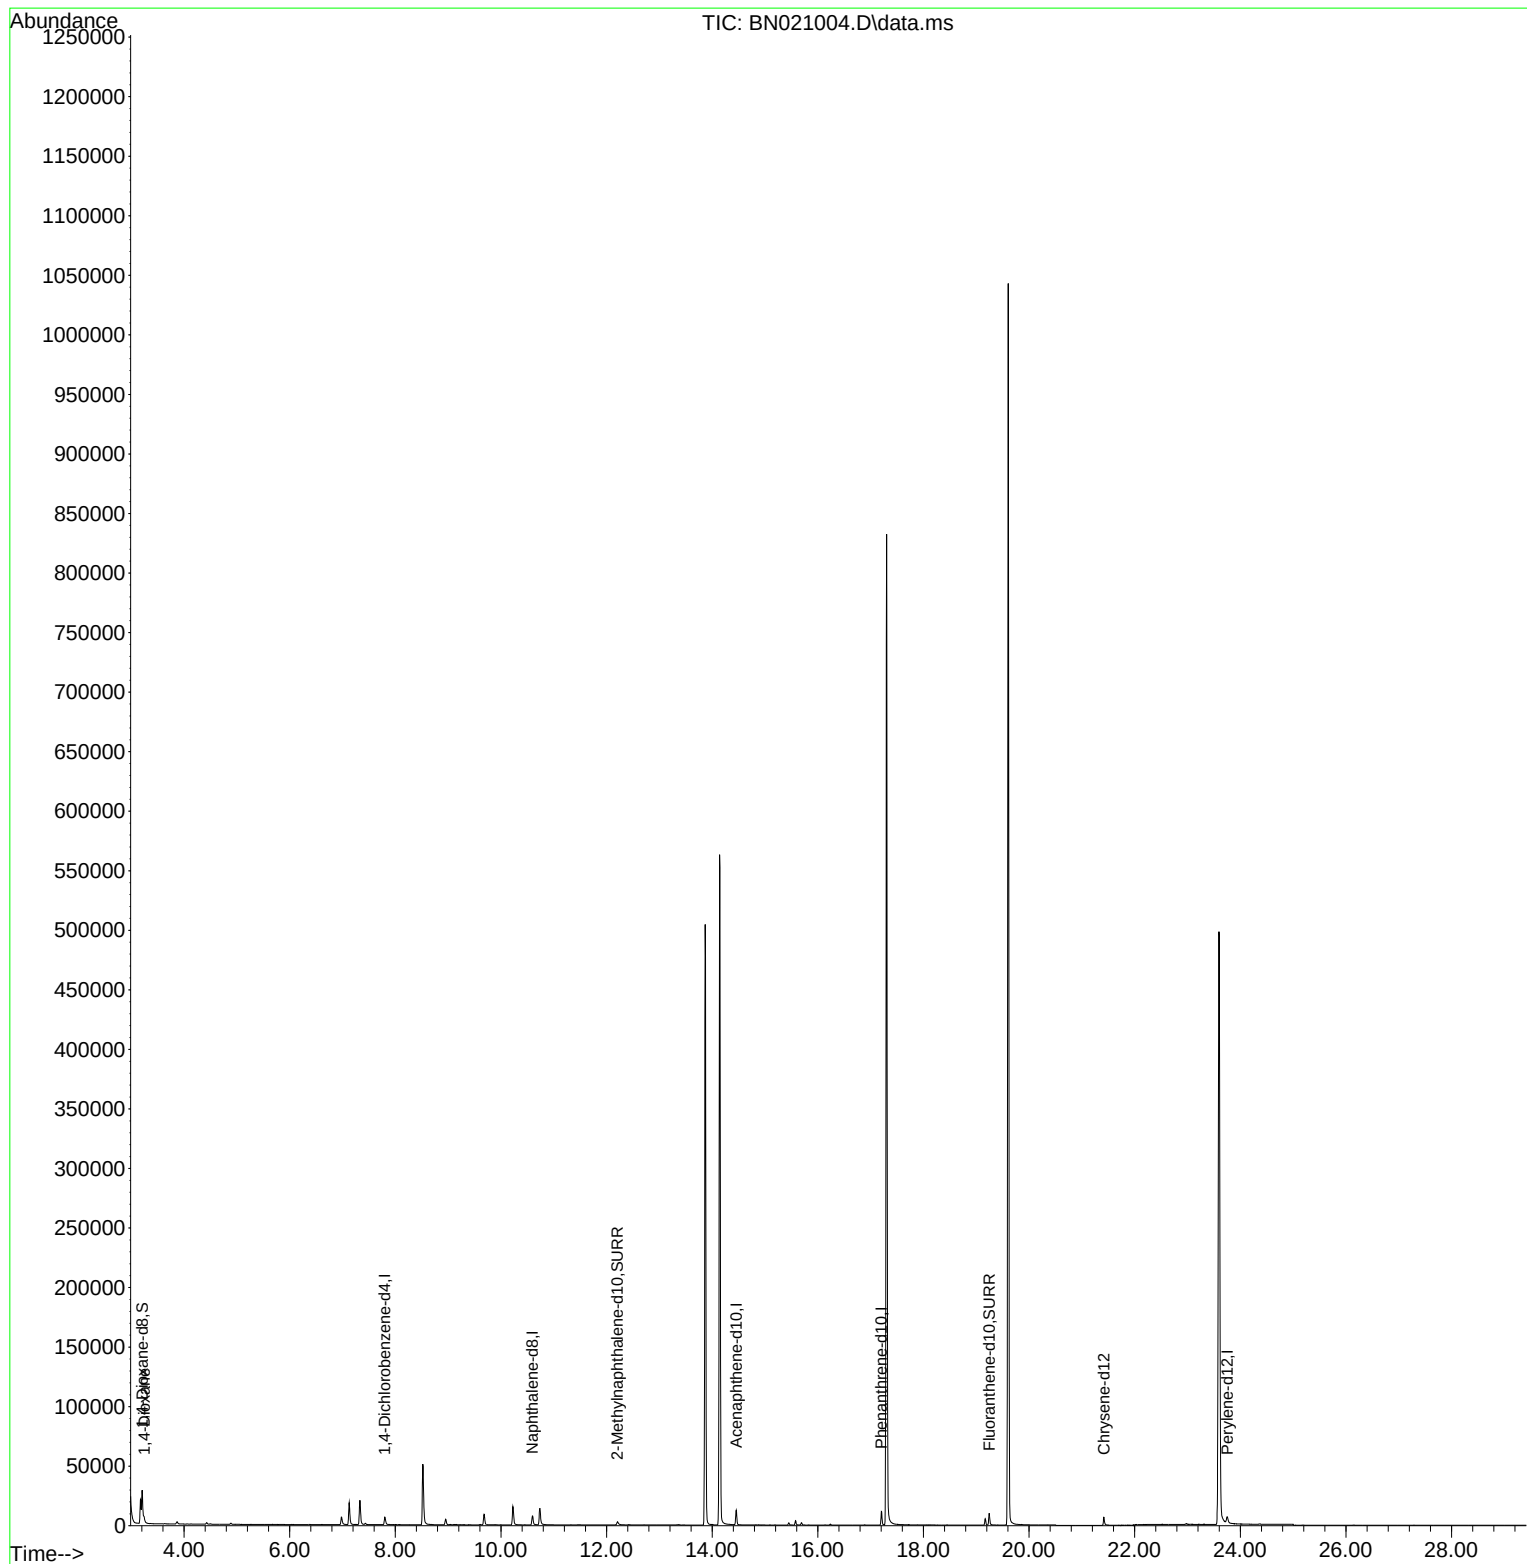

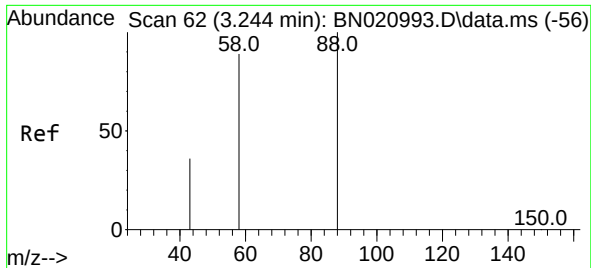

#2
 1,4-Dioxane
 Concen: 0.435 ng/ul
 RT: 3.244 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN021004.D
 Acq: 05 Aug 2022 00:26

Instrument :
 BNA_N
 ClientSampleId :
 GBJG8

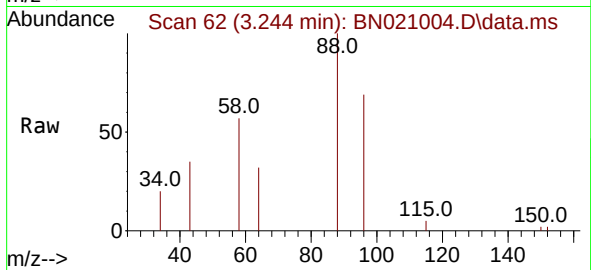

Tgt Ion:	88	Resp:	2186
Ion	Ratio	Lower	Upper
88	100		
43	34.9	31.4	47.0
58	56.9	49.0	73.6

