

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
 Data File : BN021047.D
 Acq On : 06 Aug 2022 04:27
 Operator : CG/JU
 Sample : N4026-13
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJH7

Quant Time: Aug 06 05:05:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 16:31:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	3072	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.591	136	9862	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.452	164	5732	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.201	188	11290	0.400	ng/ul	0.00
17) Chrysene-d12	21.410	240	8720	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	8982	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	14068	3.580	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.202	152	4967	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.240	212	11757	0.437	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.245	88	360	0.089	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080422\
Data File : BN021047.D
Acq On : 06 Aug 2022 04:27
Operator : CG/JU
Sample : N4026-13
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJH7


Quant Time: Aug 06 05:05:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 16:31:11 2022
Response via : Initial Calibration

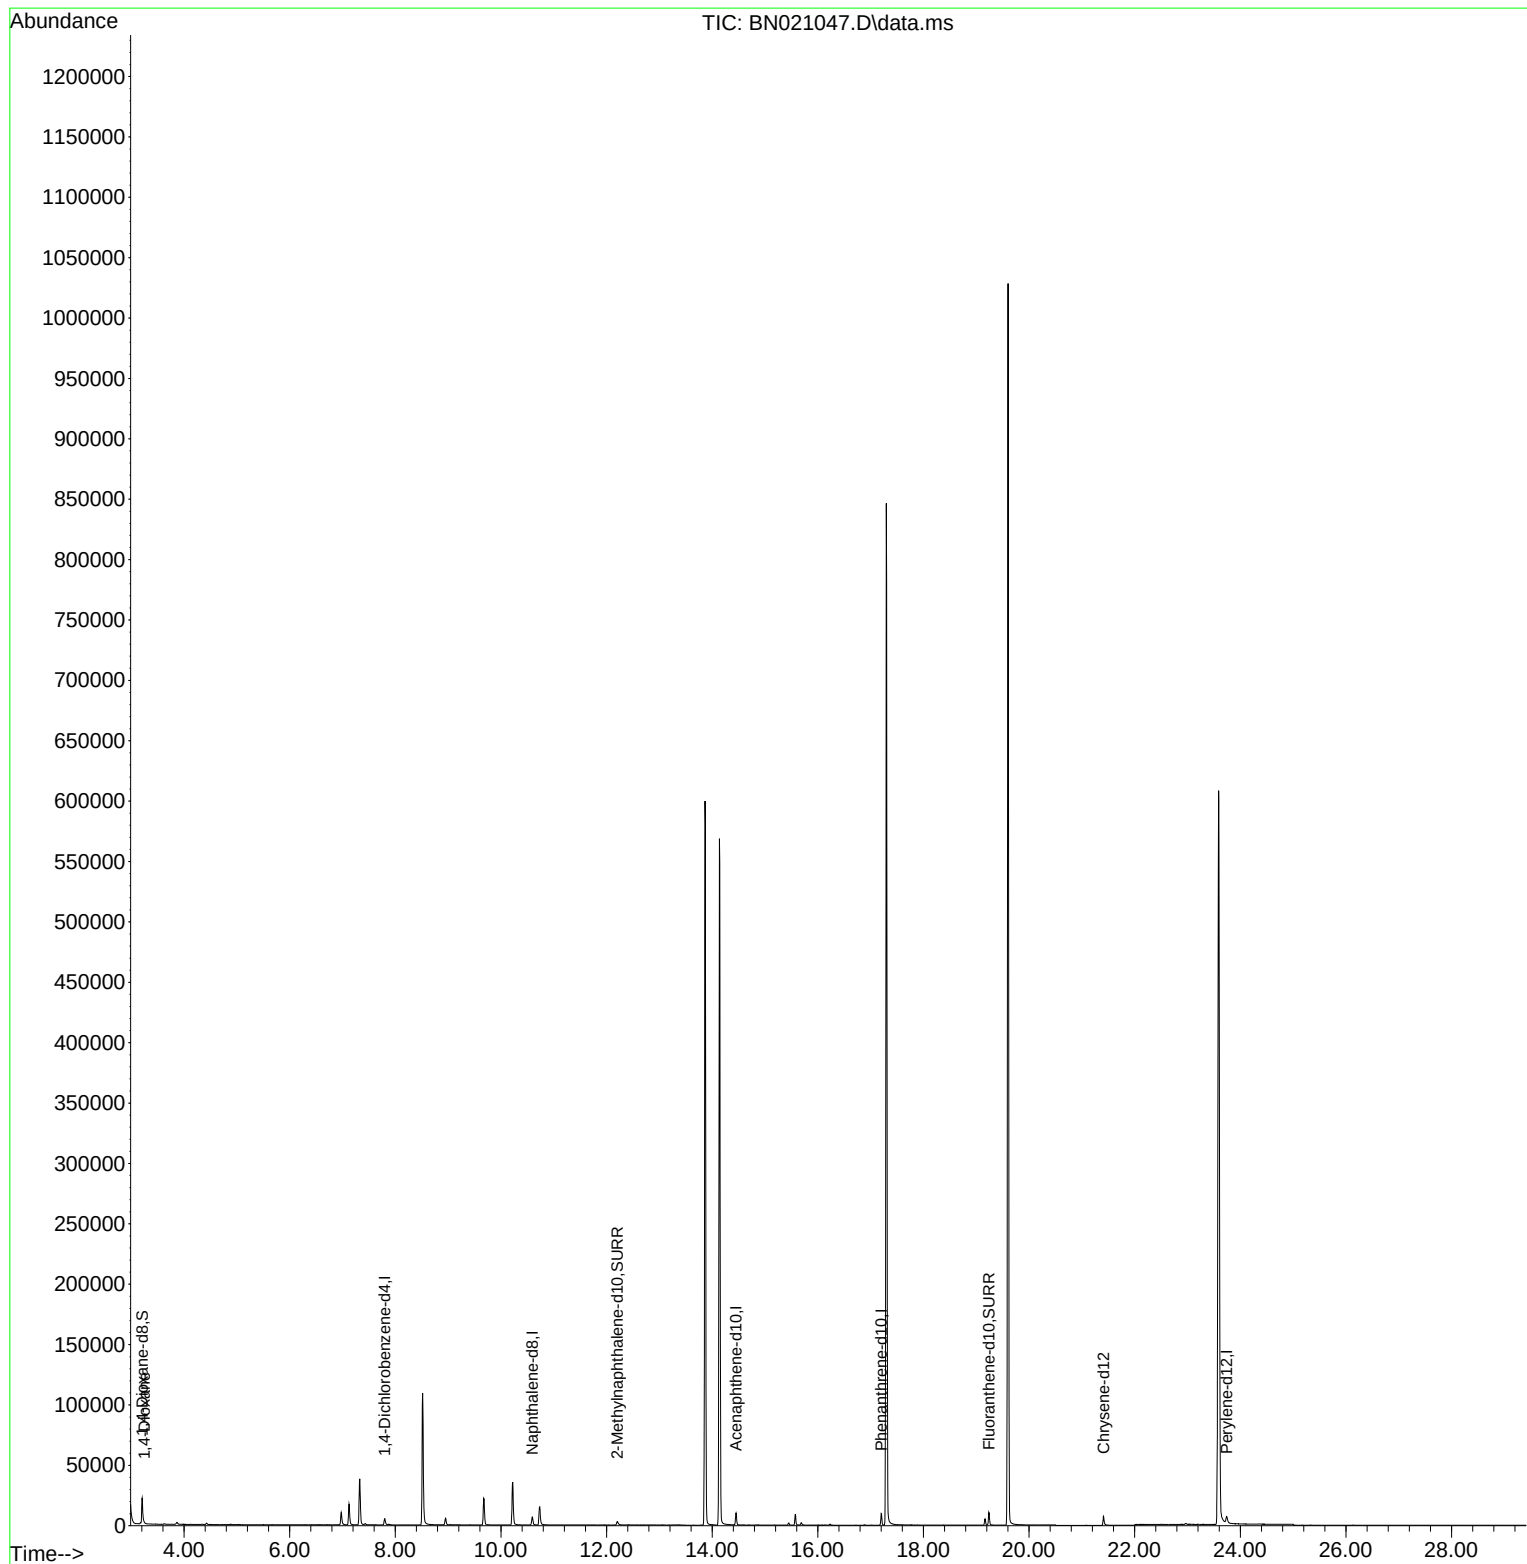

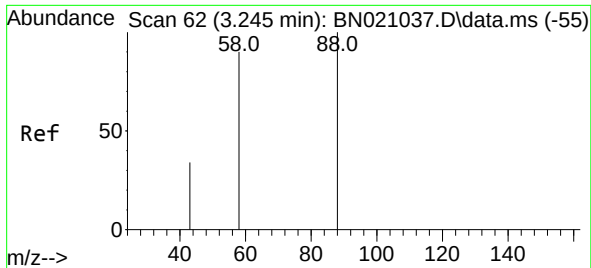

#2
 1,4-Dioxane
 Concen: 0.089 ng/ul
 RT: 3.245 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN021047.D
 Acq: 06 Aug 2022 04:27

Instrument :
 BNA_N
 ClientSampleId :
 GBJH7

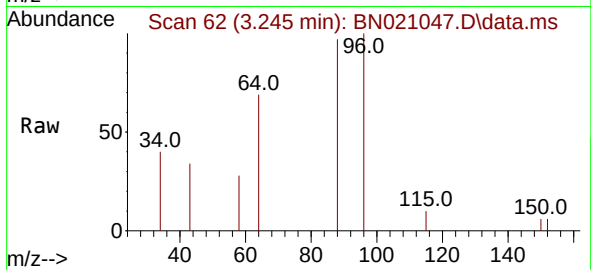

Tgt Ion:	88	Resp:	360
Ion	Ratio	Lower	Upper
88	100		
43	34.5	31.4	47.0
58	28.3	49.0	73.6#

