
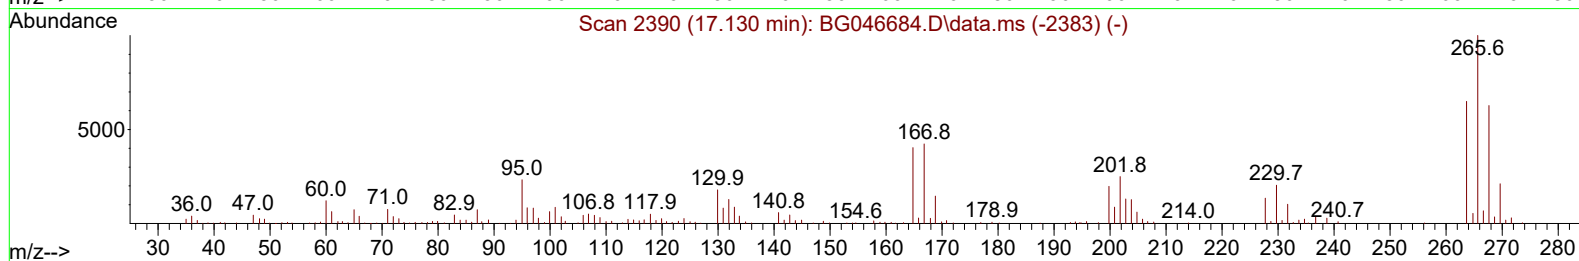
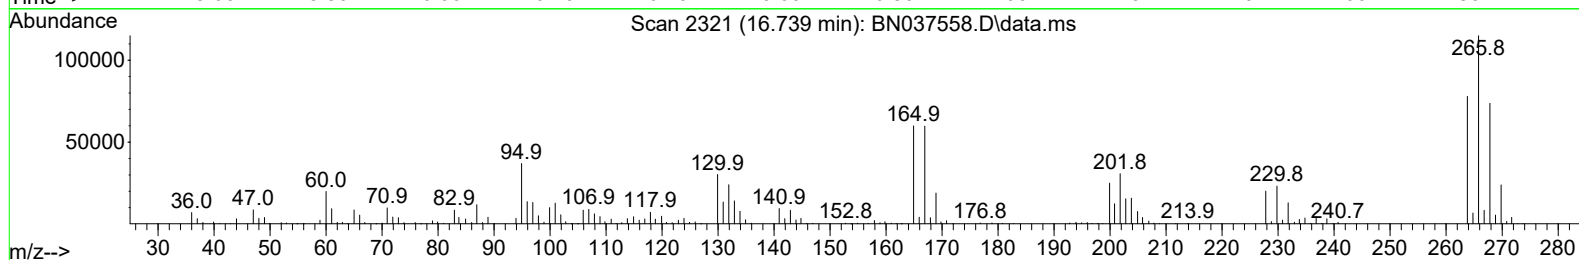


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080525\
Data File : BN037558.D
Acq On : 05 Aug 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:49:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

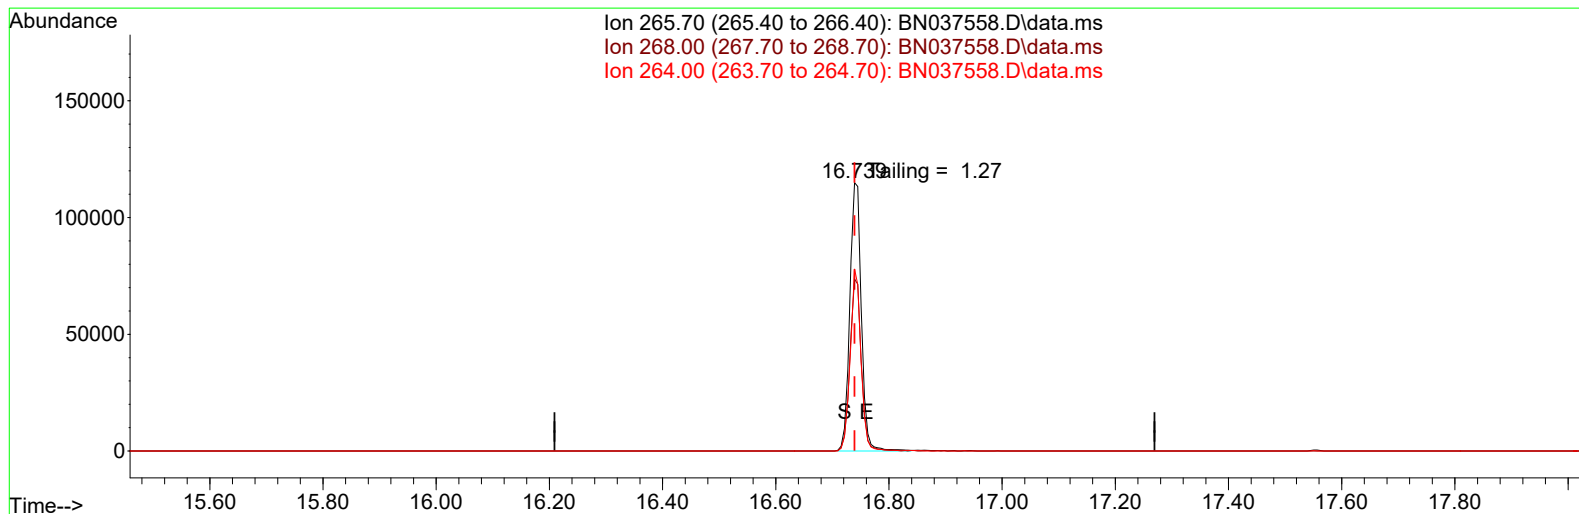

TIC: BN037558.D\data.ms

(70) Pentachlorophenol (C)




16.739min (0.000) 277.06 ng

response 162965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.12
264.00	61.60	67.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080525\
Data File : BN037558.D
Acq On : 05 Aug 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:49:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

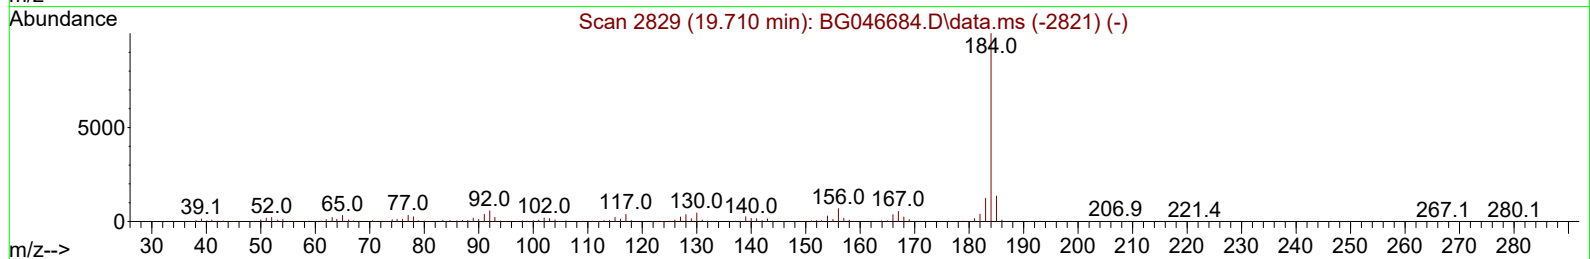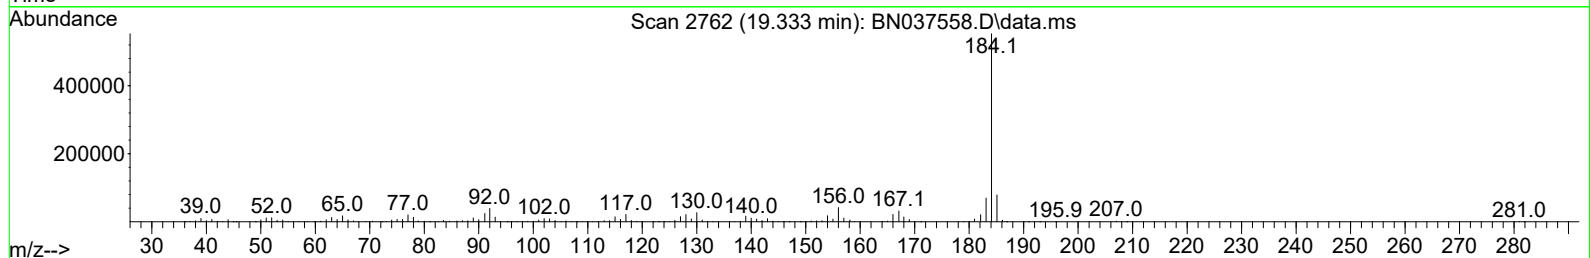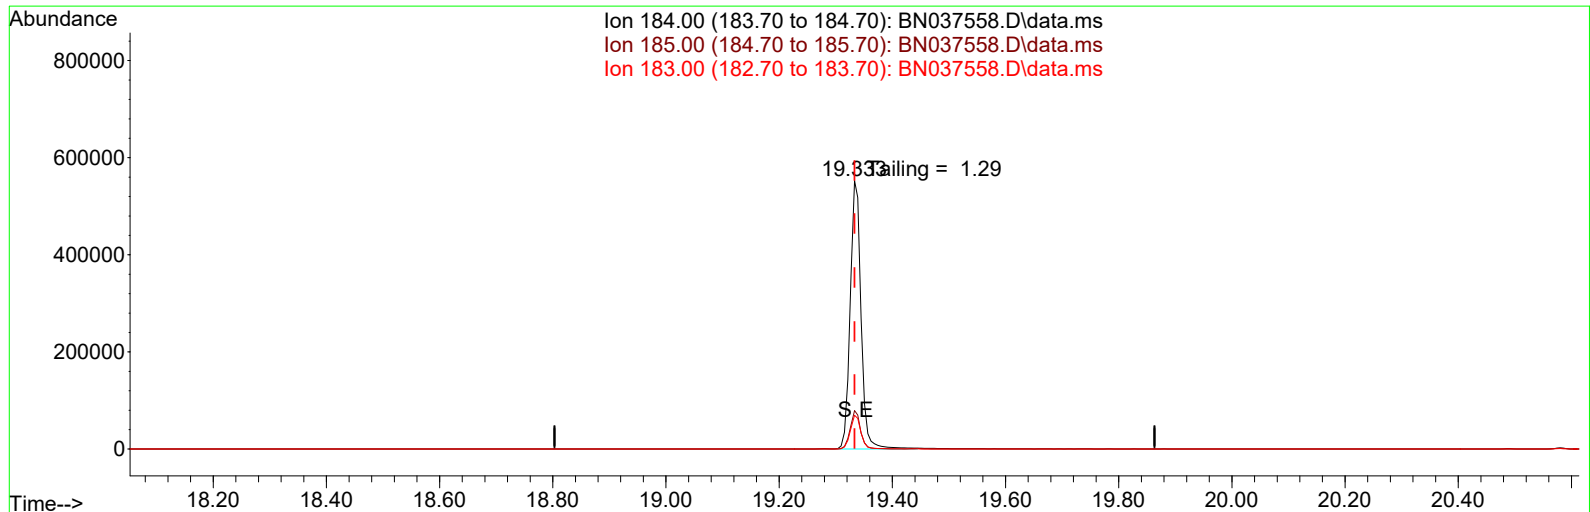

TIC: BN037558.D\data.ms

(77) Benzidine

19.333min (0.000) 0.00 ng

response 738941

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	12.60
0.00	0.00	0.00