


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080525\
Data File : BN037558.D
Acq On : 05 Aug 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 19 01:46:16 2025

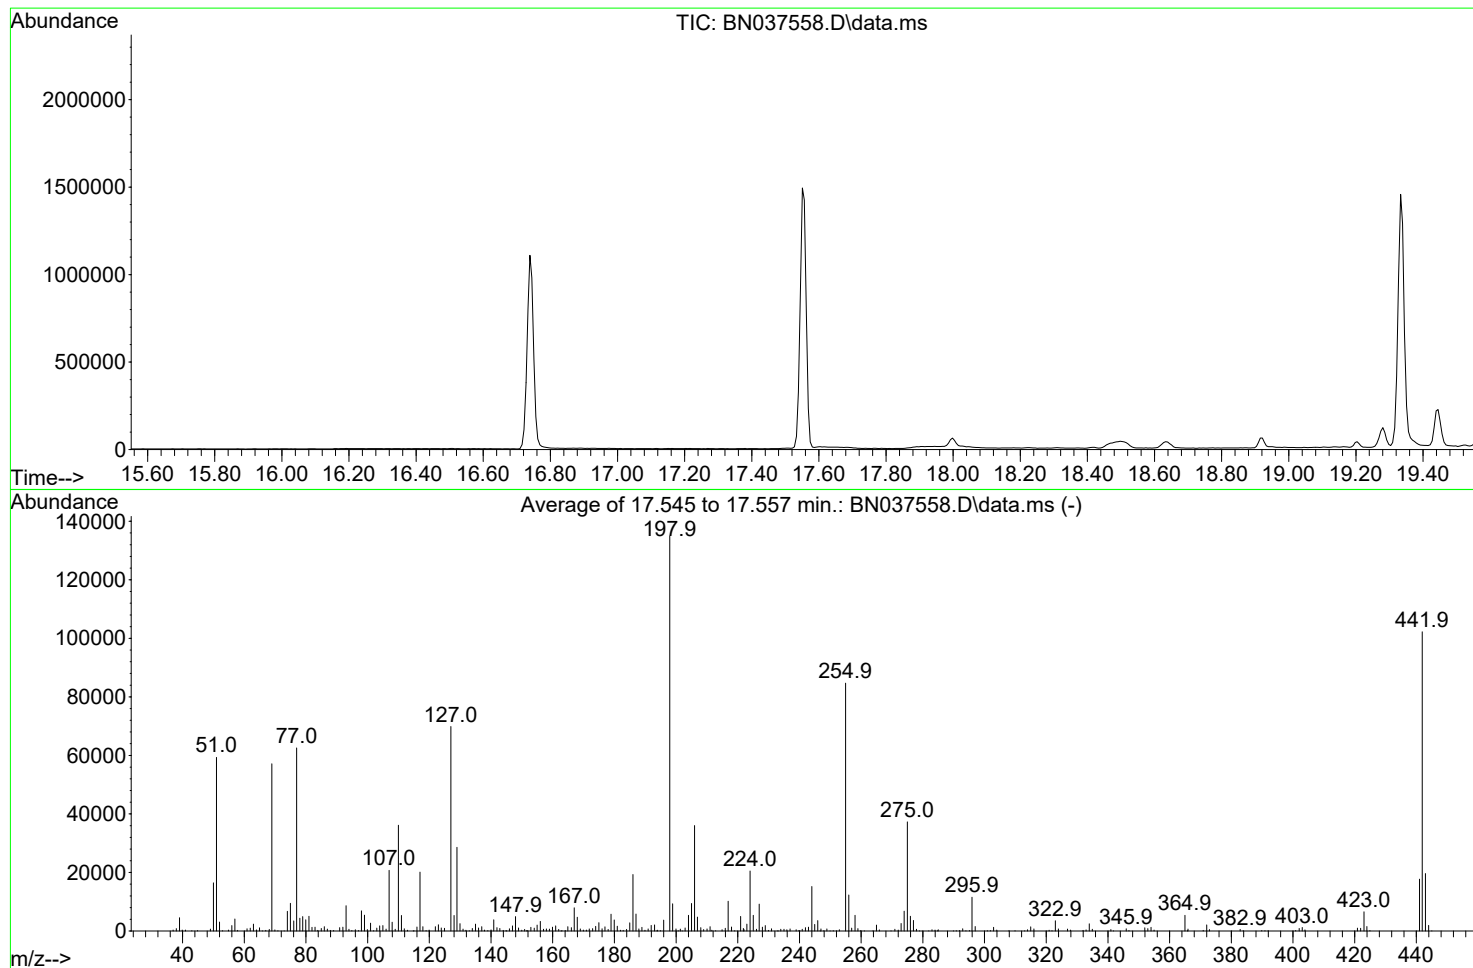

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	529	PASS
69	69	100	100	100.0	57147	PASS
70	69	0.00	2	0.6	370	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134912	PASS
199	198	5	9	6.9	9307	PASS
365	198	1	100	4.0	5372	PASS
441	443	0.01	150	90.3	17710	PASS
442	442	100	100	100.0	102248	PASS
443	442	15	24	19.2	19611	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/5/2025	BNA_N	<u>BN037558.D</u>
Compound Name	Response	Retention Time
DDT	445735	20.58
DDD	4329	20.192
DDE	60	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4389	450124	0.98

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080525\
Data File : BN037558.D
Acq On : 05 Aug 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 01:49:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

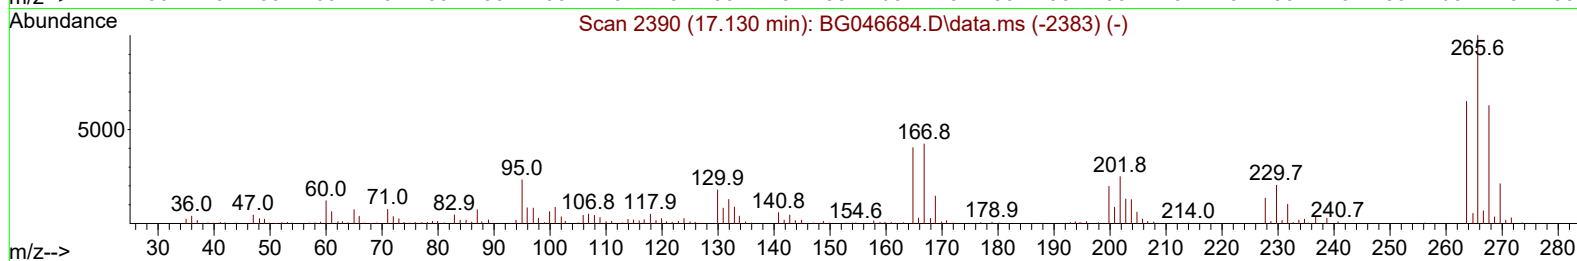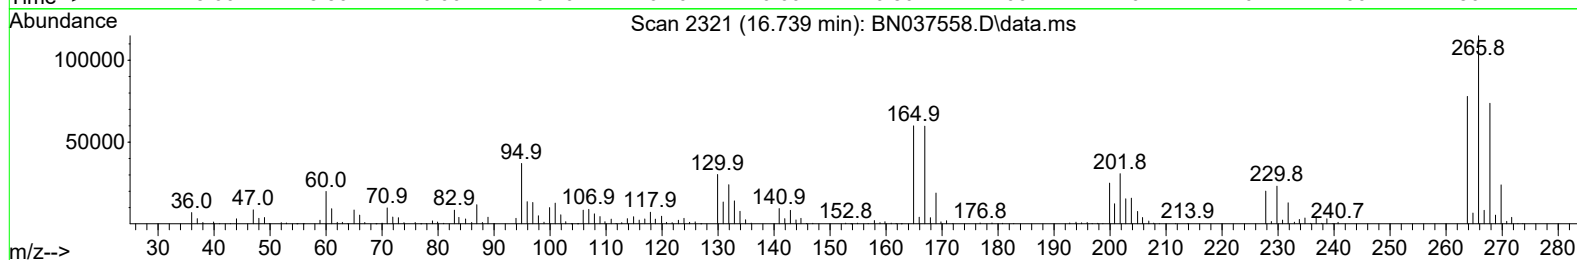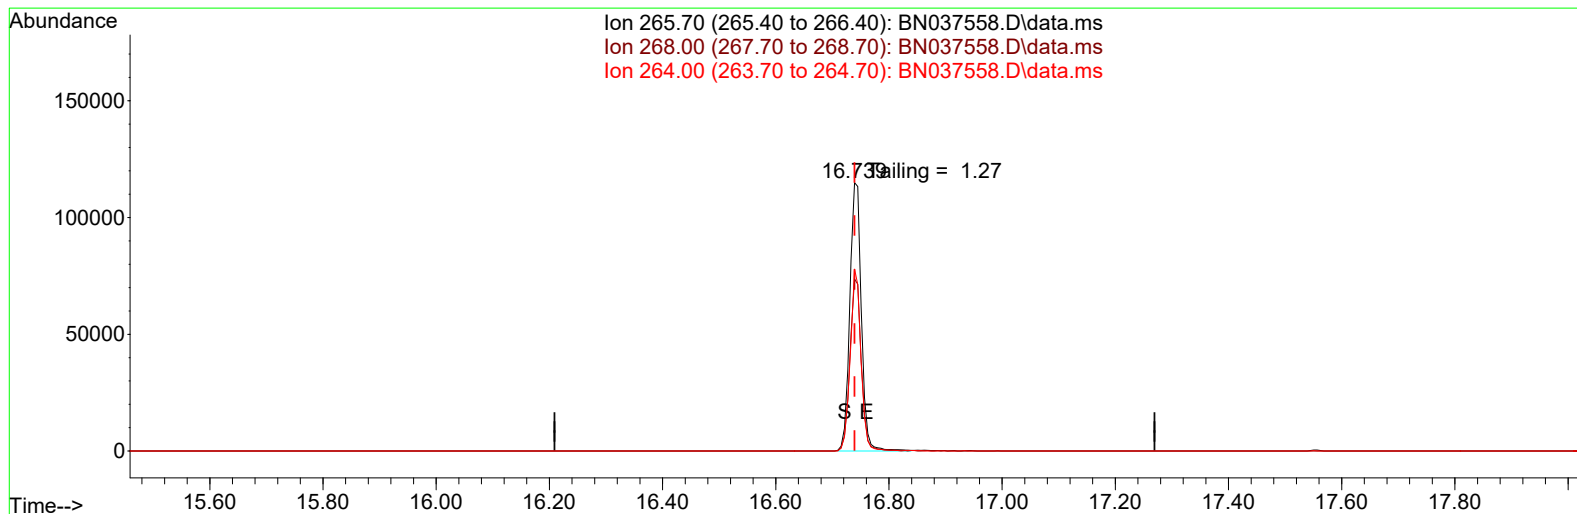

TIC: BN037558.D\data.ms

(70) Pentachlorophenol (C)

16.739min (0.000) 277.06 ng




response 162965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.12
264.00	61.60	67.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080525\
Data File : BN037558.D
Acq On : 05 Aug 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 01:49:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

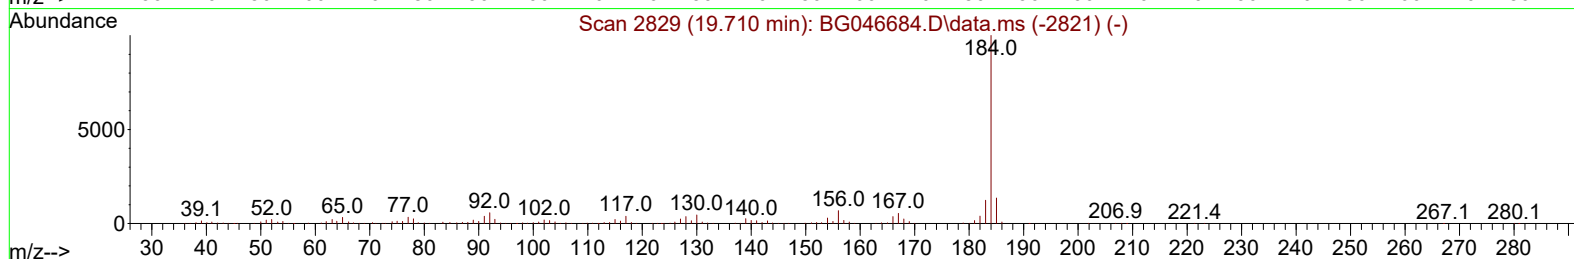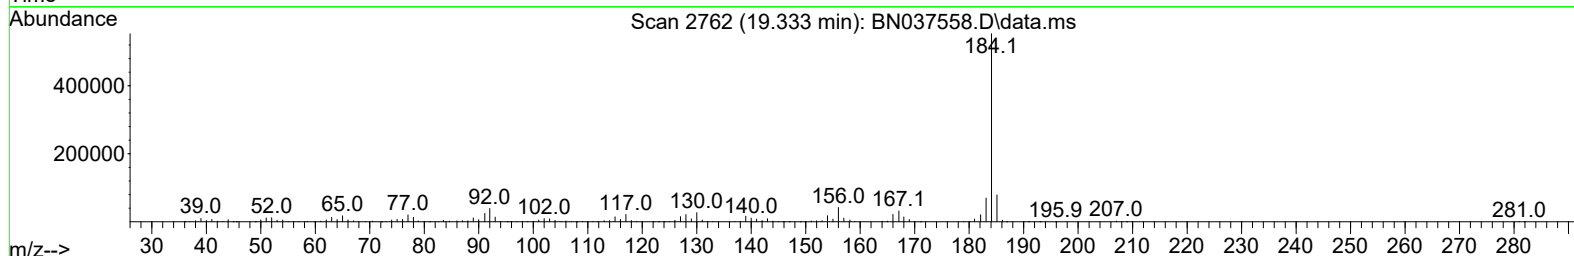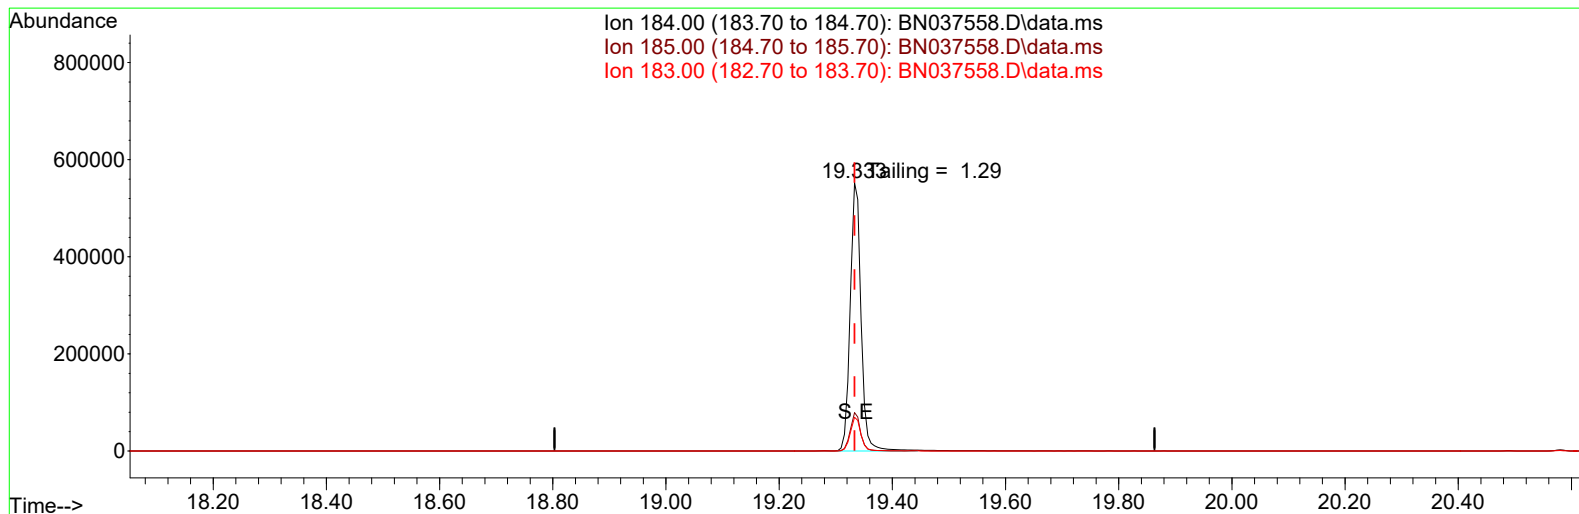

TIC: BN037558.D\data.ms

(77) Benzidine

19.333min (0.000) 0.00 ng

response 738941

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	12.60
0.00	0.00	0.00