
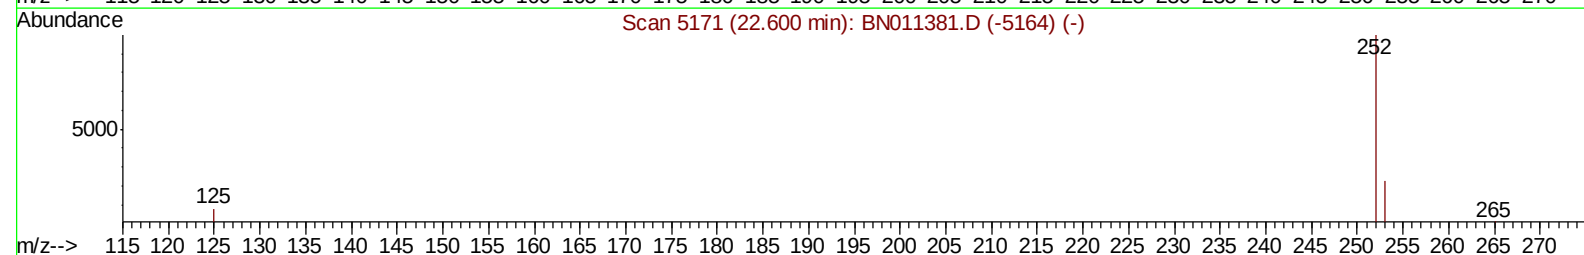
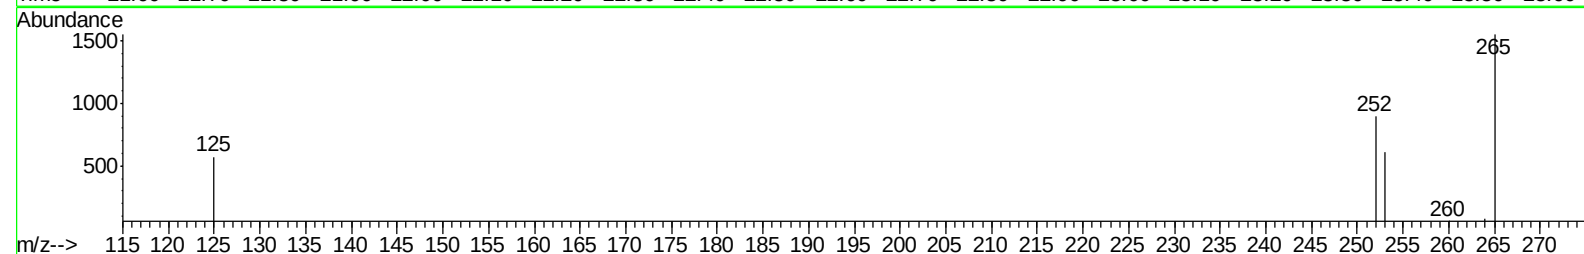


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\
Data File : BN011385.D
Acq On : 06 Aug 2020 18:38
Operator : CG/JU
Sample : L3419-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 07 02:06:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 07 02:04:45 2020
Response via : Initial Calibration

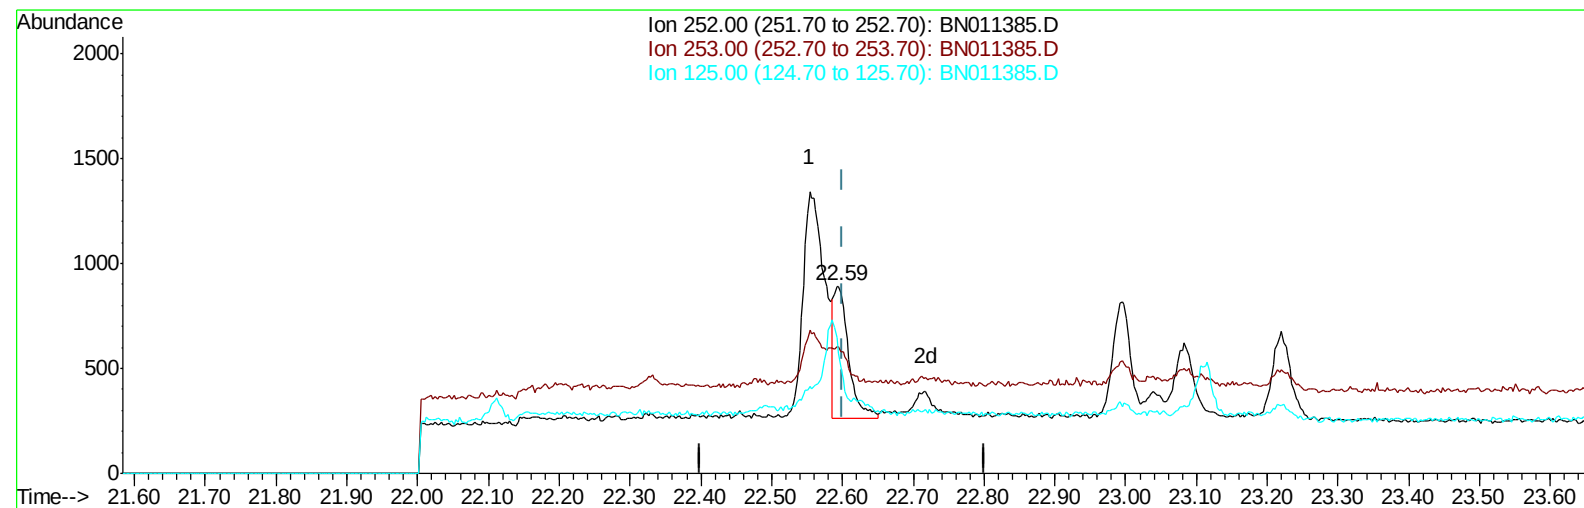

TIC: BN011385.D

(22) Benzo(k)fluoranthene

22.595min (-0.006) 0.04ng/ul m

response 879

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	67.94#
125.00	15.70	64.24#
0.00	0.00	0.00