

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\
 Data File : BN011387.D
 Acq On : 06 Aug 2020 19:49
 Operator : CG/JU
 Sample : L3419-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF1

Quant Time: Aug 07 02:06:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 07 02:04:45 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	4655	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.09	164	2840	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.85
16) Chrysene-d12	21.06	240	6350	0.40	ng/ul	0.00
20) Perylene-d12	23.17	264	6713	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.80	152	2354	0.20	ng/ul	-0.01
14) Fluoranthene-d10	18.88	212	4929	0.00	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.04	252	1401	0.058	ng/ul#	Ovalue 13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\
Data File : BN011387.D
Acq On : 06 Aug 2020 19:49
Operator : CG/JU
Sample : L3419-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Quant Time: Aug 07 02:06:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 07 02:04:45 2020
Response via : Initial Calibration

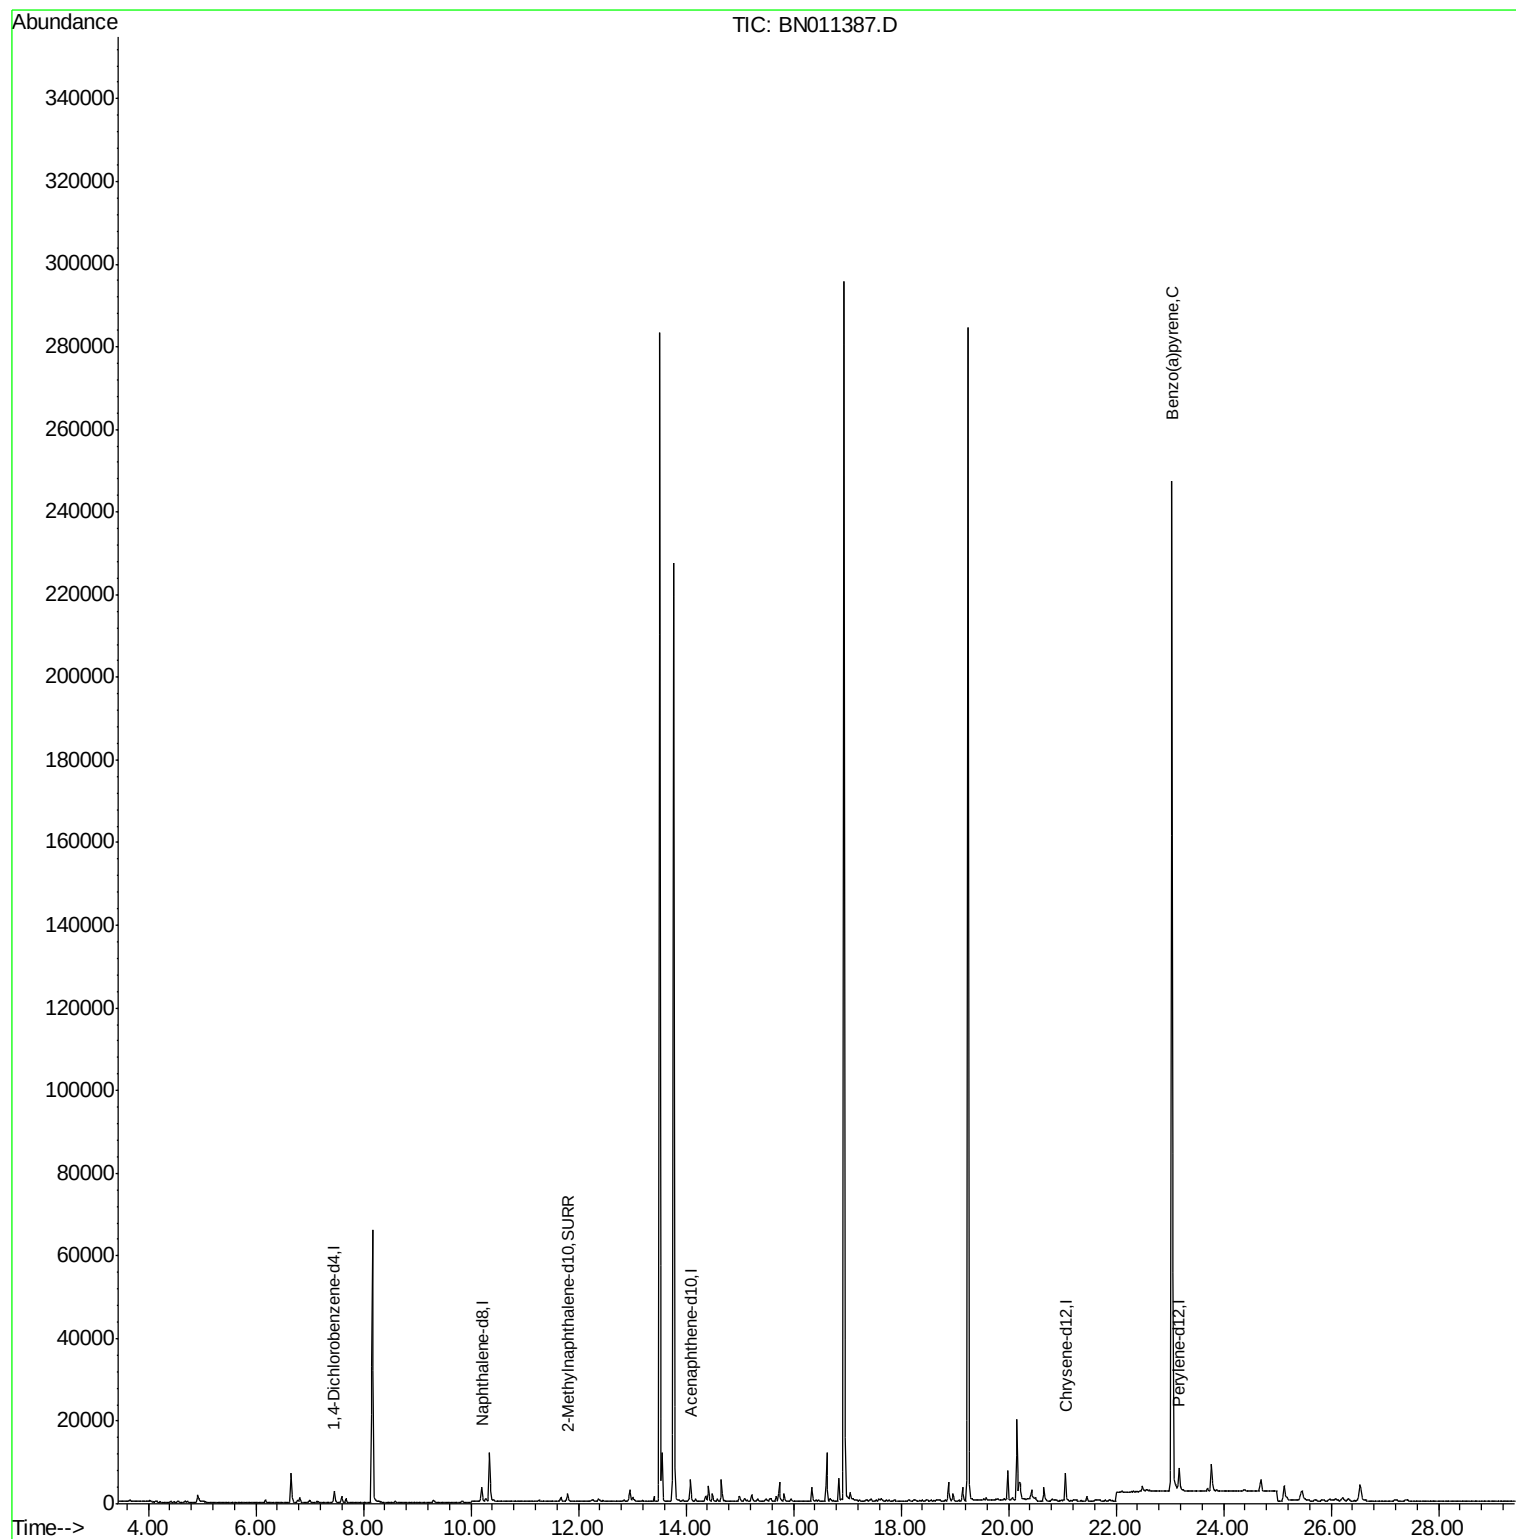

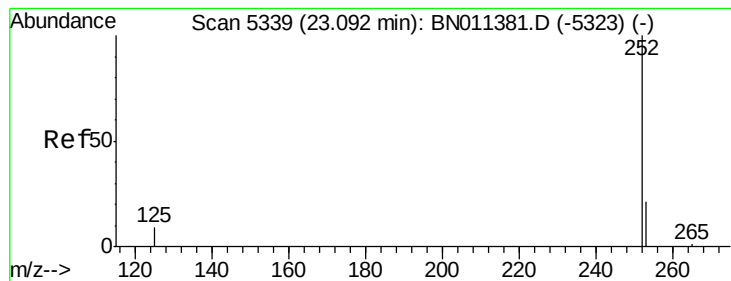

#23

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.04 min Scan# 5321

Delta R.T. -0.05 min

Lab File: BN011387.D


Acq: 06 Aug 2020 19:49

Instrument :

BNA_N

ClientSampleId :

C0AF1

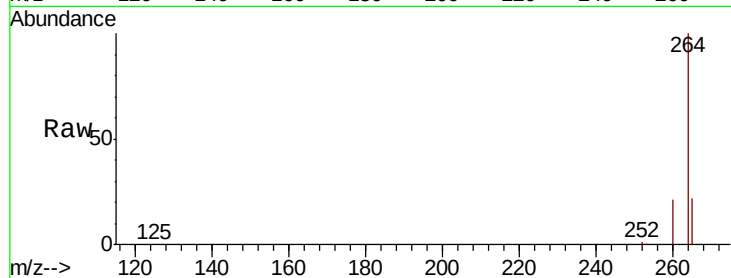

Tot Ion: 252 Resp: 1401

Ion Ratio Lower Upper

252 100

253 77.2 22.6 34.0#

125 48.1 12.6 18.8#

