


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
Data File : BN011373.D
Acq On : 06 Aug 2020 11:21
Operator : CG/JU
Sample : PB130603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 06 12:17:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 06 12:09:32 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK03

Manual Integrations
APPROVED

mohammad
8/7/2020 1:52:53 PM

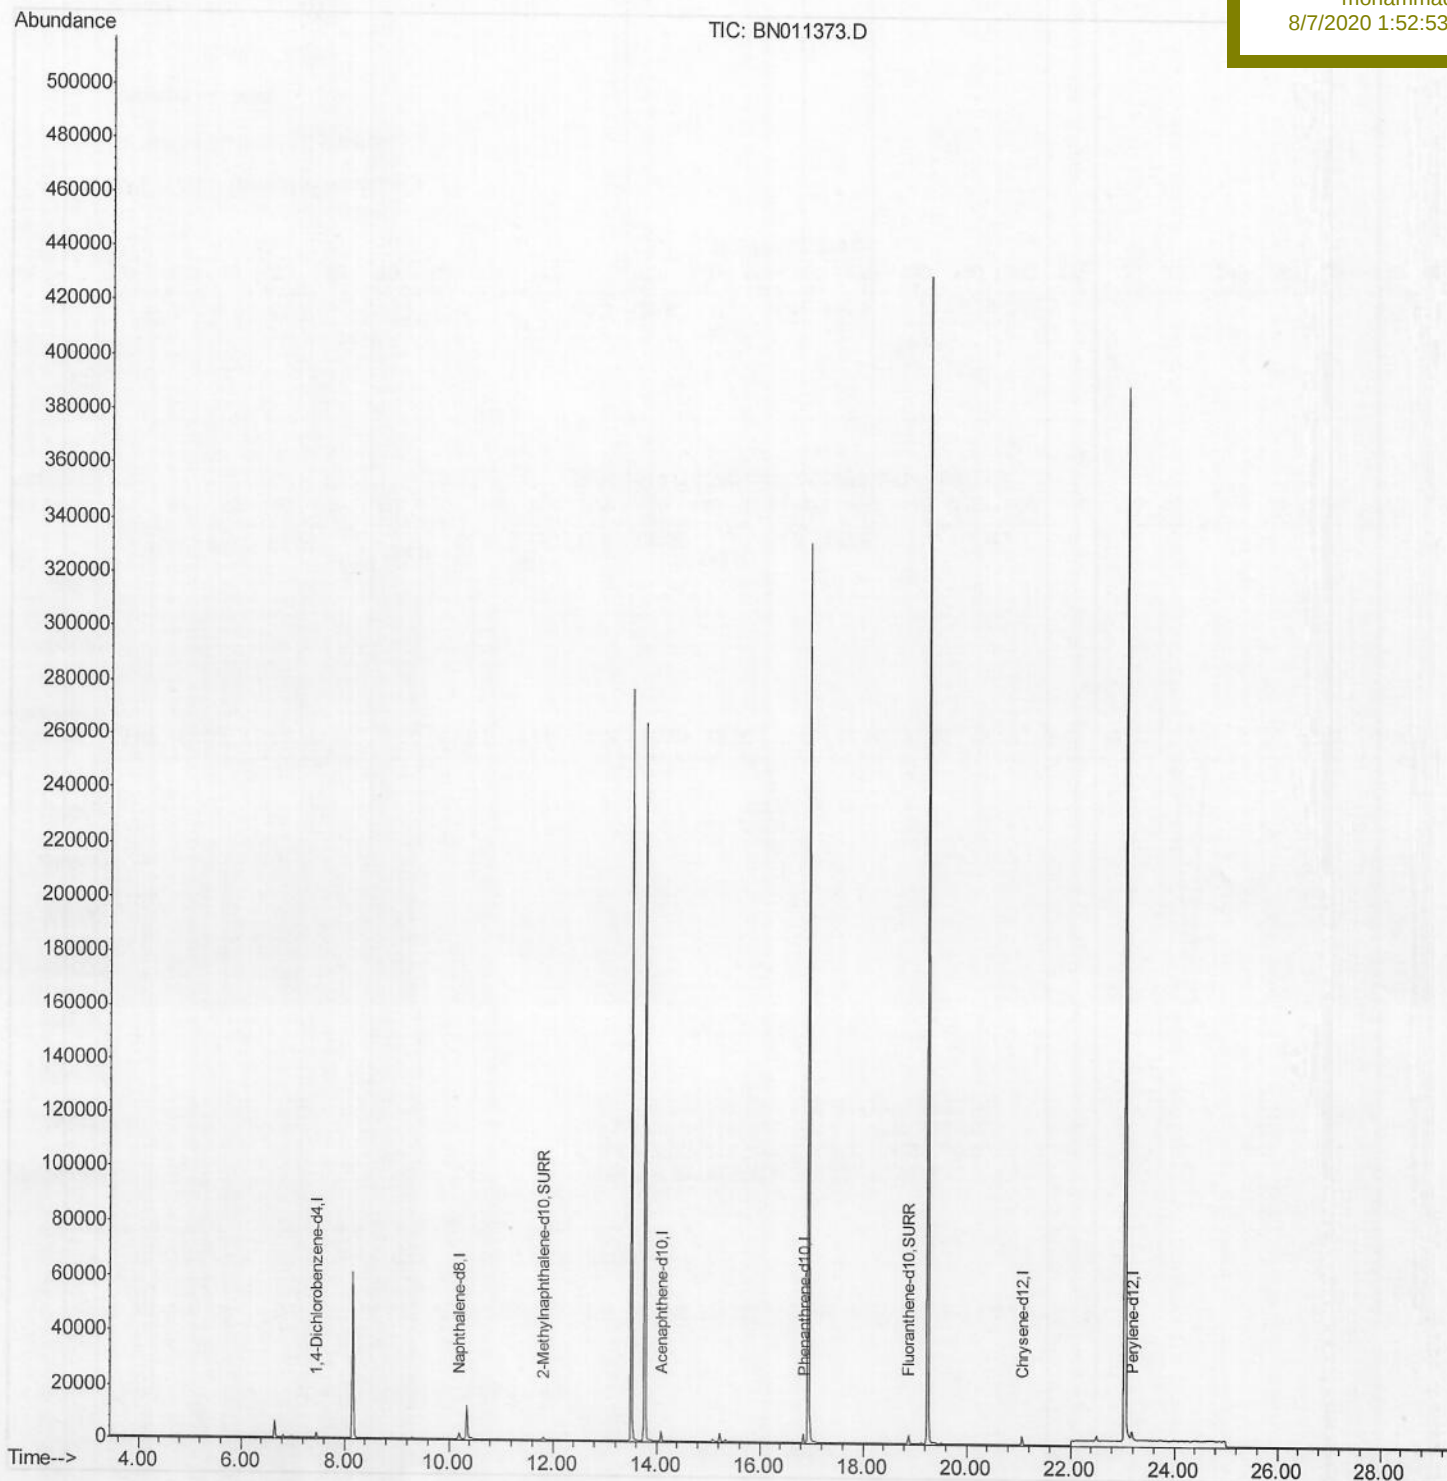

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\

Data File : BN011373.D

Acq On : 06 Aug 2020 11:21

Operator : CG/JU

Sample : PB130603BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 06 12:11:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Aug 06 12:09:32 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


SBLK03

Manual Integrations

APPROVED

mohammad

8/7/2020 1:52:53 PM

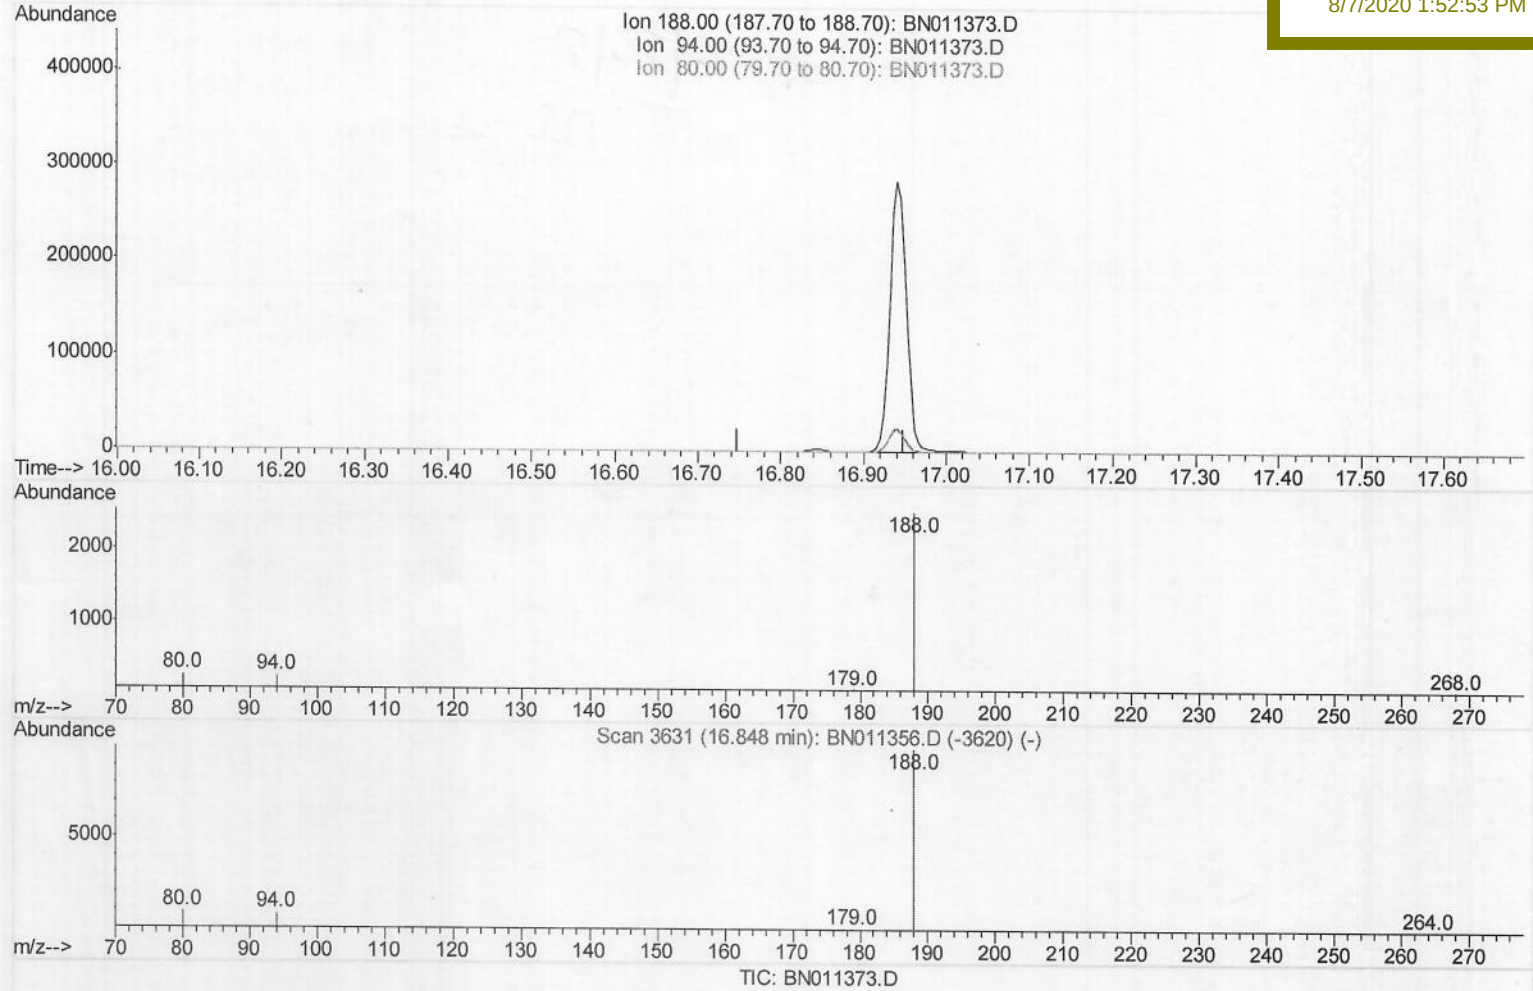

(10) Phenanthrene-d10 (I)

16.848min (-16.848) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\

Data File : BN011373.D

Acq On : 06 Aug 2020 11:21

Operator : CG/JU

Sample : PB130603BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 06 12:11:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Aug 06 12:09:32 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :



SBLK03

Manual Integrations

APPROVED

mohammad

8/7/2020 1:52:53 PM

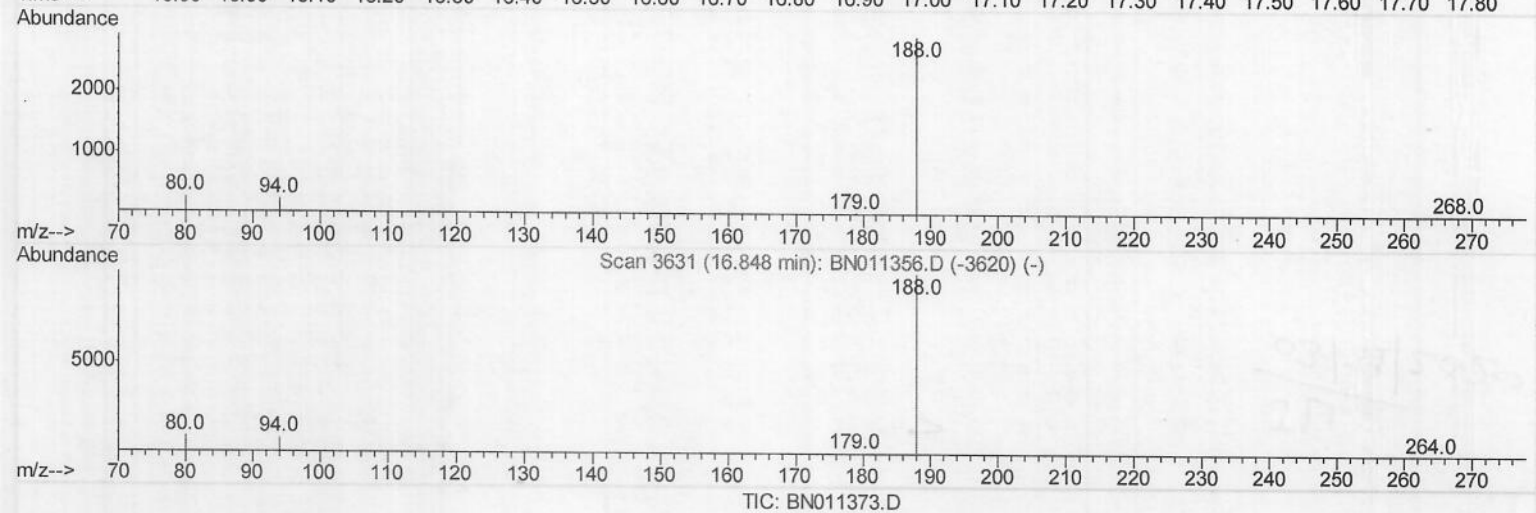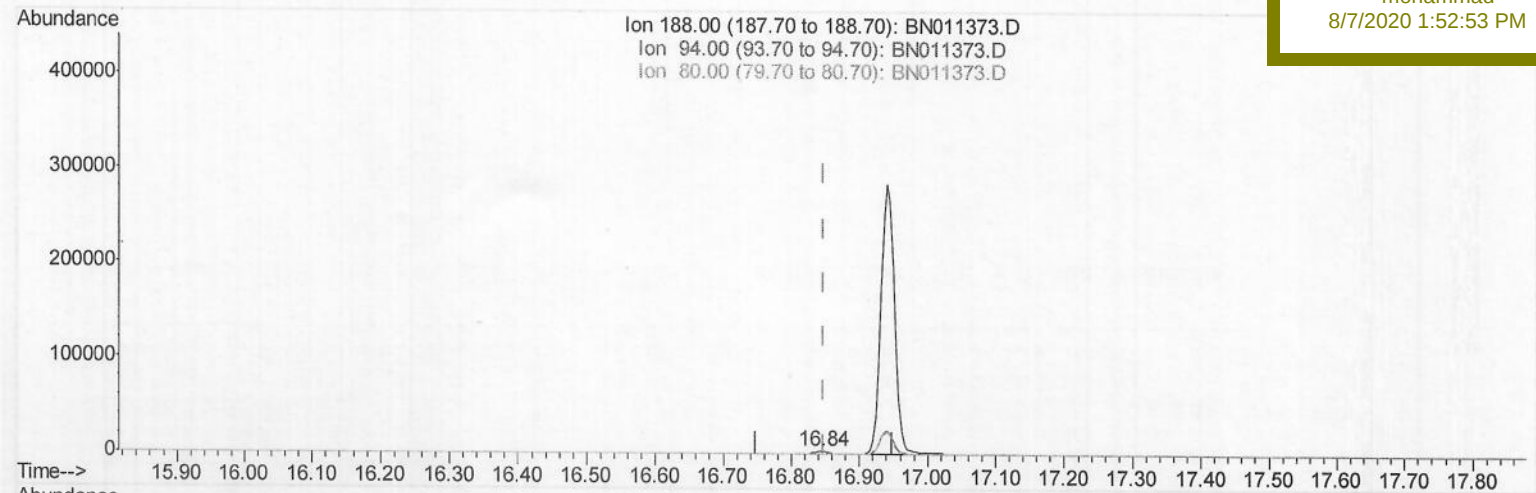

(10) Phenanthrene-d10 (I)

16.844min (-0.004) 0.40ng/ul m

response 4096

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	8.66
80.00	10.30	9.94
0.00	0.00	0.00

> JU
08/07/20

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
Data File : BN011373.D
Acq On : 06 Aug 2020 11:21
Operator : CG/JU
Sample : PB130603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 06 12:17:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 06 12:09:32 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK03

Manual Integrations
APPROVED

mohammad
8/7/2020 1:52:53 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	974	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	3174	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.09	164	1884	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.84	188	4096m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	3548	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	4485	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	1838	0.23	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	4150	0.21	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 08/08/20