


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
Data File : BN011380.D
Acq On : 06 Aug 2020 15:38
Operator : CG/JU
Sample : L3487-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 06 16:16:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 06 12:09:32 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
F4L04

Manual Integrations
APPROVED

mohammad
8/7/2020 1:53:09 PM

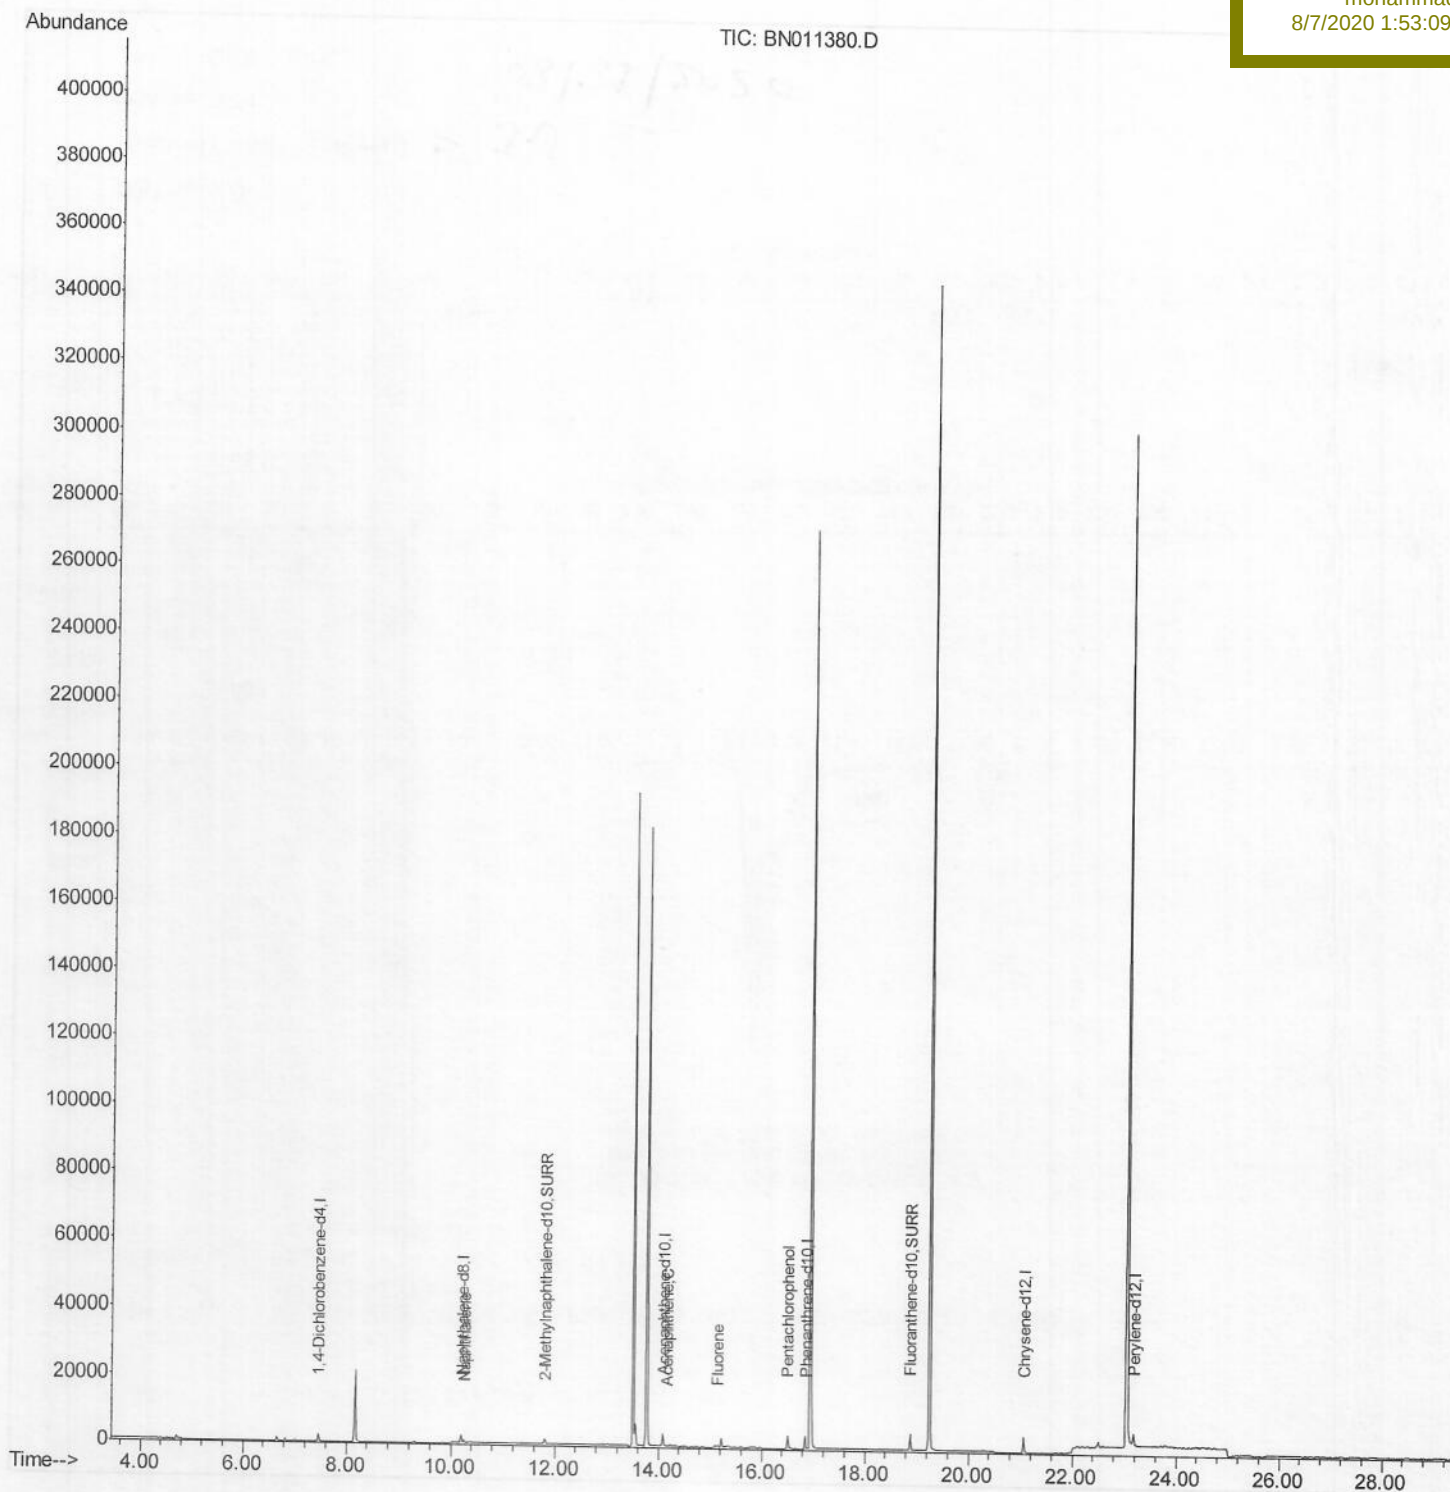

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
 Data File : BN011380.D
 Acq On : 06 Aug 2020 15:38
 Operator : CG/JU
 Sample : L3487-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 06 16:15:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 06 12:09:32 2020
 Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

F4L04

Manual Integrations
 APPROVED

mohammad
 8/7/2020 1:53:09 PM

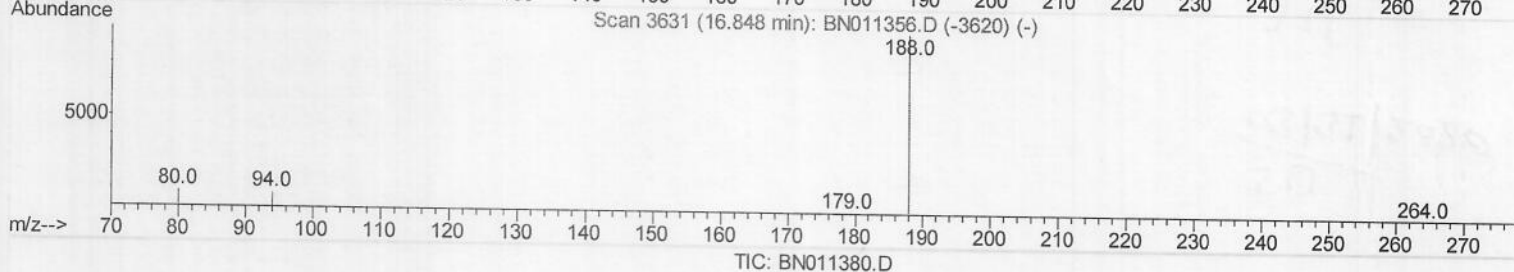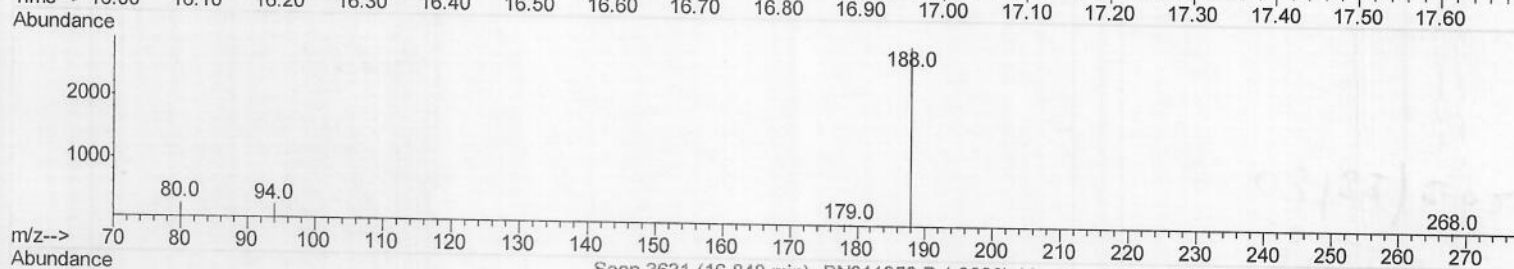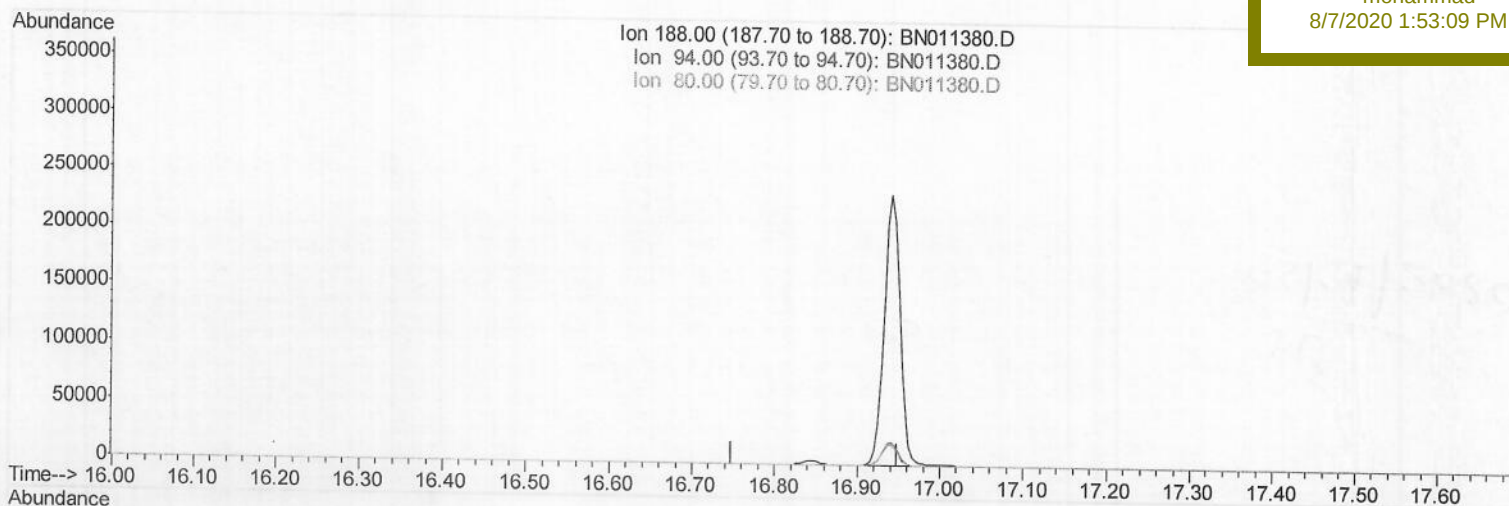

(10) Phenanthrene-d10 (I)

16.848min (-16.848) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
 Data File : BN011380.D
 Acq On : 06 Aug 2020 15:38
 Operator : CG/JU
 Sample : L3487-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 06 16:15:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 06 12:09:32 2020
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 F4L04

Manual Integrations
 APPROVED

mohammad
 8/7/2020 1:53:09 PM

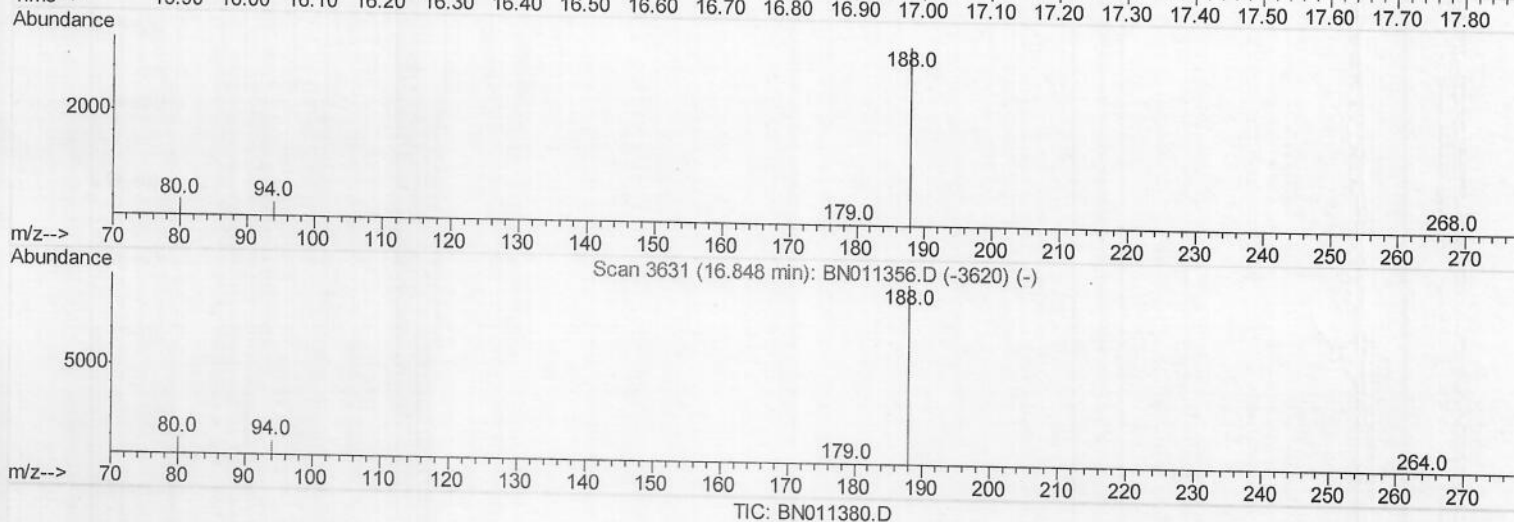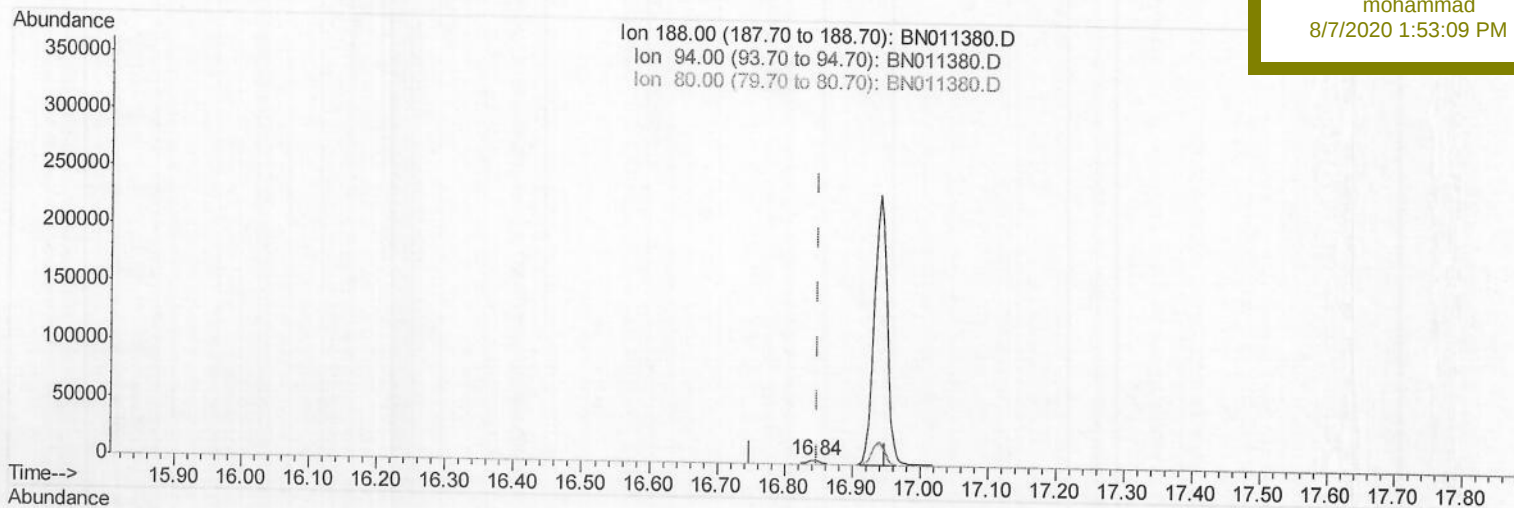

(10) Phenanthrene-d10 (I)

16.844min (-0.004) 0.40ng/ul m

response 4661

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	8.99
80.00	10.30	9.95
0.00	0.00	0.00

730 08/07/20

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN080620\
 Data File : BN011380.D
 Acq On : 06 Aug 2020 15:38
 Operator : CG/JU
 Sample : L3487-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4L04

Quant Time: Aug 06 16:16:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 06 12:09:32 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 8/7/2020 1:53:09 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1080	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	3333	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.09	164	1957	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.84	188	4661m	0.40	ng/ul	0.00
16) Chrysene-d12	21.06	240	4515	0.40	ng/ul	0.00
20) Perylene-d12	23.18	264	4837	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.80	152	2085	0.25	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	5473	0.24	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.25	128	923	0.093	ng/ul#	84
8) Acenaphthene	14.15	153	170	0.023	ng/ul#	88
9) Fluorene	15.15	166	458	0.052	ng/ul#	96
11) Pentachlorophenol	16.51	266	2636	2.307	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

25008/07/20