

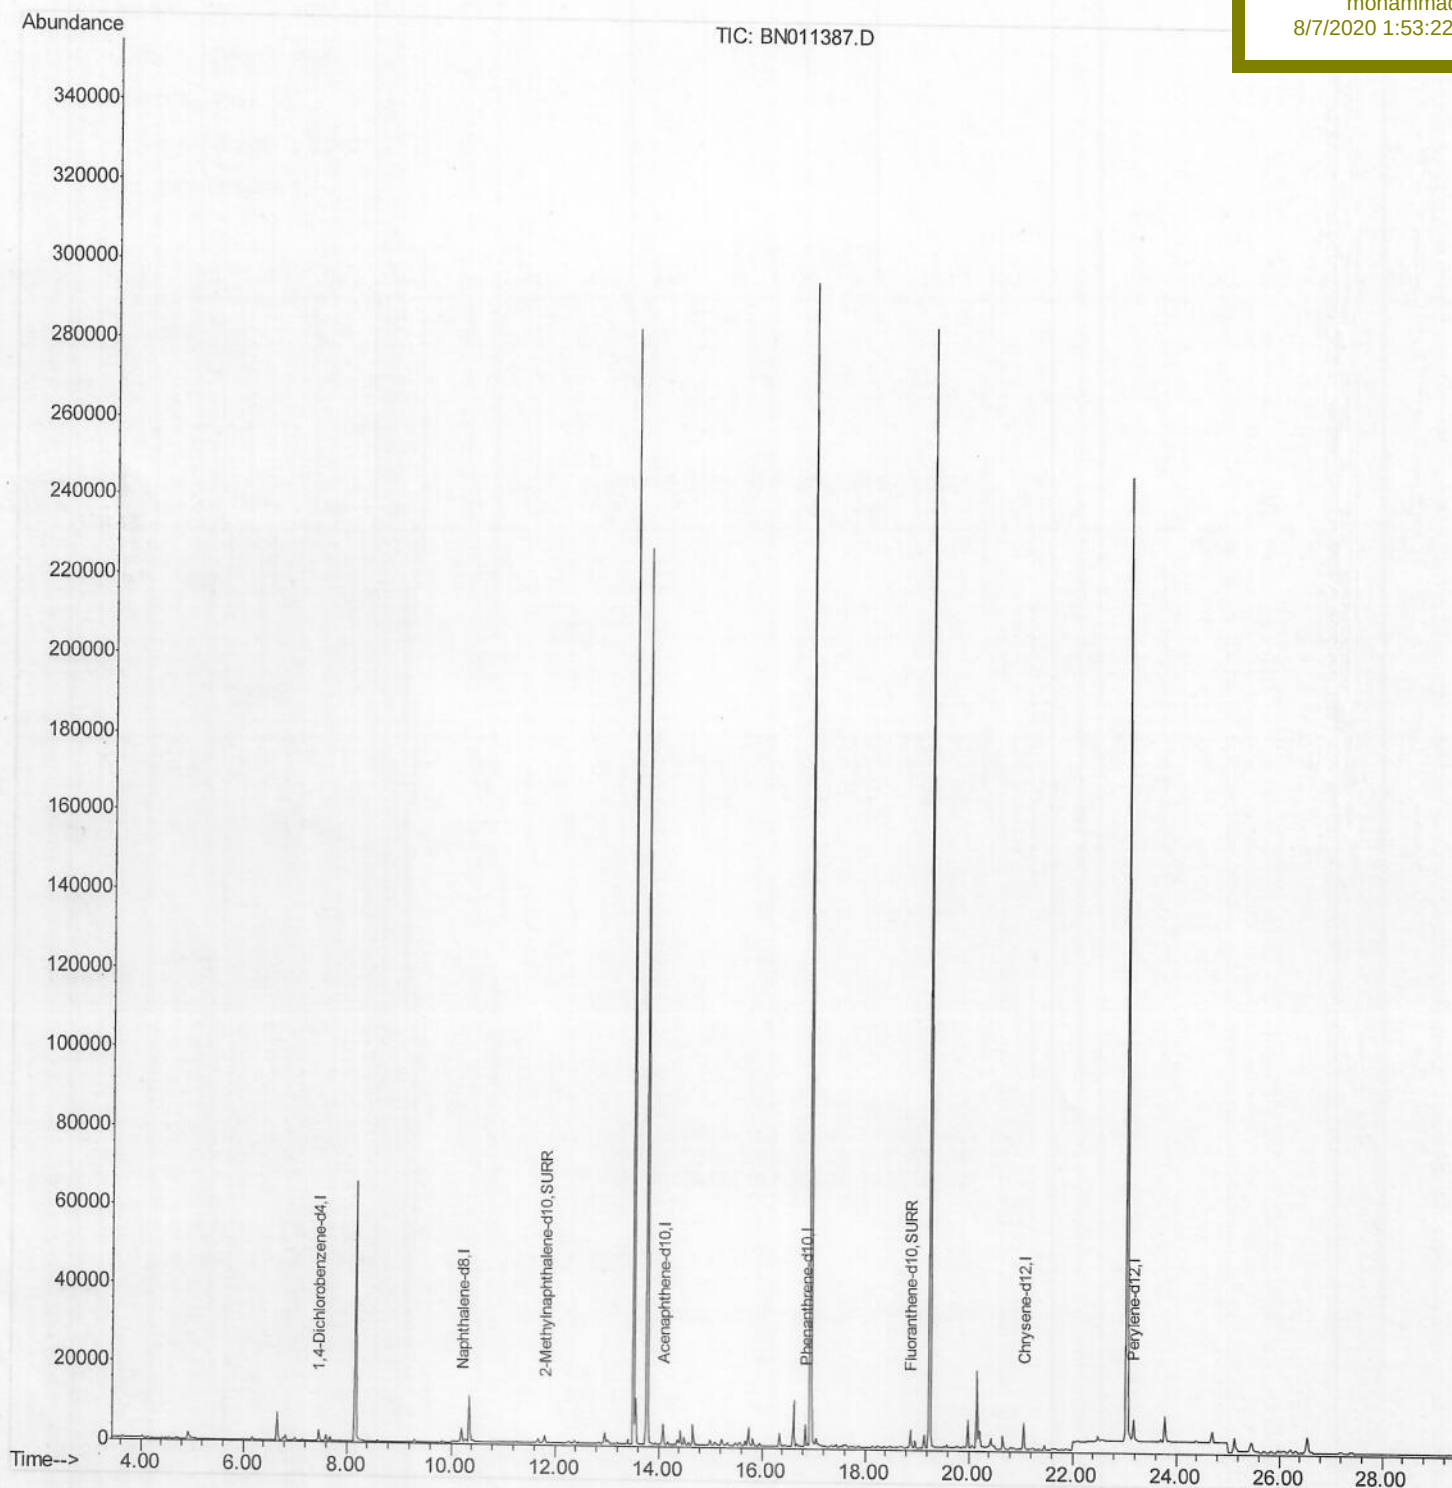
Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\
Data File : BN011387.D
Acq On : 06 Aug 2020 19:49
Operator : CG/JU
Sample : L3419-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 07 02:15:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 07 02:04:45 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/7/2020 1:53:22 PM



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\

Data File : BN011387.D

Acq On : 06 Aug 2020 19:49

Operator : CG/JU

Sample : L3419-14

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 07 02:06:25 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Aug 07 02:04:45 2020

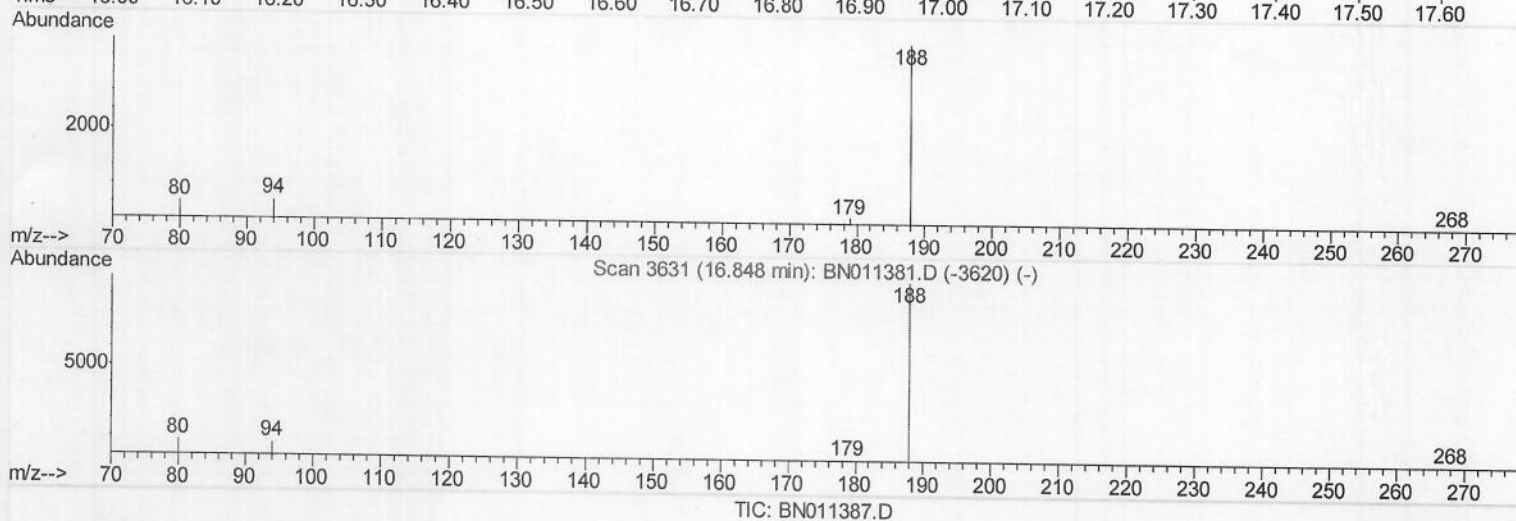
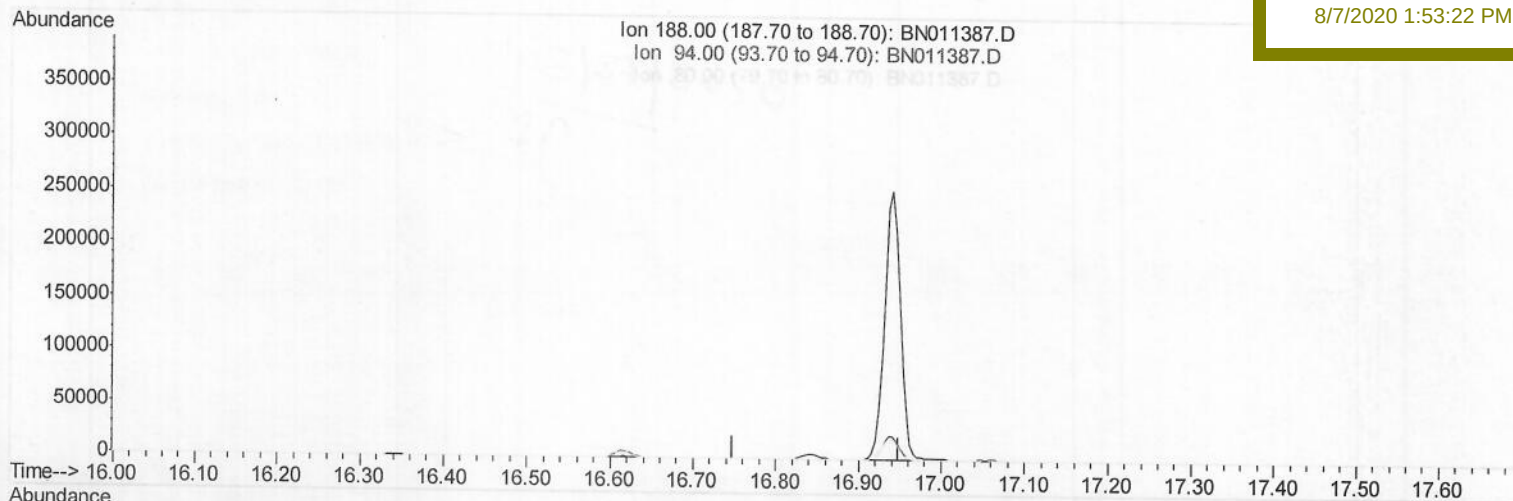
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF1

Manual Integrations
APPROVEDmohammad
8/7/2020 1:53:22 PM

(10) Phenanthrene-d10 (I)

16.848min (-16.848) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.90	0.00#
80.00	10.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\

Data File : BN011387.D

Acq On : 06 Aug 2020 19:49

Operator : CG/JU

Sample : L3419-14

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 07 02:06:25 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Aug 07 02:04:45 2020

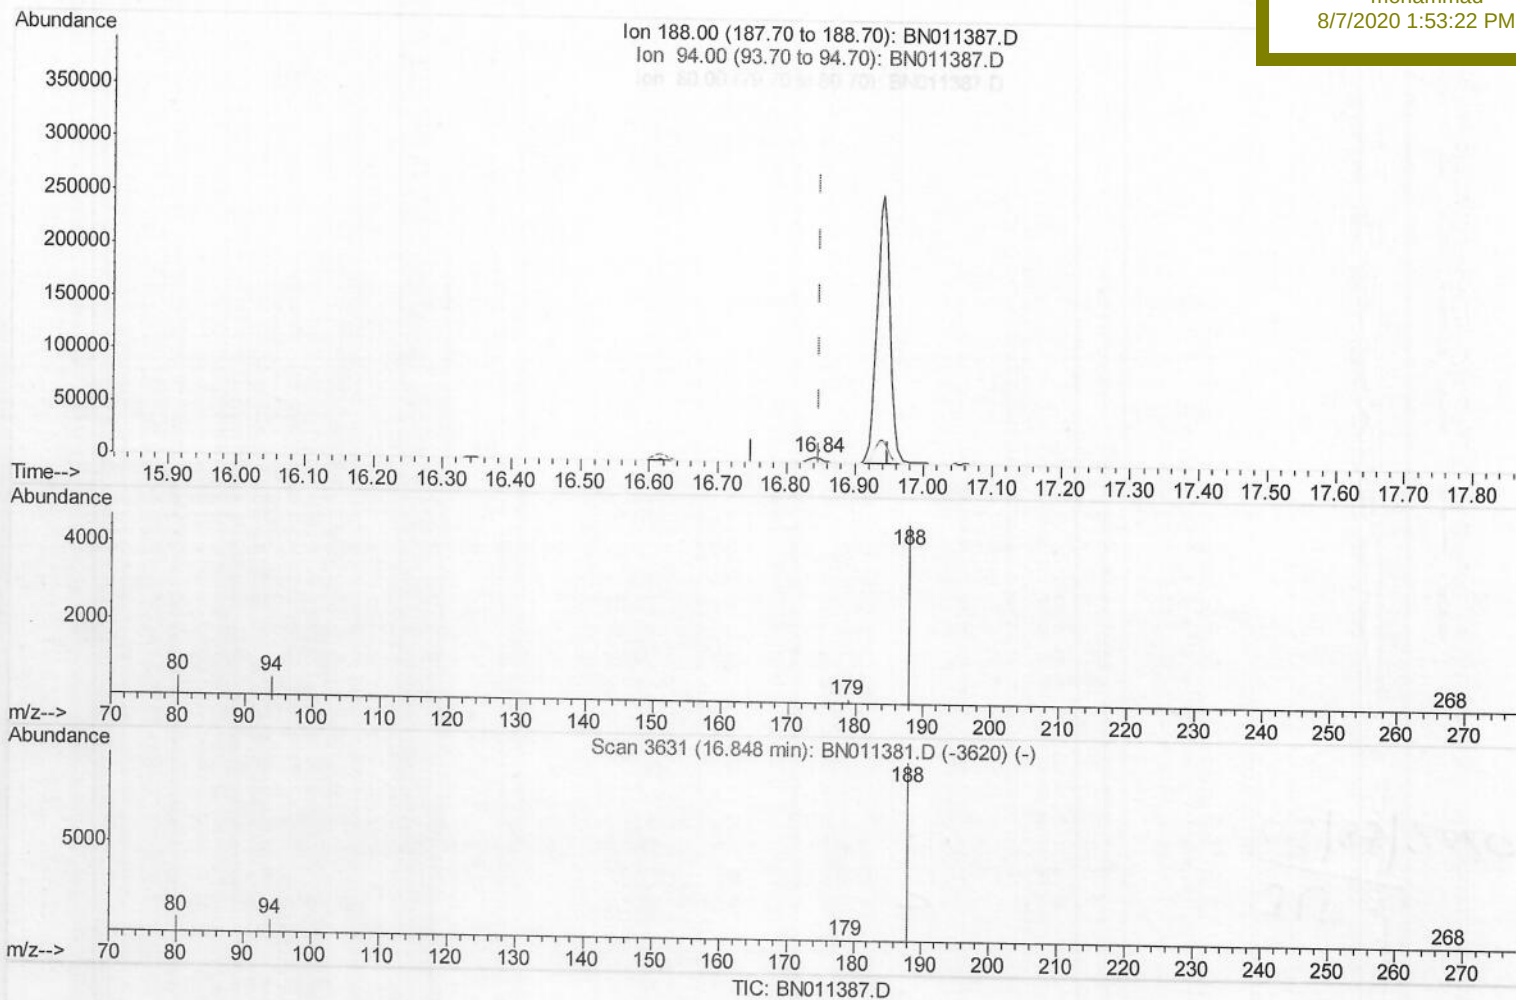
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

C0AF1

Manual Integrations
APPROVEDmohammad
8/7/2020 1:53:22 PM

(10) Phenanthrene-d10 (I)

16.844min (-0.004) 0.40ng/ul m

response 6465

Ion	Exp%	Act%
188.00	100	100
94.00	8.90	11.48#
80.00	10.30	11.27
0.00	0.00	0.00

7 JU 08/07/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080620\
Data File : BN011387.D
Acq On : 06 Aug 2020 19:49
Operator : CG/JU
Sample : L3419-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 07 02:15:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 07 02:04:45 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/7/2020 1:53:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	1381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.20	136	4655	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.09	164	2840	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.84	188	6465m	0.40	ng/ul	0.00
16) Chrysene-d12	21.06	240	6350	0.40	ng/ul	0.00
20) Perylene-d12	23.17	264	6713	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.80	152	2354	0.20	ng/ul	-0.01
14) Fluoranthene-d10	18.88	212	4929	0.16	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JSU 08/07/20