
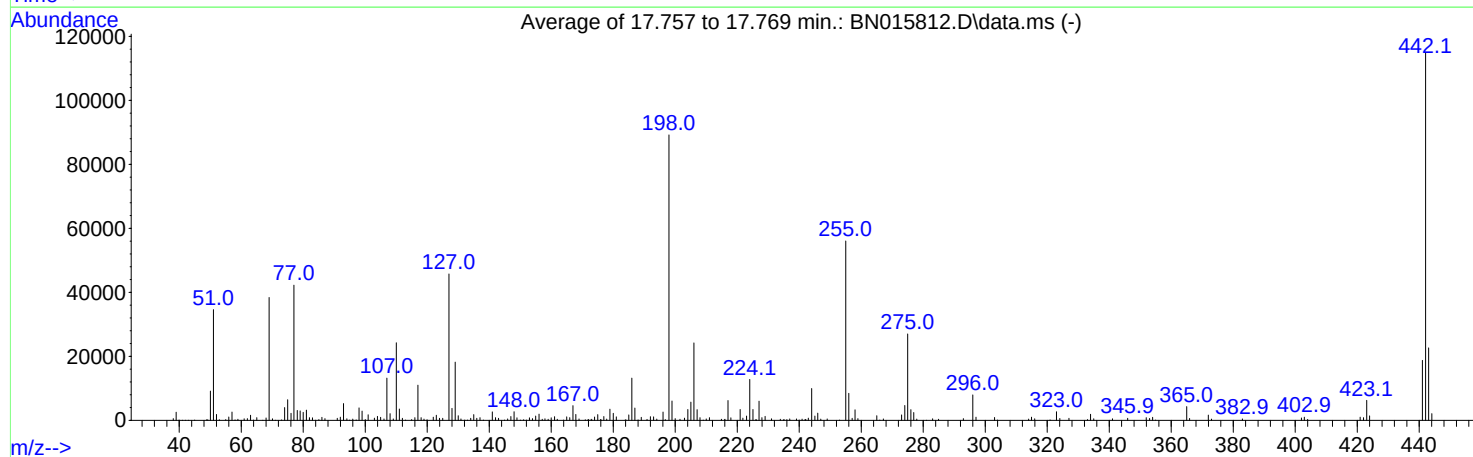


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080621\
 Data File : BN015812.D
 Acq On : 06 Aug 2021 17:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 07 04:36:21 2021

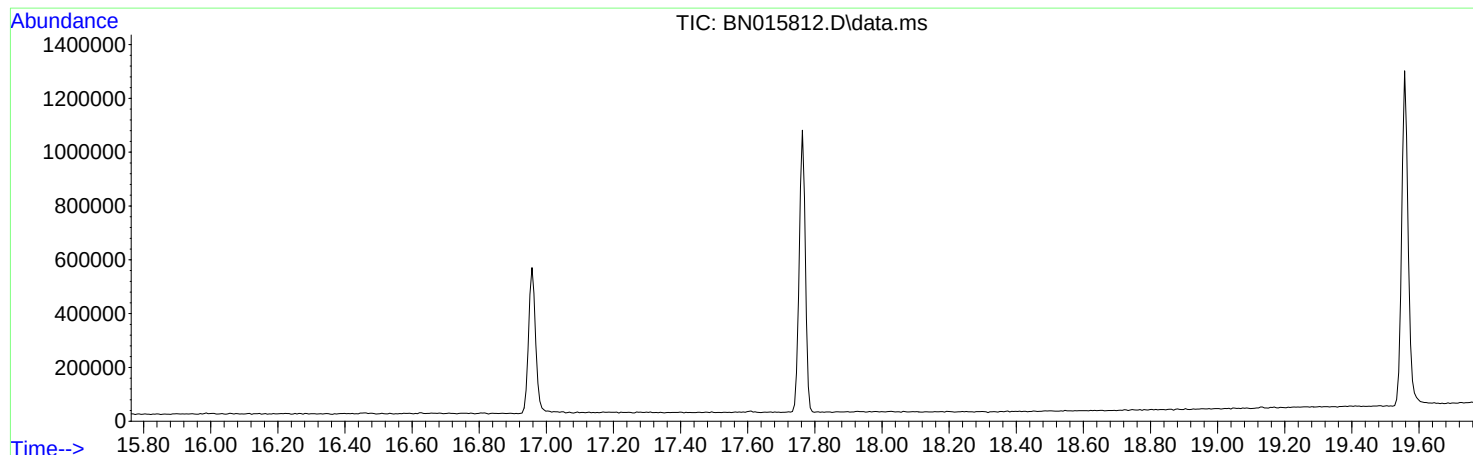

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	34611	PASS
68	69	0.00	2	1.9	748	PASS
69	198	0.00	100	43.1	38420	PASS
70	69	0.00	2	1.4	522	PASS
127	198	10	80	51.3	45739	PASS
197	198	0.00	2	0.3	248	PASS
198	198	100	100	100.0	89200	PASS
199	198	5	9	6.8	6033	PASS
275	198	10	60	30.3	26995	PASS
365	198	1	100	4.8	4325	PASS
441	198	0.01	100	21.0	18749	PASS
442	442	50	100	100.0	114973	PASS
443	442	15	24	19.7	22651	PASS