
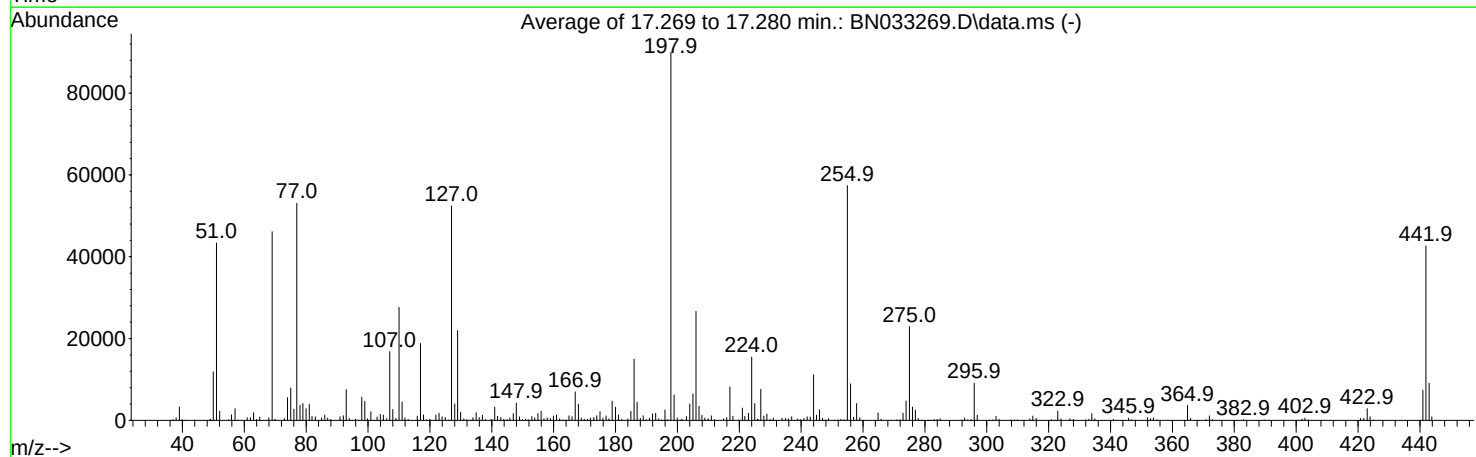


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080624\
Data File : BN033269.D
Acq On : 06 Aug 2024 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 05 23:57:48 2024

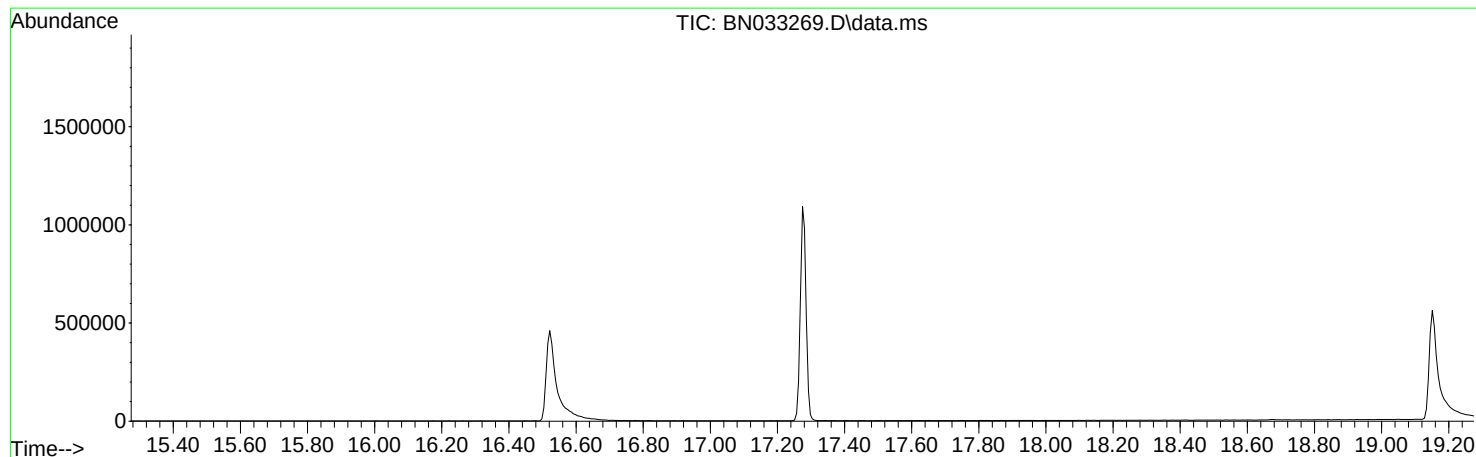




AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	43379	PASS
68	69	0.00	2	1.2	573	PASS
69	198	0.00	100	51.3	46109	PASS
70	69	0.00	2	0.6	256	PASS
127	198	10	80	58.3	52397	PASS
197	198	0.00	2	0.1	125	PASS
198	198	100	100	100.0	89928	PASS
199	198	5	9	6.9	6205	PASS
275	198	10	60	25.5	22919	PASS
365	198	1	100	4.1	3654	PASS
441	198	0.01	100	8.2	7401	PASS
442	442	50	100	100.0	42683	PASS
443	442	15	24	21.3	9090	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080624\
Data File : BN033269.D
Acq On : 06 Aug 2024 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 13:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

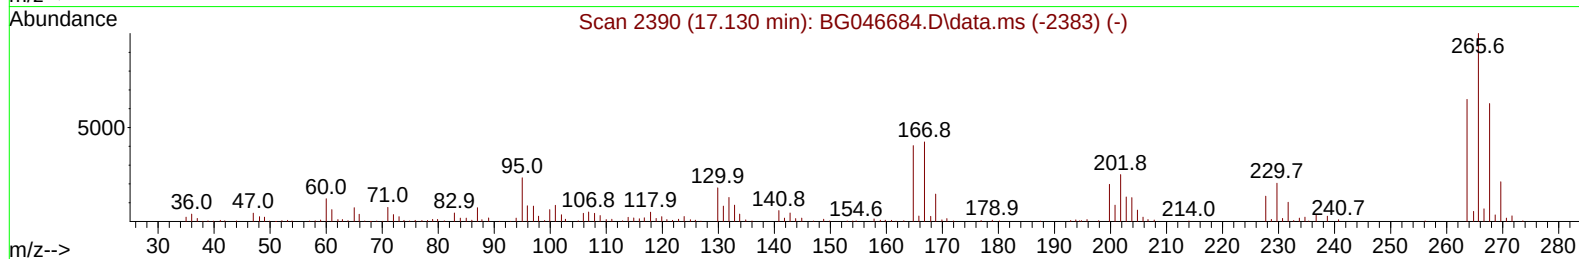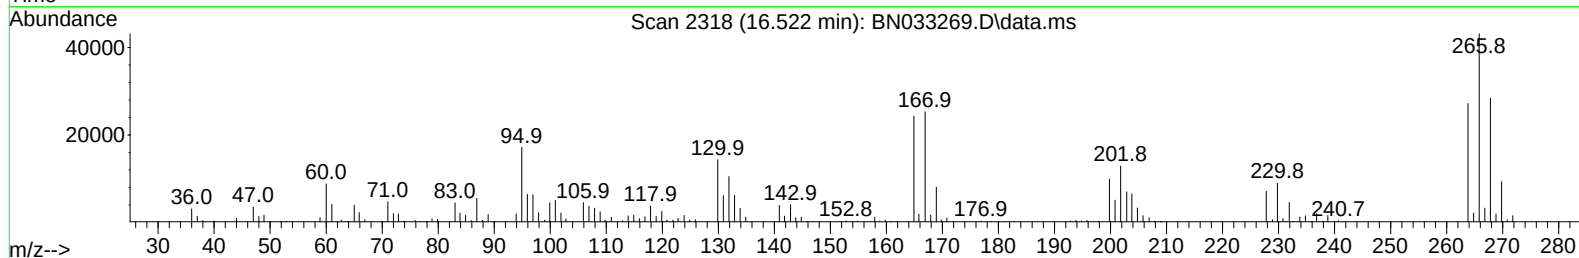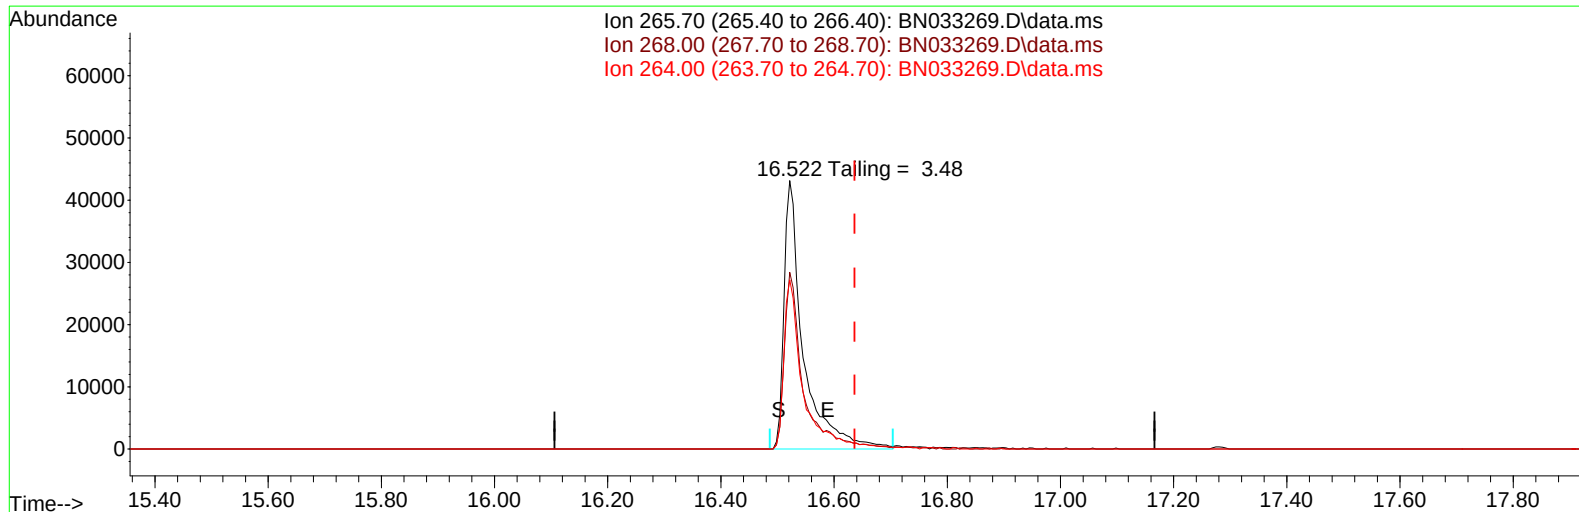

TIC: BN033269.D\data.ms

(70) Pentachlorophenol (C)

16.522min (-0.114) 21165.06 ng




response 101652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.84
264.00	61.60	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080624\
Data File : BN033269.D
Acq On : 06 Aug 2024 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 13:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

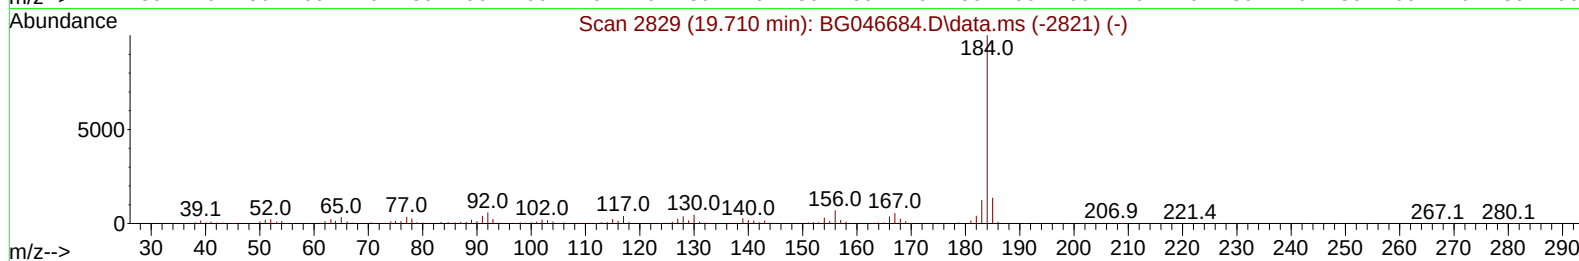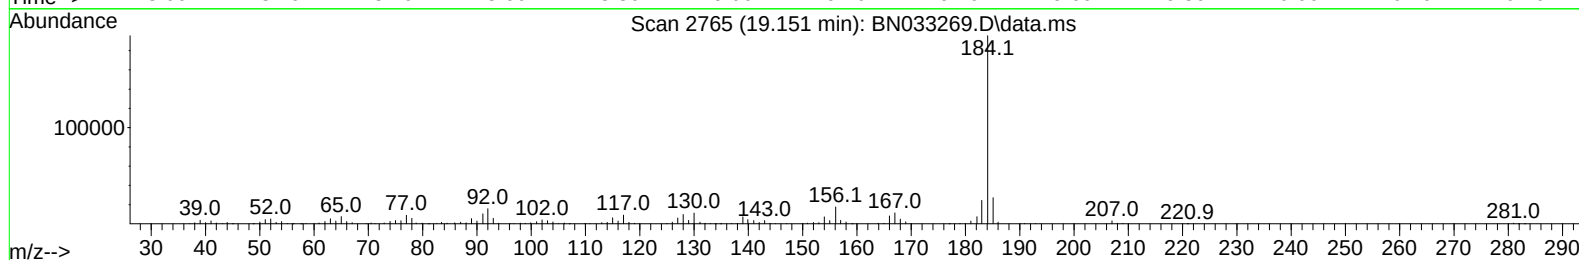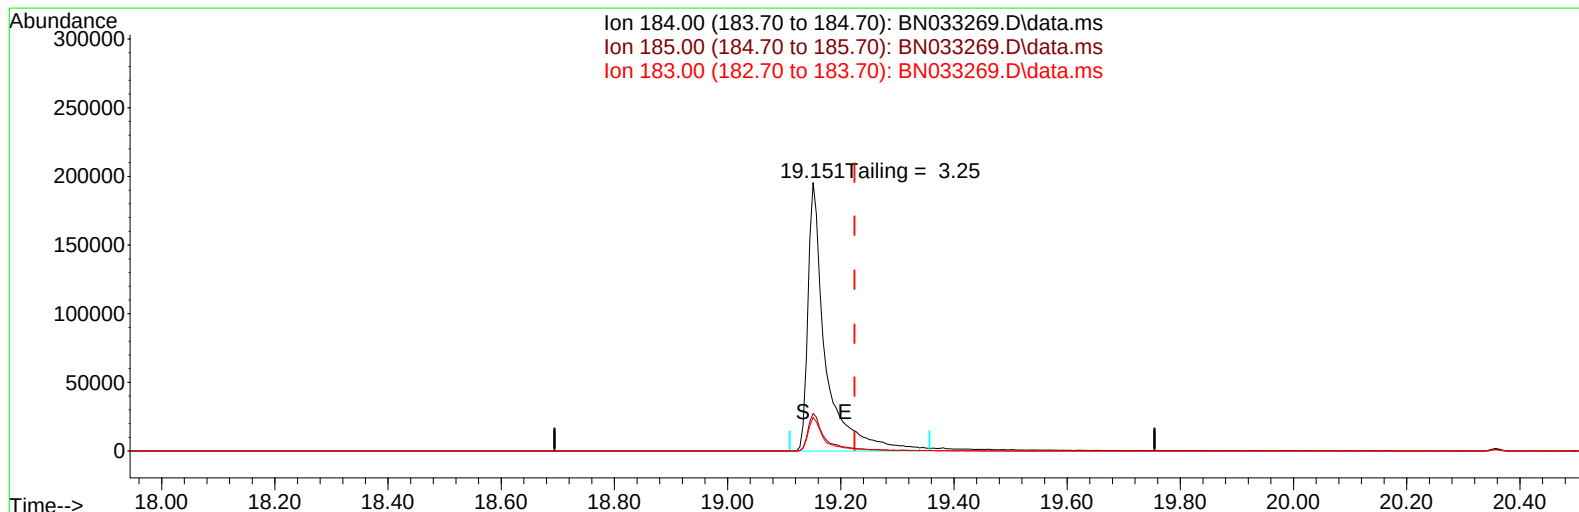

TIC: BN033269.D\data.ms

(77) Benzidine

19.151min (-0.073) 0.00 ng m

response 423776

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/6/2024	BNA_N	<u>BN033269.D</u>
Compound Name	Response	Retention Time
DDT	360019	20.357
DDD	4228	19.963
DDE	138	19.416
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4366	364385	1.20

Instrument :
BNA_N
ClientSampleId :
DFTPP