
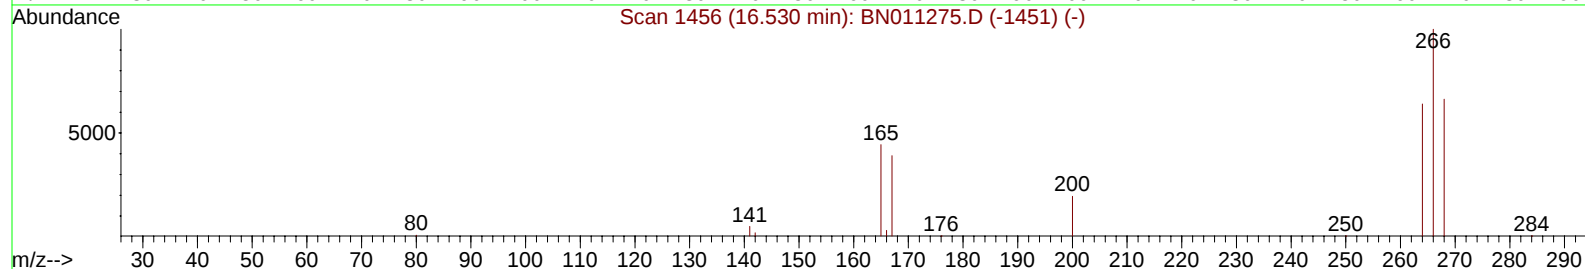
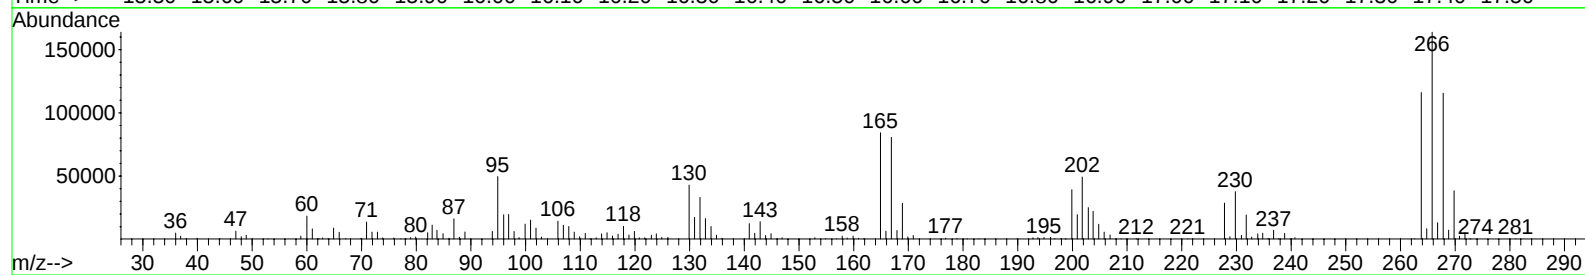


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080720\
 Data File : BN011391.D
 Acq On : 07 Aug 2020 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 16:51:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN072820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 31 12:17:46 2020
 Response via : Initial Calibration

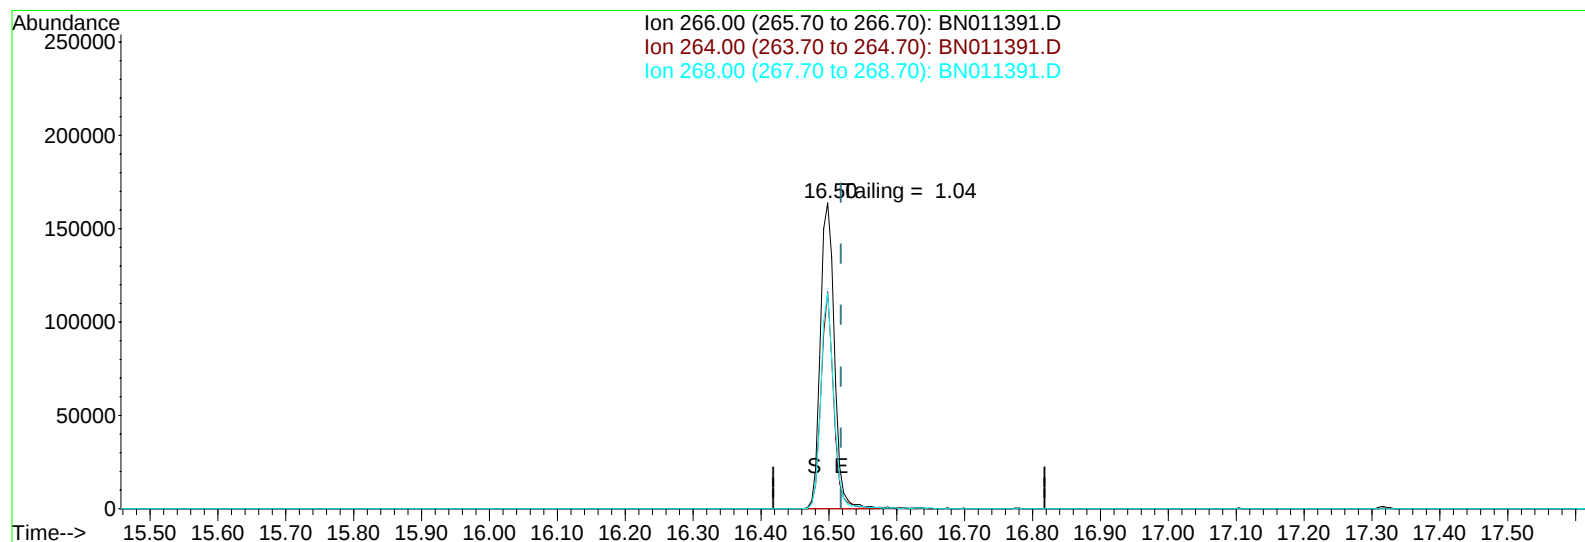

TIC: BN011391.D

(24) Pentachlorophenol

16.498min (-0.020) 8148.39ng

response 237604

Ion	Exp%	Act%
266.00	100	100
264.00	63.90	62.79
268.00	69.40	64.79
0.00	0.00	0.00