


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080720\
 Data File : BN011391.D
 Acq On : 07 Aug 2020 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 31 12:17:46 2020

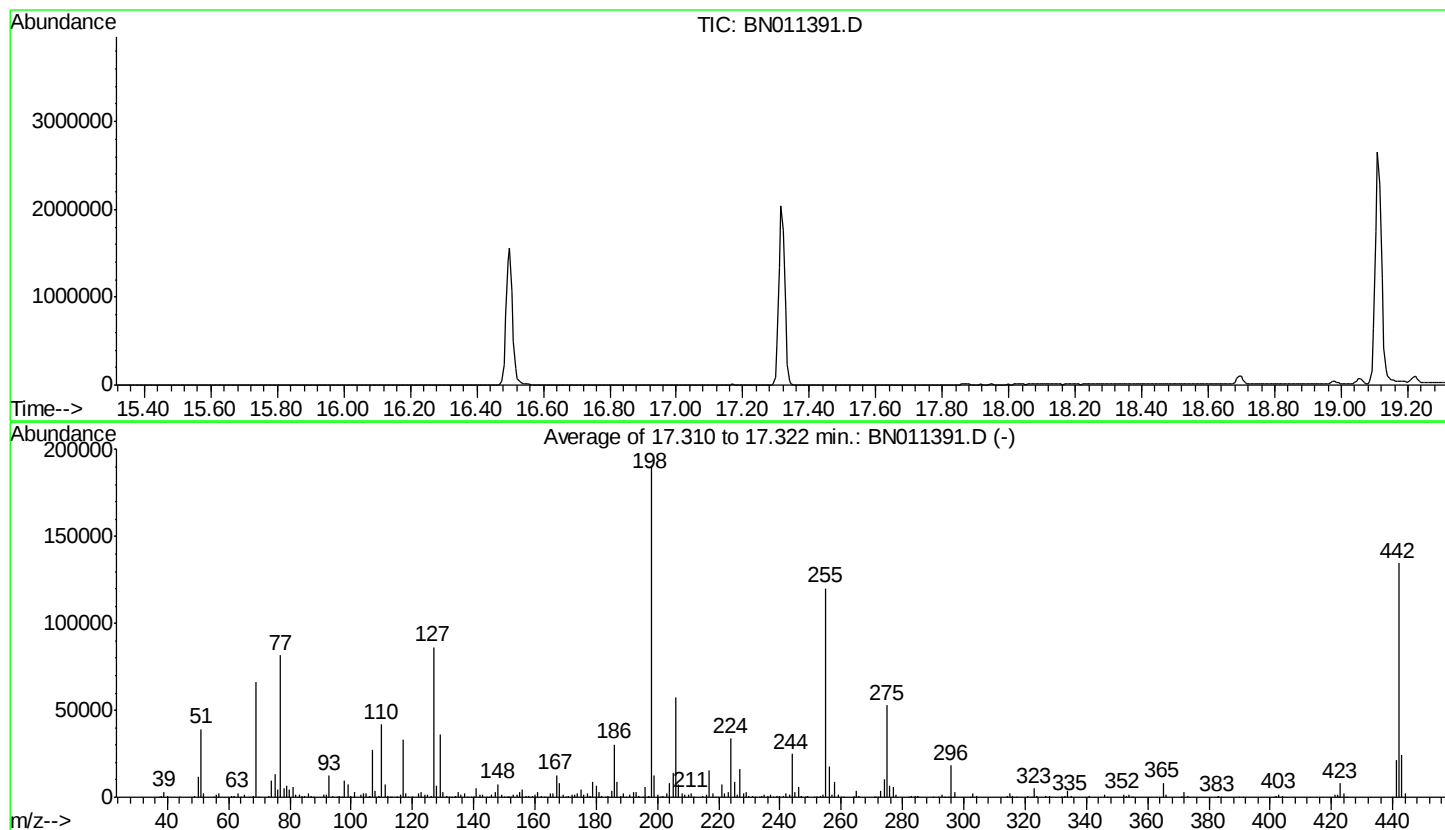

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2429

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.6	39221	PASS
68	69	0.00	2	1.2	816	PASS
69	198	0.00	100	34.6	65986	PASS
70	69	0.00	2	0.6	391	PASS
127	198	10	80	45.2	86218	PASS
197	198	0.00	2	0.4	820	PASS
198	198	100	100	100.0	190784	PASS
199	198	5	9	6.4	12302	PASS
275	198	10	60	27.6	52736	PASS
365	198	1	100	4.4	8375	PASS
441	198	0.01	100	11.1	21095	PASS
442	198	50	100	70.5	134522	PASS
443	442	15	24	18.1	24359	PASS