

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
 Data File : BN021092.D
 Acq On : 09 Aug 2022 19:22
 Operator : CG/JU
 Sample : N4069-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 09 23:13:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	3220	0.400	ng/ul	0.00
4) Naphthalene-d8	10.585	136	10789	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.443	164	6357	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.193	188	12716	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240	10240	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	8848	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	14736	3.577	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	4831	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	13027	0.412	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.593	202	1788	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.575	252	2902	0.078	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
Data File : BN021092.D
Acq On : 09 Aug 2022 19:22
Operator : CG/JU
Sample : N4069-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 09 23:13:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

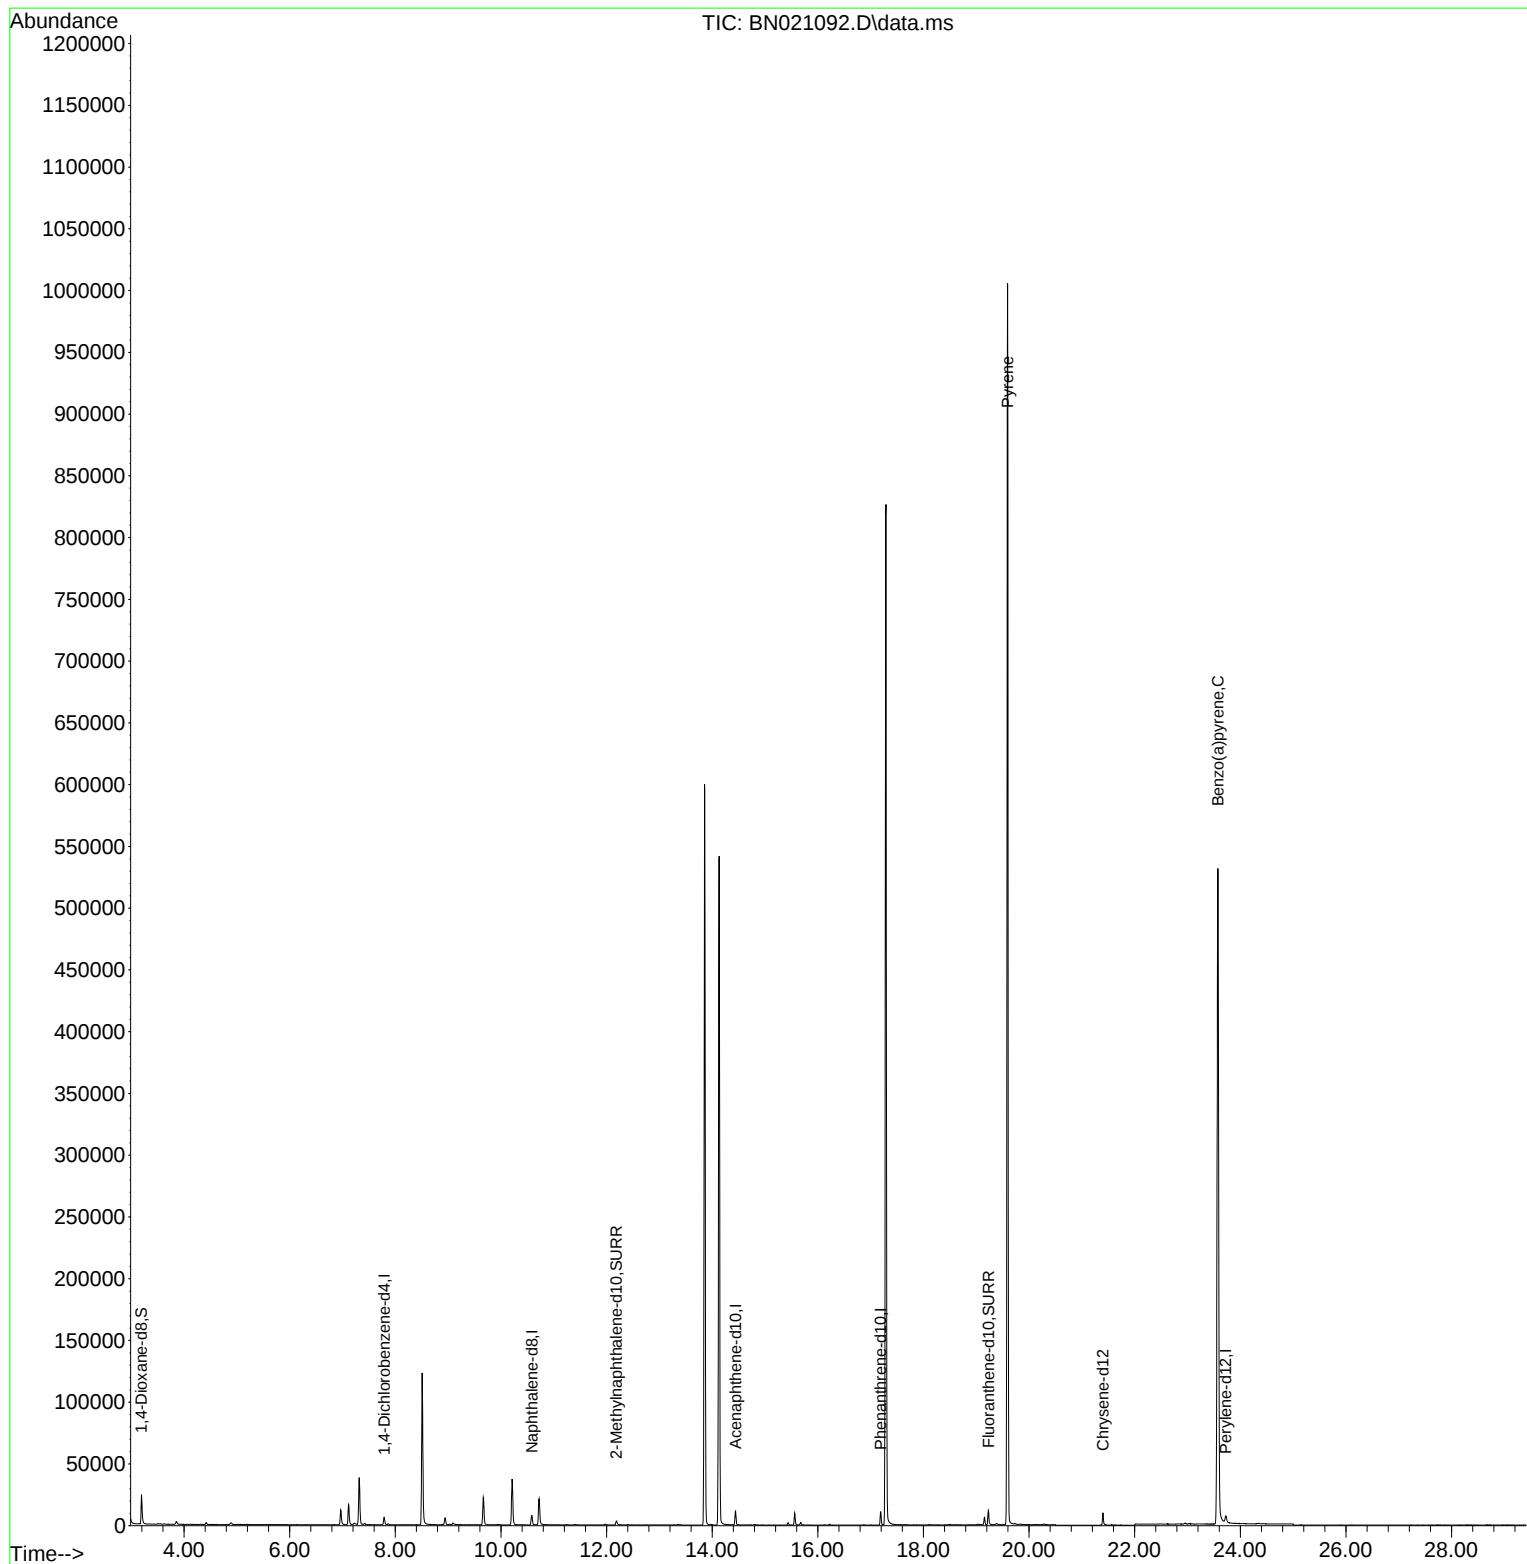

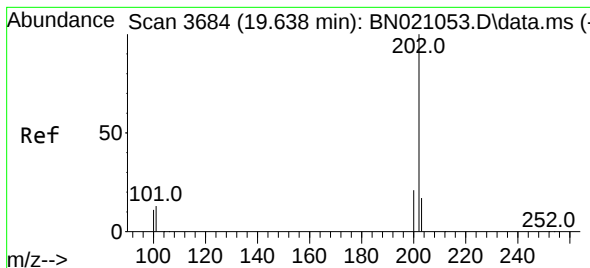

#20

Pyrene

Concen: 0.038 ng/u1

RT: 19.593 min Scan# 3

Delta R.T. -0.031 min

Lab File: BN021092.D

Acq: 09 Aug 2022 19:22

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:202 Resp: 1788

Ion Ratio Lower Upper

202 100

101 177.1 11.3 16.9#

100 1258.7 9.0 13.4#

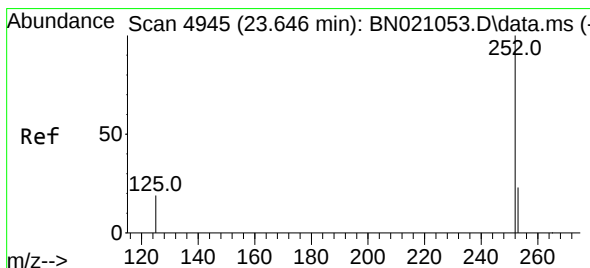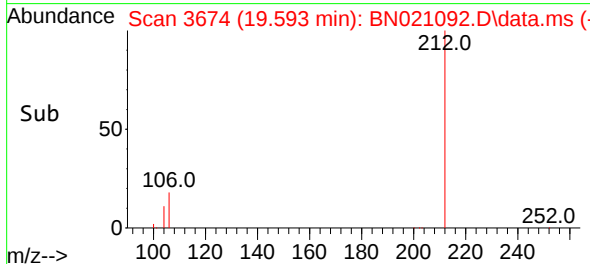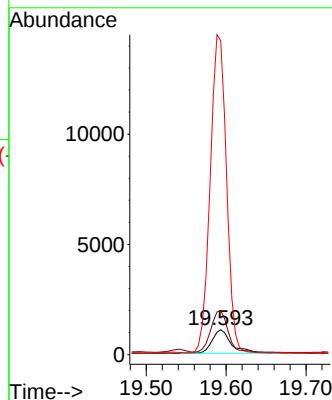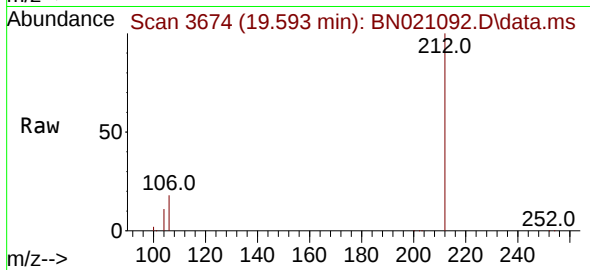

#26

Benzo(a)pyrene

Concen: 0.078 ng/u1

RT: 23.575 min Scan# 4921

Delta R.T. -0.059 min

Lab File: BN021092.D

Acq: 09 Aug 2022 19:22

Tgt Ion:252 Resp: 2902

Ion Ratio Lower Upper

252 100

253 47.9 22.1 33.1#

125 37.1 14.7 22.1#

