

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
 Data File : BN021085.D
 Acq On : 09 Aug 2022 14:55
 Operator : CG/JU
 Sample : N4069-17
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJM1

Quant Time: Aug 09 23:12:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	4068	0.400	ng/ul	0.00
4) Naphthalene-d8	10.585	136	13197	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.443	164	7834	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.189	188	15431	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240	11313	0.400	ng/ul	0.00
23) Perylene-d12	23.730	264	10336	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	18417	3.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	5822	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	14375	0.411	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.232	88	503	0.094	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
Data File : BN021085.D
Acq On : 09 Aug 2022 14:55
Operator : CG/JU
Sample : N4069-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJM1

Quant Time: Aug 09 23:12:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

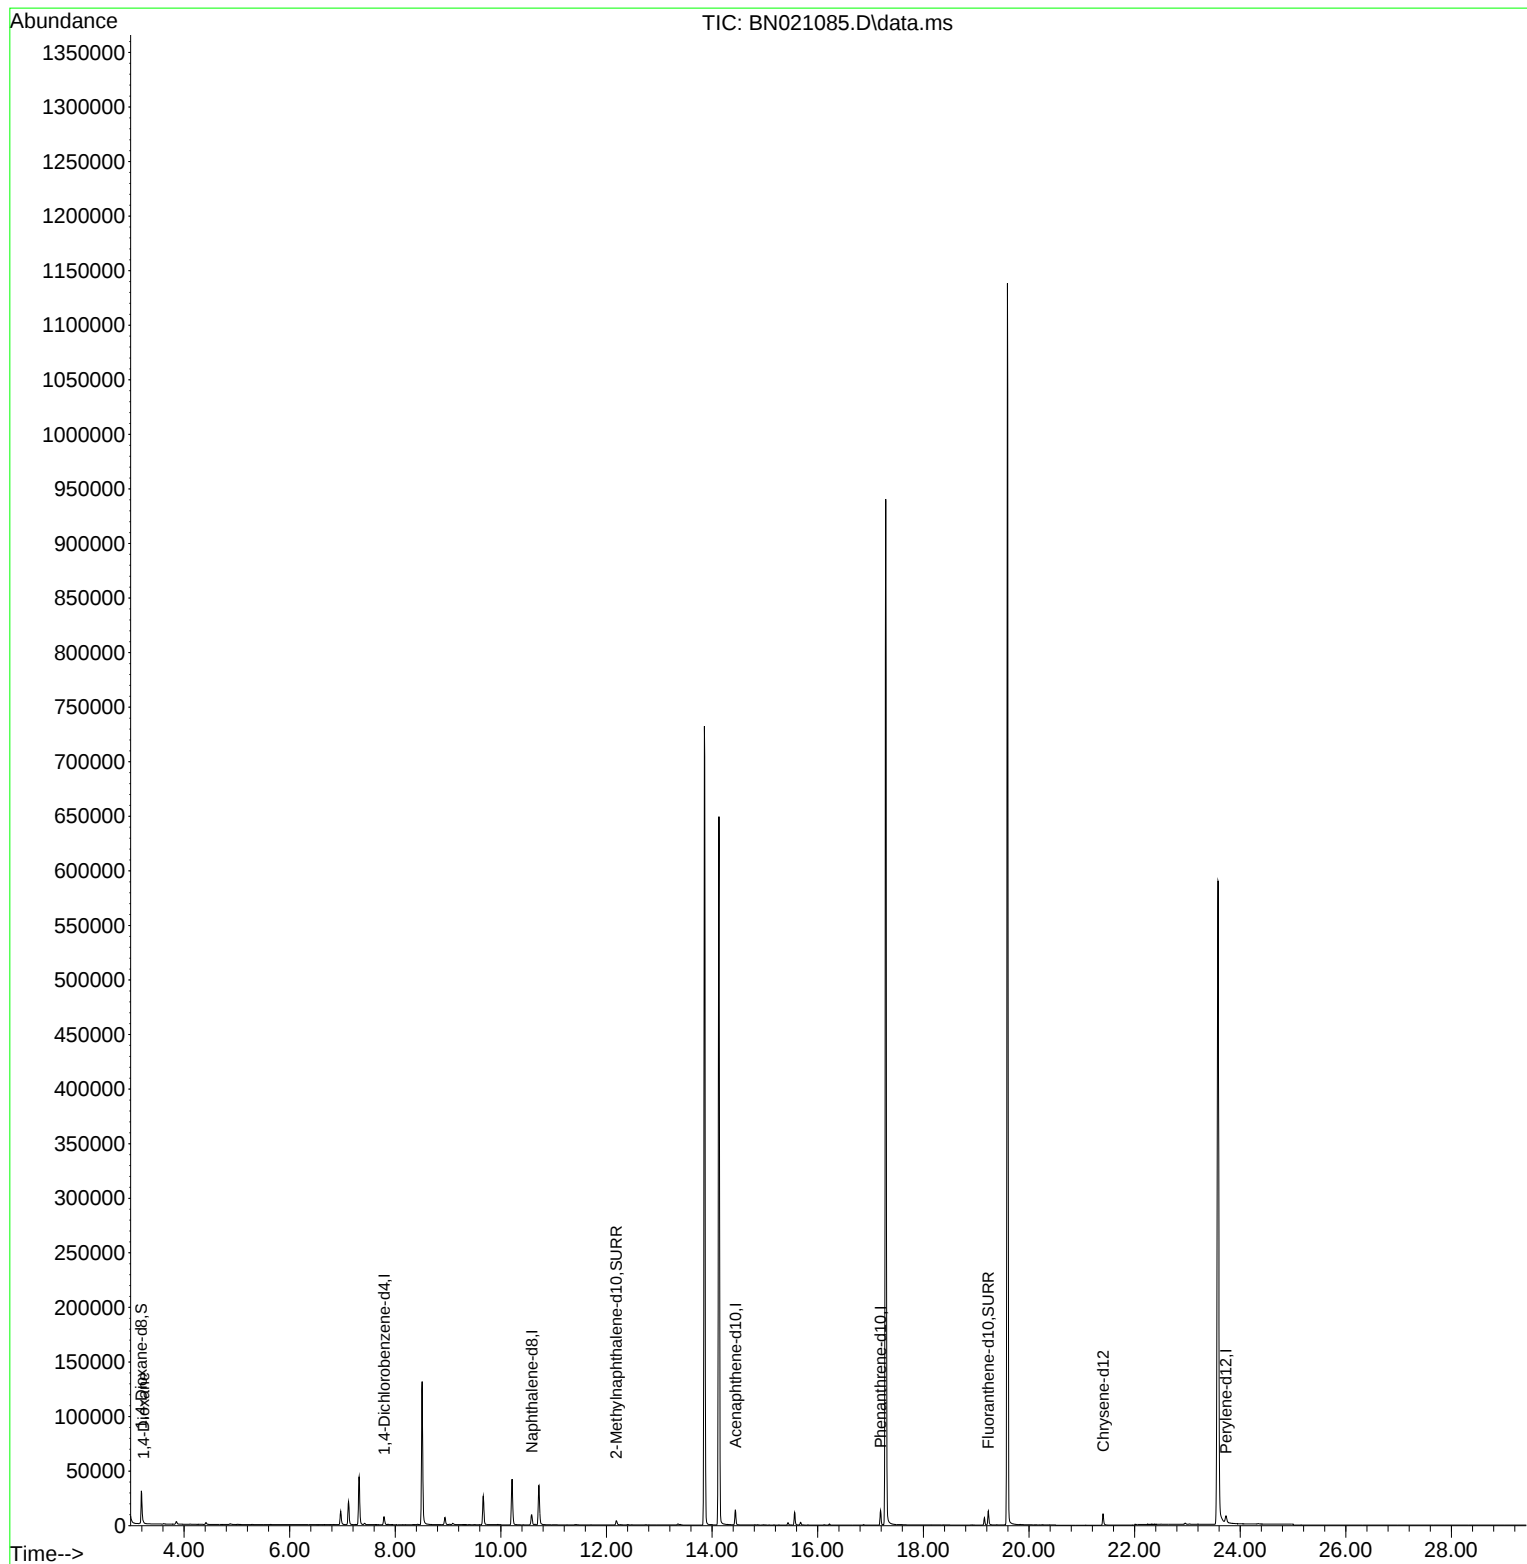

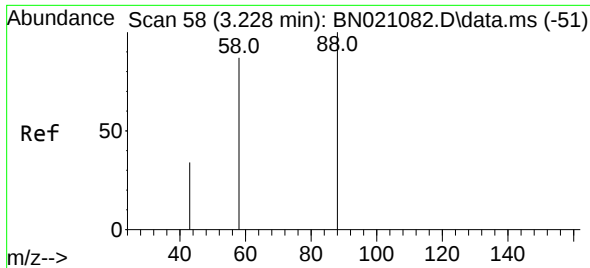

#2
 1,4-Dioxane
 Concen: 0.094 ng/ul
 RT: 3.232 min Scan# 59
 Delta R.T. 0.004 min
 Lab File: BN021085.D
 Acq: 09 Aug 2022 14:55

Instrument :
 BNA_N
 ClientSampleId :
 GBJM1

Tgt Ion:	88	Resp:	503
Ion	Ratio	Lower	Upper
88	100		
43	41.4	31.4	47.0
58	30.1	49.0	73.6

