

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
 Data File : BN021090.D
 Acq On : 09 Aug 2022 18:05
 Operator : CG/JU
 Sample : N4069-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJL9

Quant Time: Aug 09 23:13:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	3433	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	11508	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.442	164	6781	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.192	188	13635	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	10600	0.400	ng/ul	0.00
23) Perylene-d12	23.722	264	10004	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	17955	4.088	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.190	152	5774	0.342	ng/ul	0.01
18) Fluoranthene-d10	19.230	212	14485	0.442	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.228	88	261	0.058	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
Data File : BN021090.D
Acq On : 09 Aug 2022 18:05
Operator : CG/JU
Sample : N4069-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJL9


Quant Time: Aug 09 23:13:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

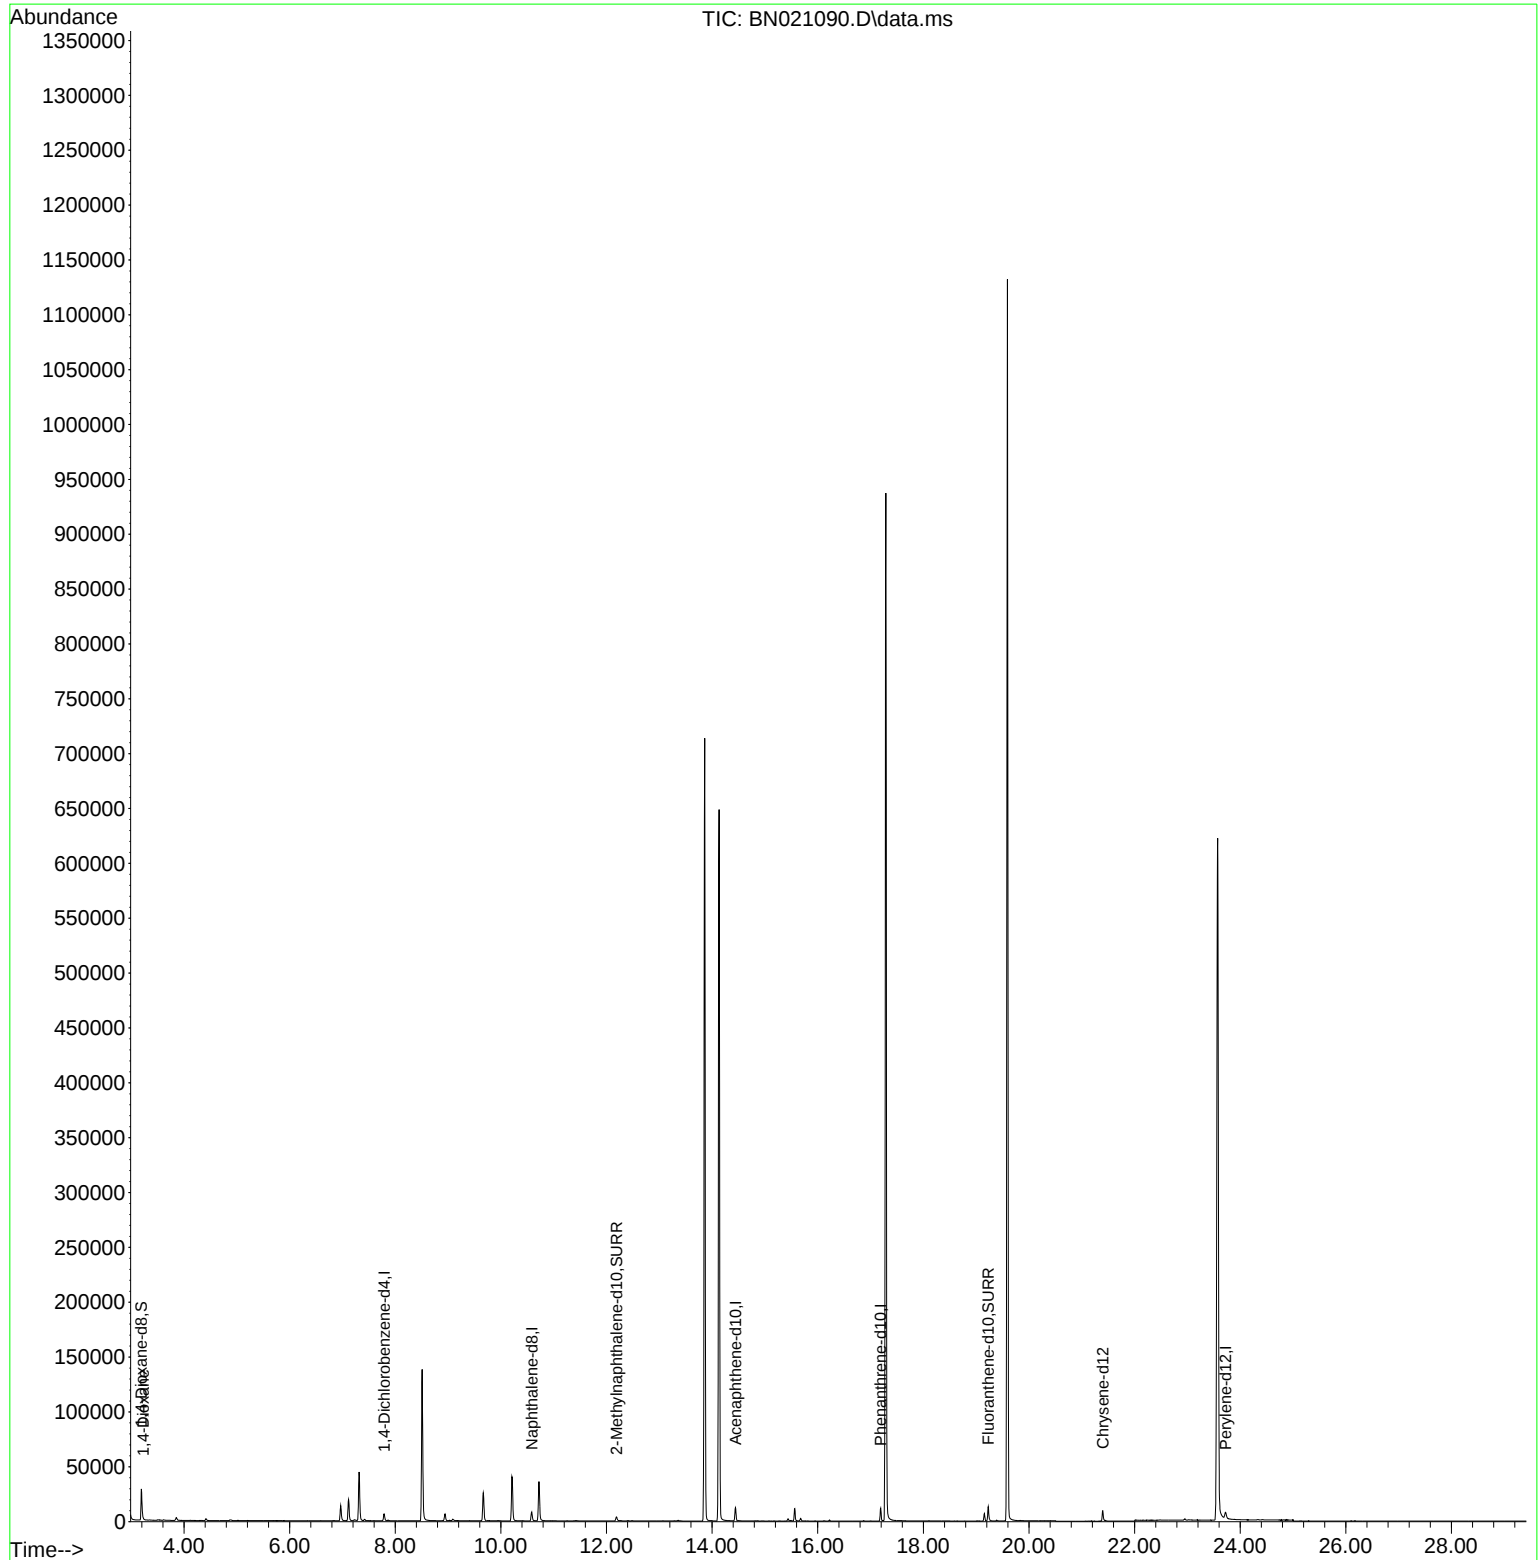

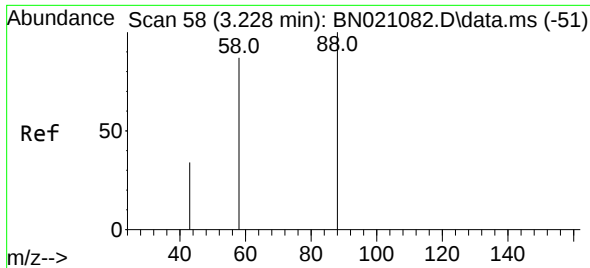

#2
 1,4-Dioxane
 Concen: 0.058 ng/ul
 RT: 3.228 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BN021090.D
 Acq: 09 Aug 2022 18:05

Instrument :
 BNA_N
 ClientSampleId :
 GBJL9

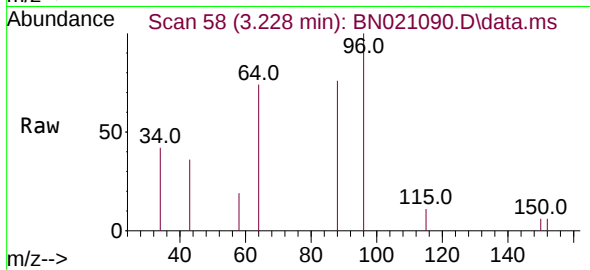

Tgt Ion:	88	Resp:	261
Ion	Ratio	Lower	Upper
88	100		
43	47.6	31.4	47.0#
58	25.2	49.0	73.6#

