

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
 Data File : BN021091.D
 Acq On : 09 Aug 2022 18:44
 Operator : CG/JU
 Sample : N4069-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJK4

Quant Time: Aug 09 23:13:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	3291	0.400	ng/ul	0.00
4) Naphthalene-d8	10.585	136	10941	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.443	164	6452	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	13171	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	10517	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	9244	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	16855	4.003	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	5526	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	13763	0.424	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.228	88	304	0.070	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
Data File : BN021091.D
Acq On : 09 Aug 2022 18:44
Operator : CG/JU
Sample : N4069-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJK4

Quant Time: Aug 09 23:13:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

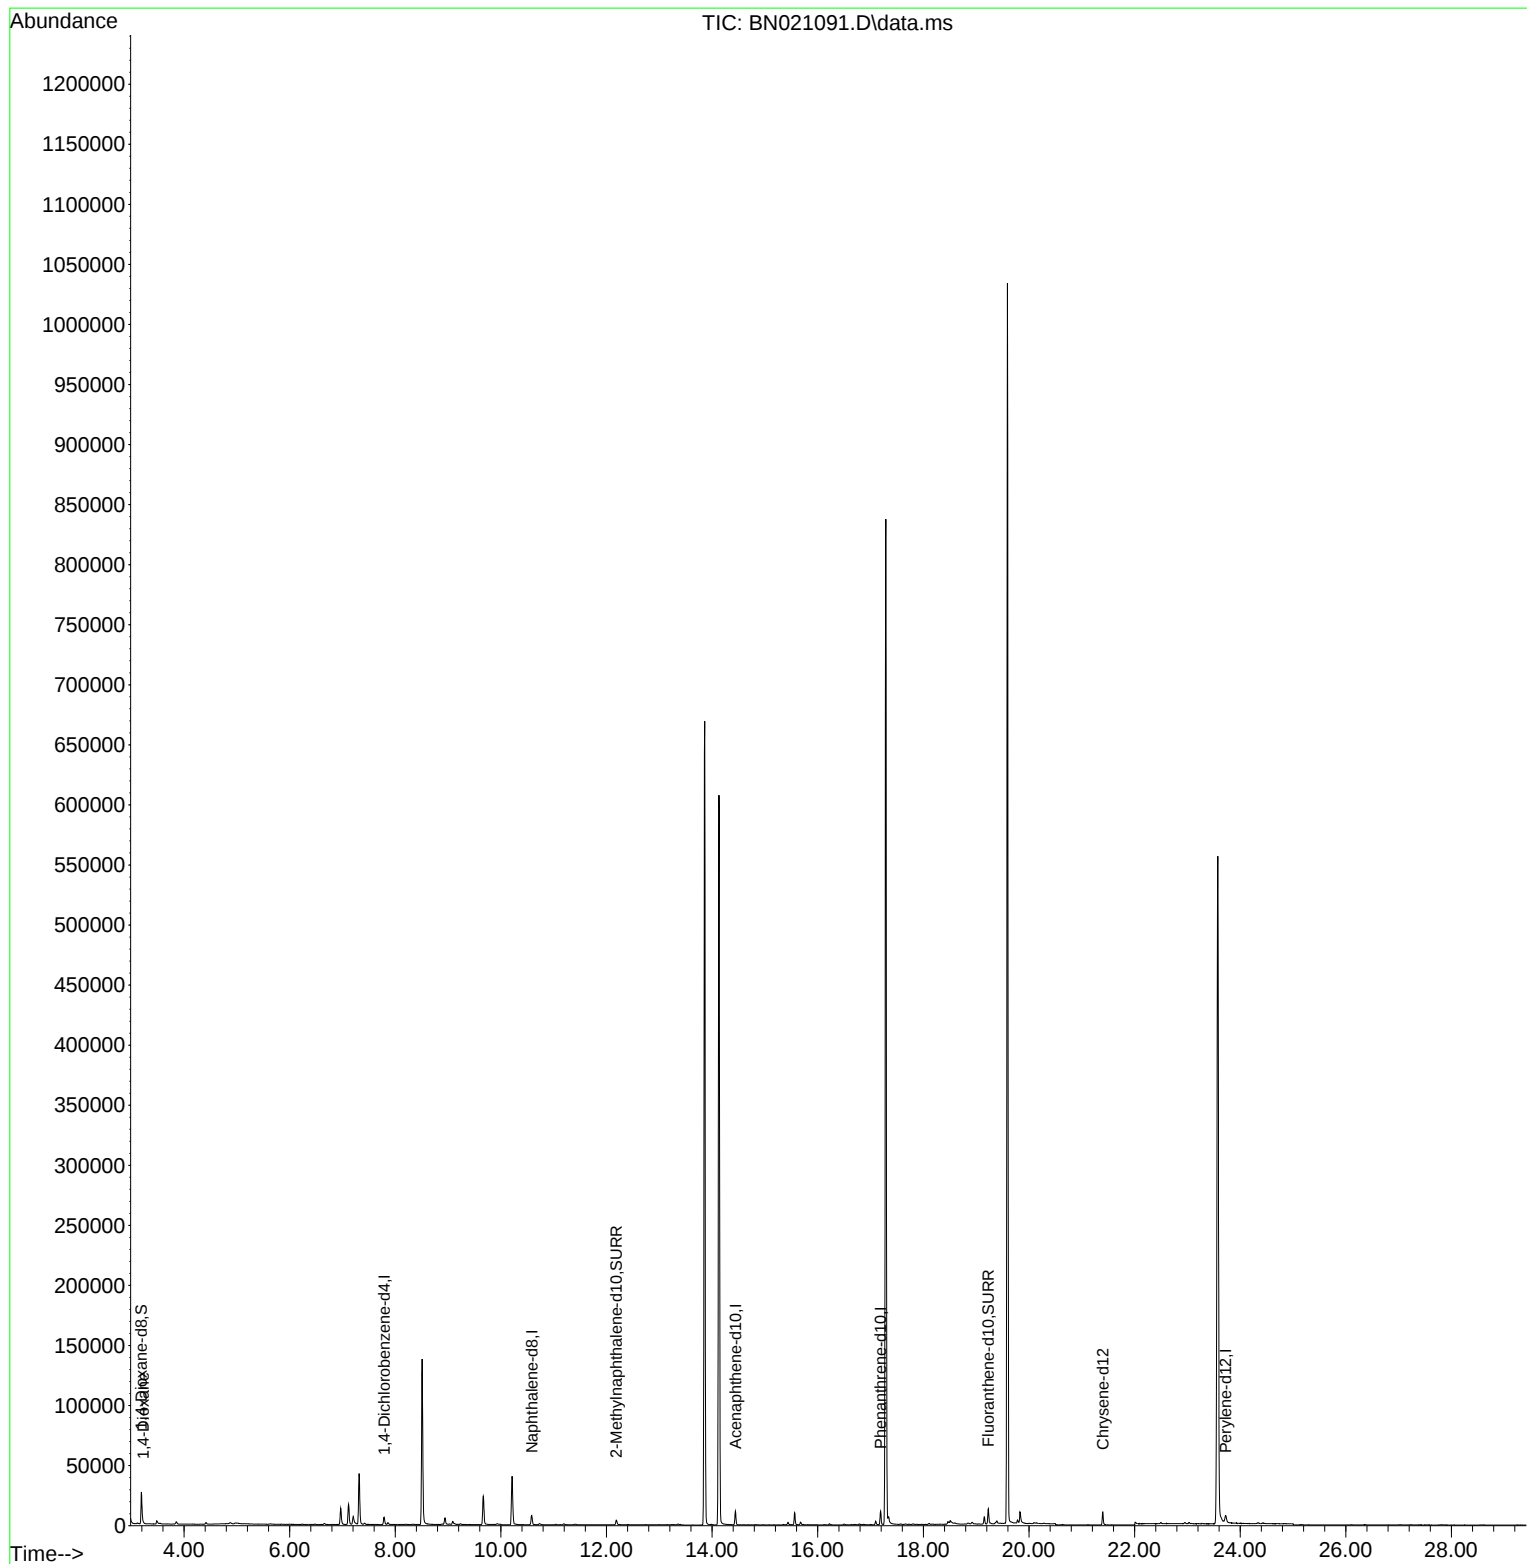

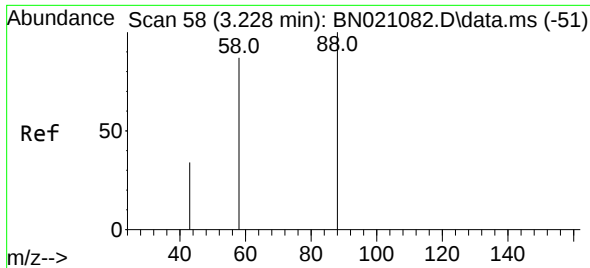

#2

1,4-Dioxane

Concen: 0.070 ng/ul

RT: 3.228 min Scan# 58

Delta R.T. -0.000 min

Lab File: BN021091.D


Acq: 09 Aug 2022 18:44

Instrument :

BNA_N

ClientSampleId :

GBJK4

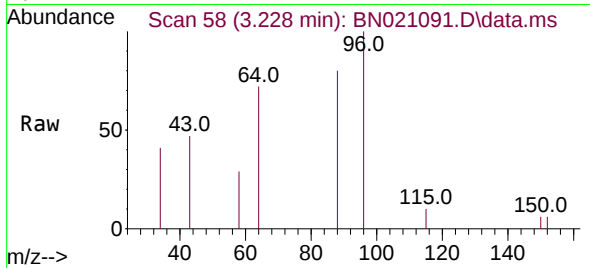

Tgt Ion: 88 Resp: 304

Ion Ratio Lower Upper

88 100

43 59.2 31.4 47.0#

58 36.8 49.0 73.6#

