

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
 Data File : BN021104.D
 Acq On : 10 Aug 2022 03:33
 Operator : CG/JU
 Sample : N4095-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJM8

Quant Time: Aug 10 04:54:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	2987	0.400	ng/ul	0.00
4) Naphthalene-d8	10.580	136	9959	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.438	164	5769	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.189	188	11377	0.400	ng/ul	0.00
17) Chrysene-d12	21.392	240	8644	0.400	ng/ul	-0.01
23) Perylene-d12	23.716	264	8137	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	16272	4.258	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	4285	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.226	212	10695	0.401	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	748	0.190	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080922\
Data File : BN021104.D
Acq On : 10 Aug 2022 03:33
Operator : CG/JU
Sample : N4095-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJM8

Quant Time: Aug 10 04:54:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

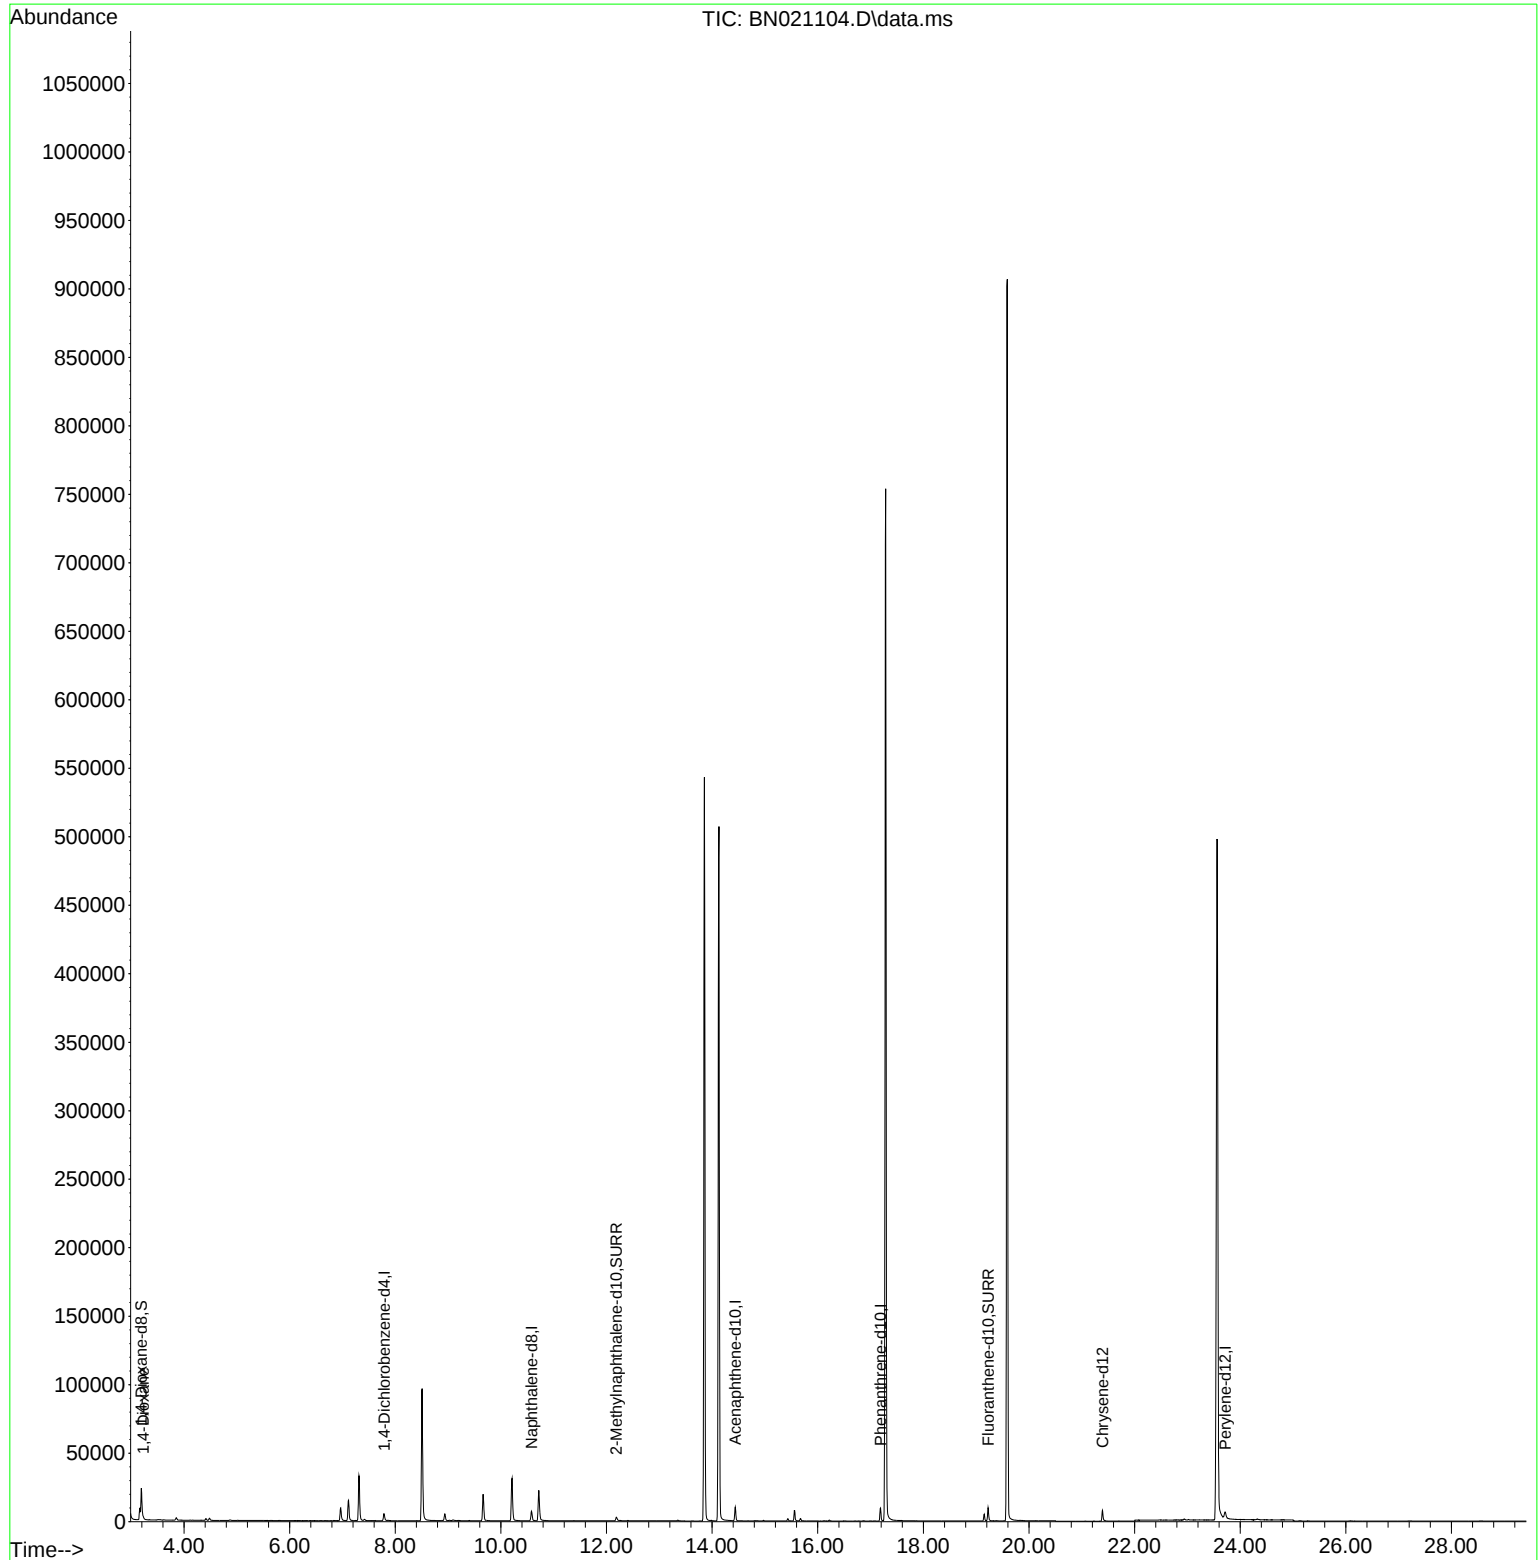

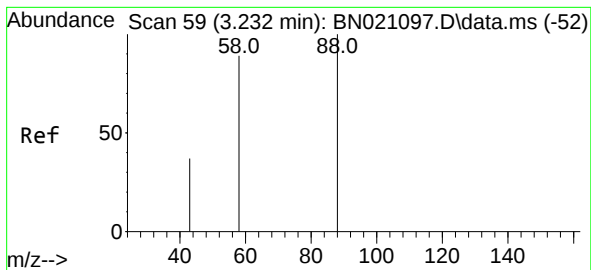

#2

1,4-Dioxane

Concen: 0.190 ng/ul

RT: 3.228 min Scan# 58

Delta R.T. -0.000 min

Lab File: BN021104.D


Acq: 10 Aug 2022 03:33

Instrument :

BNA_N

ClientSampleId :

GBJM8

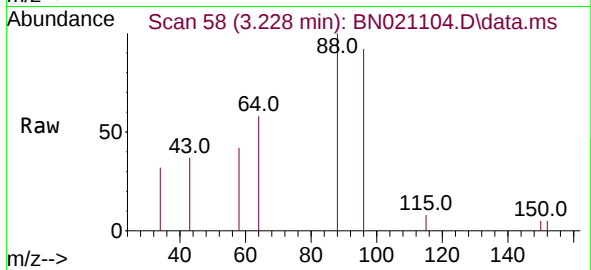

Tgt Ion: 88 Resp: 748

Ion Ratio Lower Upper

88 100

43 36.7 31.4 47.0

58 42.4 49.0 73.6#

