

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
 Data File : BN033322.D
 Acq On : 09 Aug 2024 18:19
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Aug 09 18:55:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 08 04:39:01 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	4193	0.400	ng	0.00
7) Naphthalene-d8	10.349	136	11697	0.400	ng	# 0.00
13) Acenaphthene-d10	14.212	164	6396	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	14966	0.400	ng	# 0.00
29) Chrysene-d12	21.175	240	13185	0.400	ng	0.00
35) Perylene-d12	23.358	264	14779	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.204	112	3746	0.339	ng	0.00
5) Phenol-d6	6.757	99	5116	0.339	ng	0.00
8) Nitrobenzene-d5	8.715	82	3193	0.447	ng	0.00
11) 2-Methylnaphthalene-d10	11.947	152	6750	0.370	ng	0.00
14) 2,4,6-Tribromophenol	15.705	330	887	0.343	ng	-0.01
15) 2-Fluorobiphenyl	12.844	172	11087	0.460	ng	0.00
27) Fluoranthene-d10	19.007	212	15023	0.365	ng	0.00
31) Terphenyl-d14	19.625	244	8708	0.383	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.196	88	1864	0.402	ng	92
3) n-Nitrosodimethylamine	3.492	42	2519	0.427	ng	# 85
6) bis(2-Chloroethyl)ether	7.024	93	5041	0.391	ng	96
9) Naphthalene	10.391	128	13349	0.406	ng	98
10) Hexachlorobutadiene	10.701	225	2672	0.443	ng	# 99
12) 2-Methylnaphthalene	12.019	142	8673	0.383	ng	98
16) Acenaphthylene	13.934	152	12321	0.395	ng	100
17) Acenaphthene	14.277	154	8384	0.423	ng	96
18) Fluorene	15.271	166	10977	0.415	ng	100
20) 4,6-Dinitro-2-methylph...	15.346	198	611	0.571	ng	# 37
21) 4-Bromophenyl-phenylether	16.176	248	3746	0.412	ng	# 78
22) Hexachlorobenzene	16.276	284	4350	0.456	ng	95
23) Atrazine	16.449	200	2333	0.311	ng	# 93
24) Pentachlorophenol	16.623	266	1197	0.358	ng	99
25) Phenanthrene	17.008	178	18121	0.418	ng	99
26) Anthracene	17.095	178	15384	0.365	ng	100
28) Fluoranthene	19.035	202	21500	0.394	ng	100
30) Pyrene	19.397	202	21896	0.422	ng	100
32) Benzo(a)anthracene	21.157	228	19517	0.381	ng	100
33) Chrysene	21.210	228	21156	0.427	ng	100
34) Bis(2-ethylhexyl)phtha...	21.139	149	7257	0.274	ng	100
36) Indeno(1,2,3-cd)pyrene	25.536	276	23480	0.363	ng	99
37) Benzo(b)fluoranthene	22.709	252	20479	0.373	ng	97
38) Benzo(k)fluoranthene	22.753	252	22143	0.415	ng	99
39) Benzo(a)pyrene	23.261	252	17277	0.354	ng	97
40) Dibenzo(a,h)anthracene	25.556	278	18680	0.366	ng	98
41) Benzo(g,h,i)perylene	26.194	276	21397	0.385	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033322.D
Acq On : 09 Aug 2024 18:19
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Aug 09 18:55:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:39:01 2024
Response via : Initial Calibration




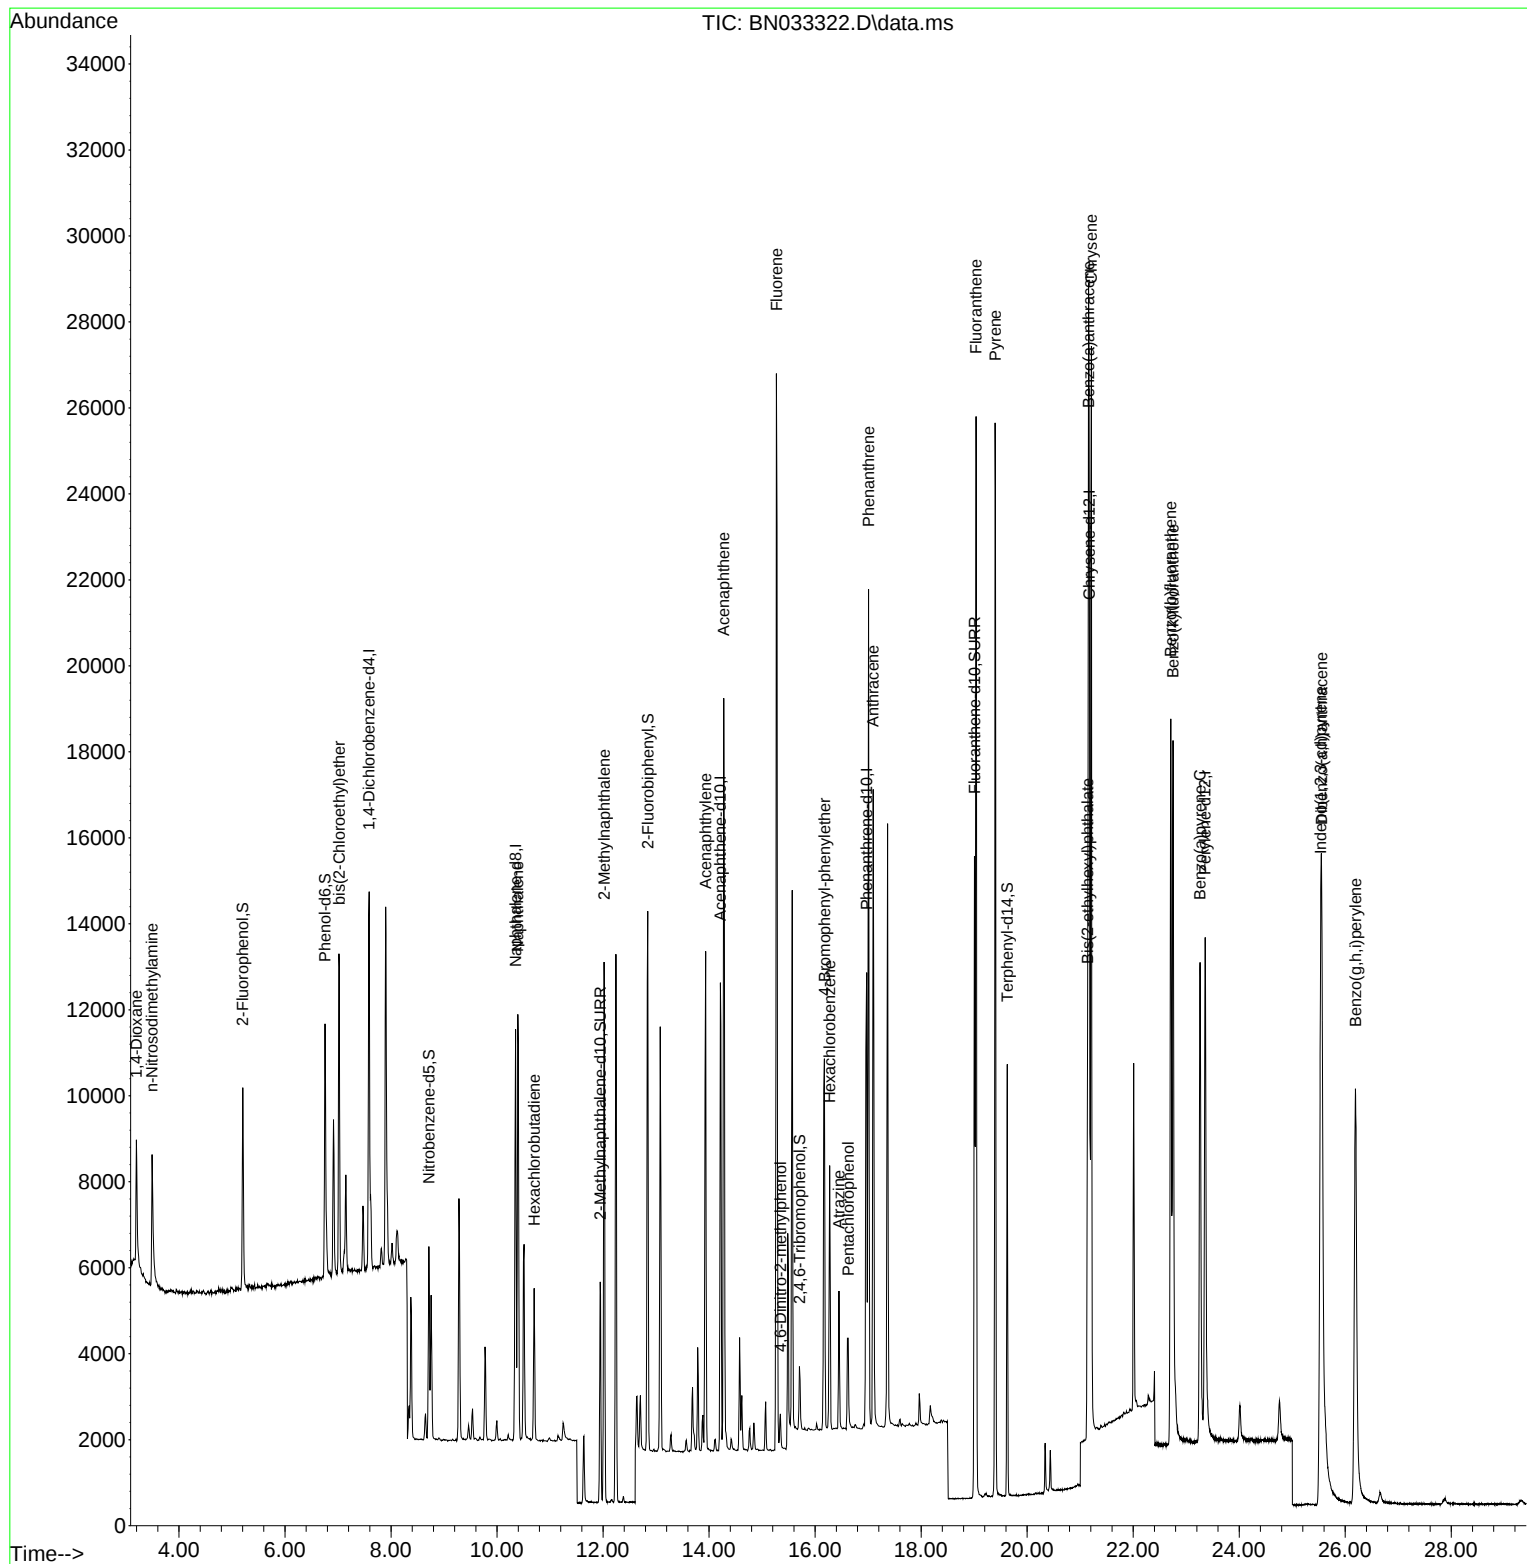




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.587 min Scan# 61
 Delta R.T. -0.002 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 4193
 Ion Ratio Lower Upper
 152 100
 150 155.5 120.7 181.1
 115 62.5 55.8 83.8

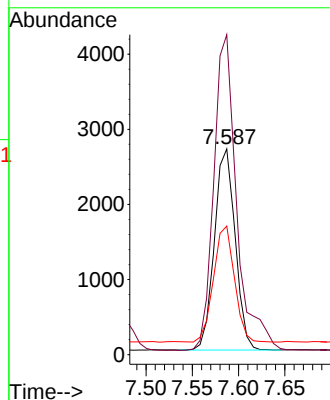

#2
 1,4-Dioxane
 Concen: 0.402 ng
 RT: 3.196 min Scan# 16
 Delta R.T. -0.002 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19

Tgt Ion: 88 Resp: 1864
 Ion Ratio Lower Upper
 88 100
 43 39.4 37.0 55.6
 58 86.7 65.1 97.7



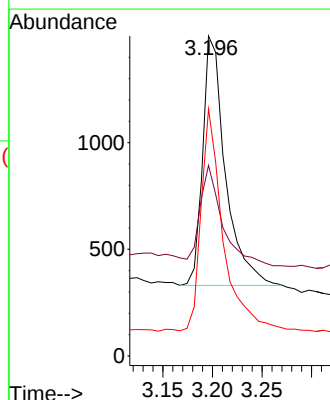



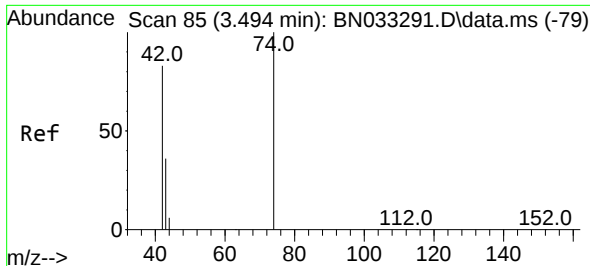

#3
 n-Nitrosodimethylamine
 Concen: 0.427 ng
 RT: 3.492 min Scan# 51
 Delta R.T. -0.002 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 42 Resp: 2519
 Ion Ratio Lower Upper
 42 100
 74 101.9 94.9 142.3
 44 6.1 7.0 10.4#

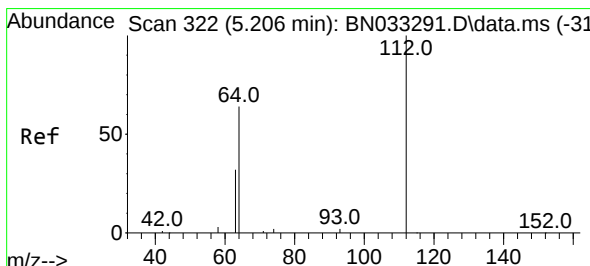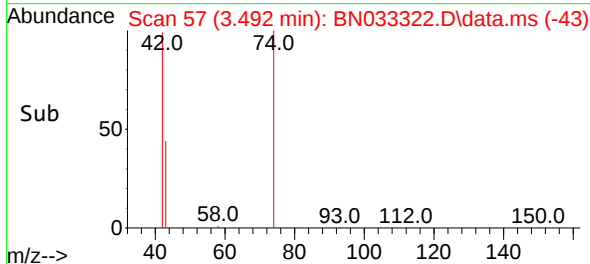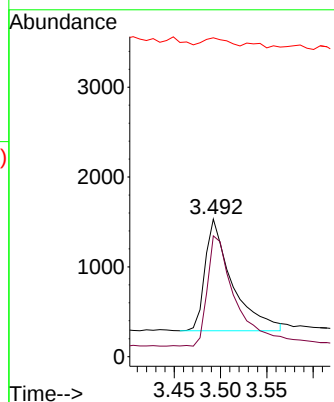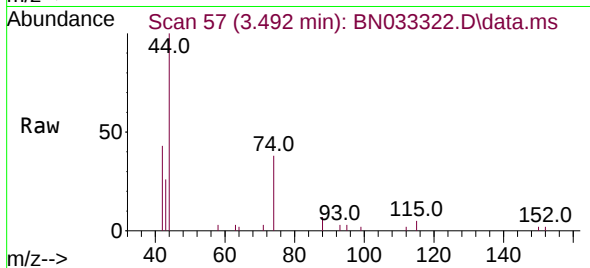

#4
 2-Fluorophenol
 Concen: 0.339 ng
 RT: 5.204 min Scan# 294
 Delta R.T. -0.002 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19

Tgt Ion: 112 Resp: 3746
 Ion Ratio Lower Upper
 112 100
 64 60.1 48.7 73.1
 63 32.0 25.4 38.2


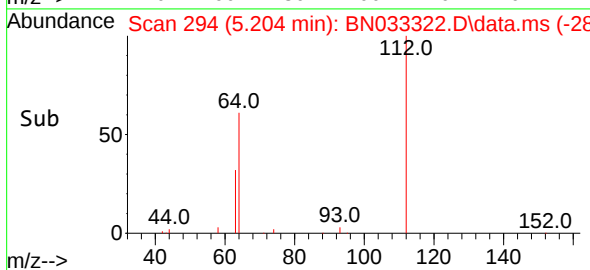
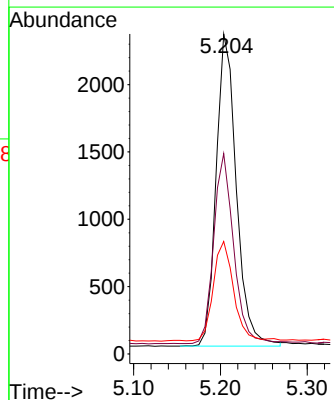
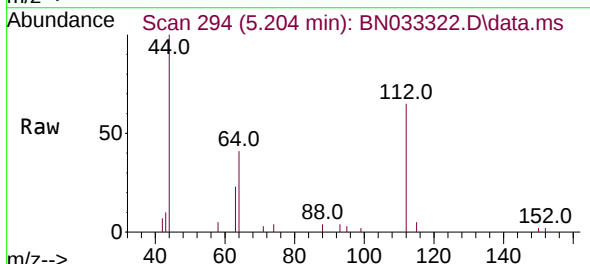




#5
Phenol-d6
Concen: 0.339 ng
RT: 6.757 min Scan# 509
Delta R.T. -0.002 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	5116
Ion	Ratio	Lower	Upper
99	100		
42	24.8	19.3	28.9
71	33.3	27.6	41.4



#6
bis(2-Chloroethyl)ether
Concen: 0.391 ng
RT: 7.024 min Scan# 546
Delta R.T. -0.002 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:	93	Resp:	5041
Ion	Ratio	Lower	Upper
93	100		
63	85.5	64.5	96.7
95	32.8	26.6	39.8




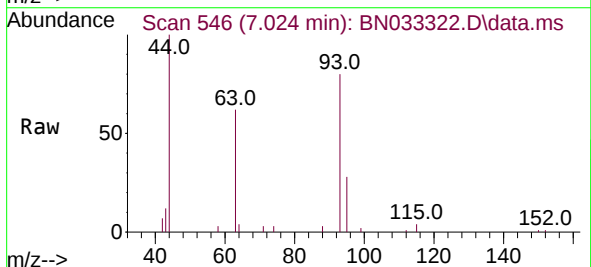




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.349 min Scan# 91
Delta R.T. -0.002 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	11697
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.9	14.9
54	9.6	11.4	17.2#
68	7.3	9.5	14.3#

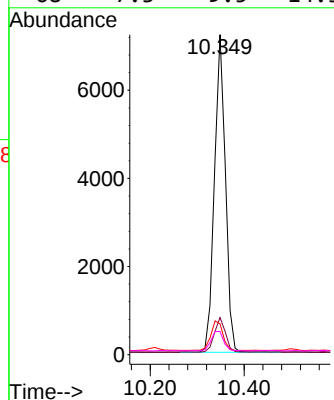

#8
Nitrobenzene-d5
Concen: 0.447 ng
RT: 8.715 min Scan# 762
Delta R.T. -0.002 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:	82	Resp:	3193
Ion Ratio	Lower	Upper	
82	100		
128	39.6	29.4	44.2
54	59.6	50.0	75.0


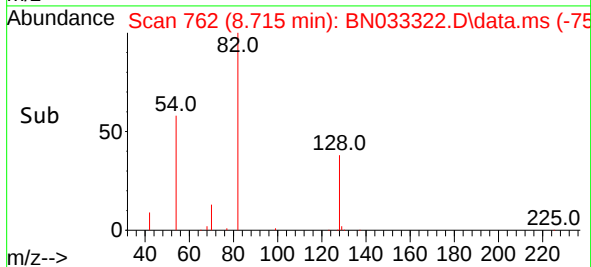
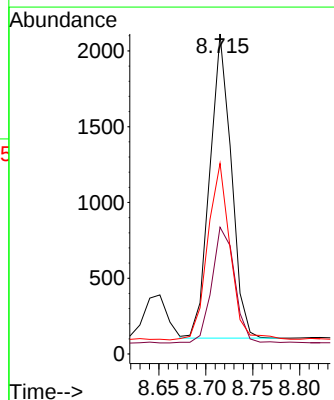
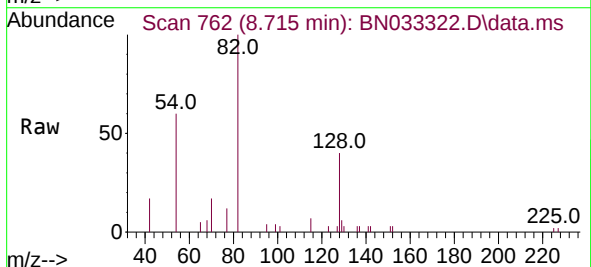




#9
Naphthalene
Concen: 0.406 ng
RT: 10.391 min Scan# 91
Delta R.T. -0.013 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 13349
Ion Ratio Lower Upper
128 100
129 11.4 10.1 15.1
127 13.8 11.4 17.2



#10
Hexachlorobutadiene
Concen: 0.443 ng
RT: 10.701 min Scan# 948
Delta R.T. -0.002 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:225 Resp: 2672
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 51.8 77.6







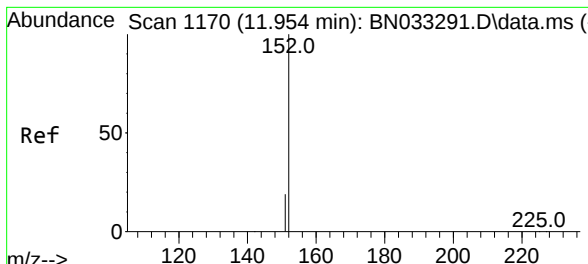

#11
2-Methylnaphthalene-d10
Concen: 0.370 ng
RT: 11.947 min Scan# 1119
Delta R.T. -0.007 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 6750
Ion Ratio Lower Upper
152 100
151 21.2 16.7 25.1

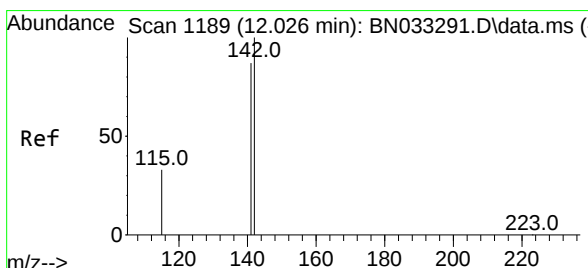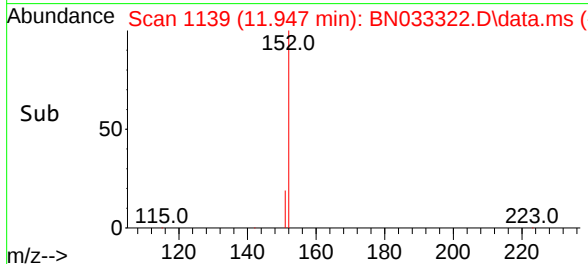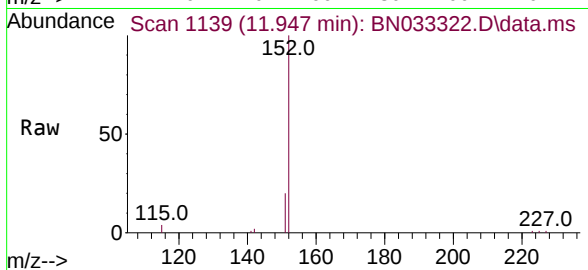

#12
2-Methylnaphthalene
Concen: 0.383 ng
RT: 12.019 min Scan# 1158
Delta R.T. -0.007 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:142 Resp: 8673
Ion Ratio Lower Upper
142 100
141 90.1 70.5 105.7
115 38.3 30.3 45.5


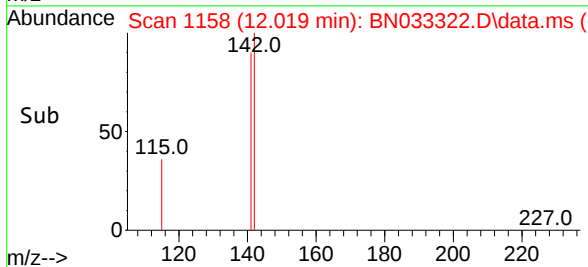

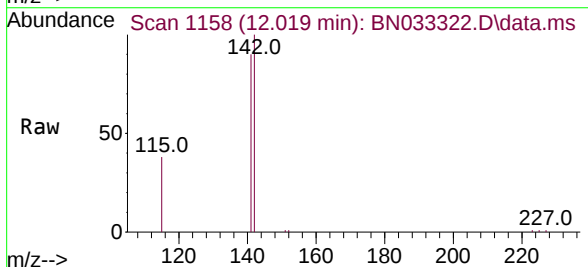


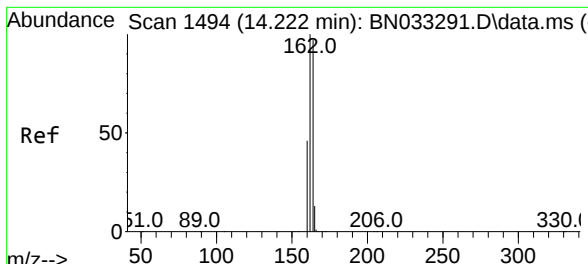

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.212 min Scan# 14
Delta R.T. -0.010 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164	Resp:	6396
Ion Ratio	Lower	Upper
164	100	
162	107.6	82.6 124.0
160	56.9	38.2 57.4

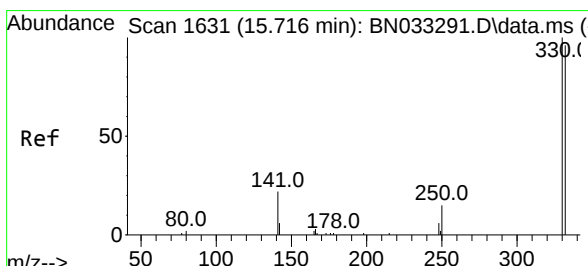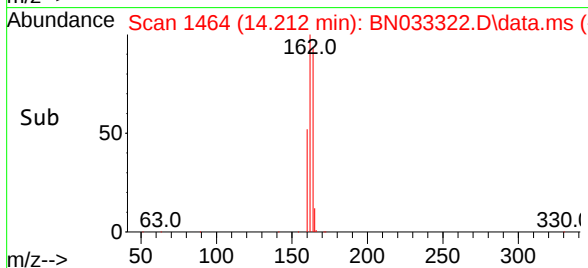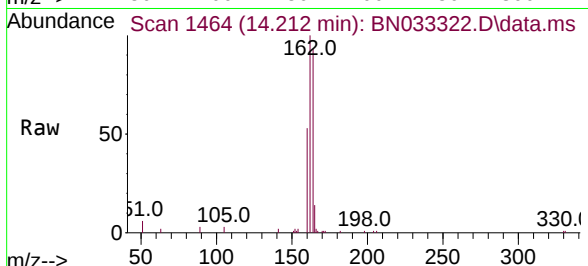

#14
2,4,6-Tribromophenol
Concen: 0.343 ng
RT: 15.705 min Scan# 1601
Delta R.T. -0.011 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:330	Resp:	887
Ion Ratio	Lower	Upper
330	100	
332	94.3	75.6 113.4
141	43.3	31.0 46.4


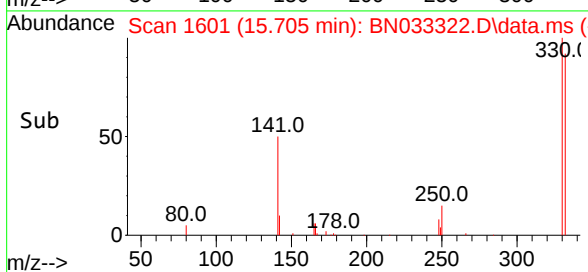

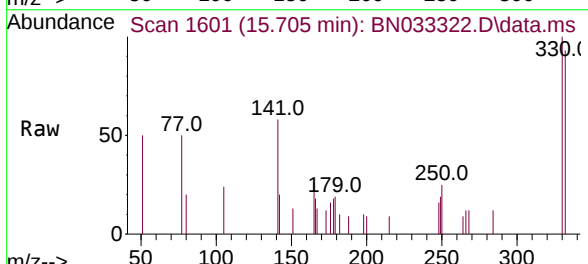




#15
2-Fluorobiphenyl
Concen: 0.460 ng
RT: 12.844 min Scan# 11
Delta R.T. 0.001 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	11087
Ion Ratio	Lower	Upper	
172	100		
171	34.5	28.3	42.5
170	23.2	19.4	29.2



#16
Acenaphthylene
Concen: 0.395 ng
RT: 13.934 min Scan# 1438
Delta R.T. 0.001 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:	152	Resp:	12321
Ion Ratio	Lower	Upper	
152	100		
151	19.5	15.7	23.5
153	12.8	10.3	15.5




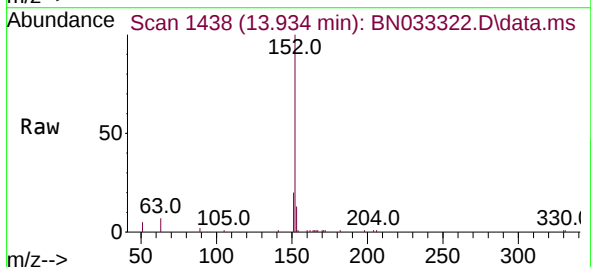




#17
Acenaphthene
Concen: 0.423 ng
RT: 14.277 min Scan# 14
Delta R.T. -0.010 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 8384
Ion Ratio Lower Upper
154 100
153 113.6 89.5 134.3
152 61.8 43.6 65.4



#18
Fluorene
Concen: 0.415 ng
RT: 15.271 min Scan# 1563
Delta R.T. -0.010 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:166 Resp: 10977
Ion Ratio Lower Upper
166 100
165 98.1 78.9 118.3
167 13.4 10.6 16.0




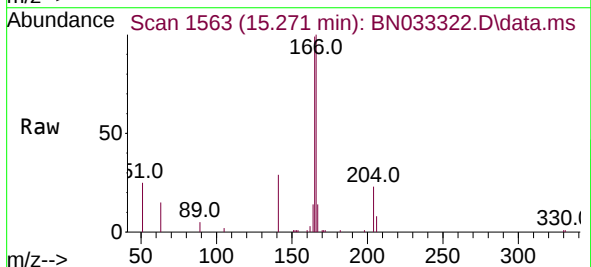


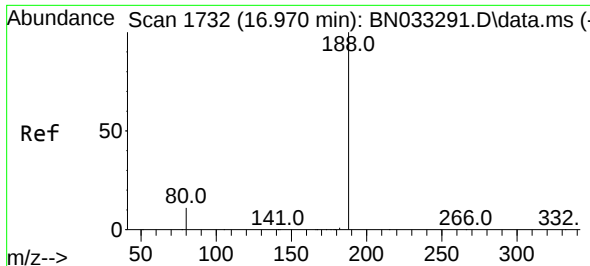

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.971 min Scan# 11
Delta R.T. 0.001 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 14966
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.9 10.5 15.7#

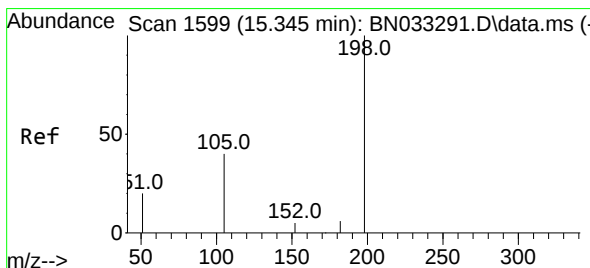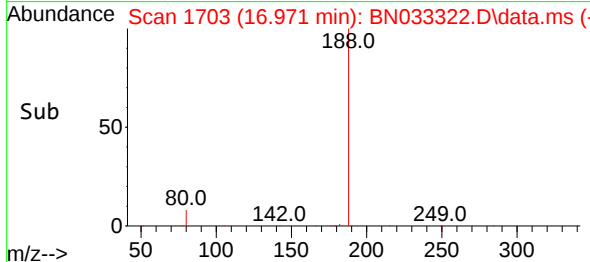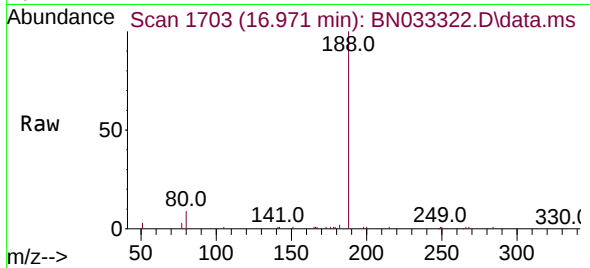

#20
4,6-Dinitro-2-methylphenol
Concen: 0.571 ng
RT: 15.346 min Scan# 1570
Delta R.T. 0.001 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:198 Resp: 611
Ion Ratio Lower Upper
198 100
51 83.4 127.9 191.9#
105 55.9 112.3 168.5#


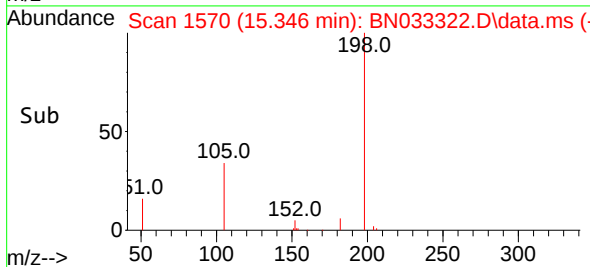

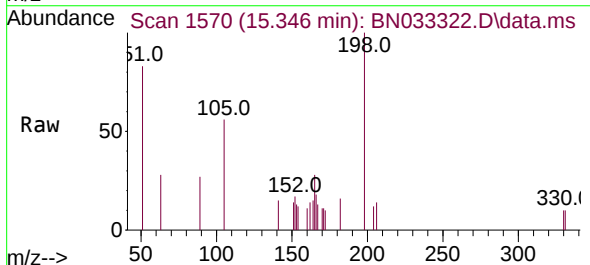


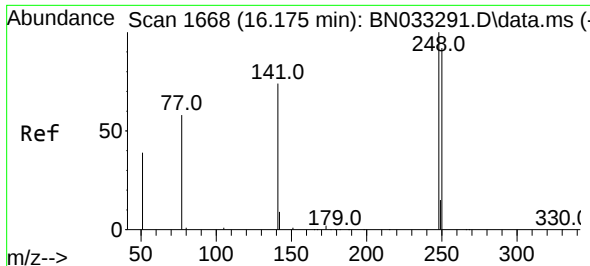

#21
4-Bromophenyl-phenylether
Concen: 0.412 ng
RT: 16.176 min Scan# 1639
Delta R.T. 0.001 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 3746
Ion Ratio Lower Upper
248 100
250 99.2 74.6 112.0
141 42.2 62.2 93.2#

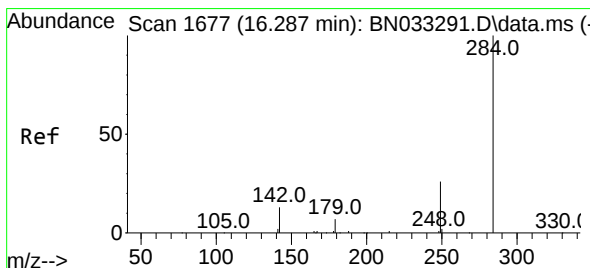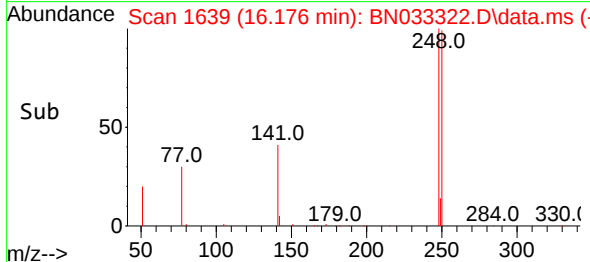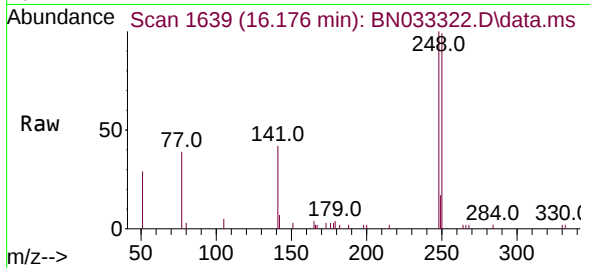

#22
Hexachlorobenzene
Concen: 0.456 ng
RT: 16.276 min Scan# 1647
Delta R.T. -0.011 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:284 Resp: 4350
Ion Ratio Lower Upper
284 100
142 41.2 30.6 45.8
249 32.8 24.6 36.8

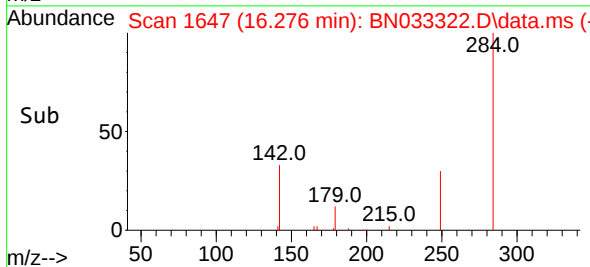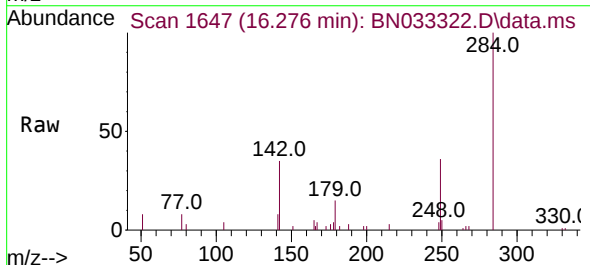

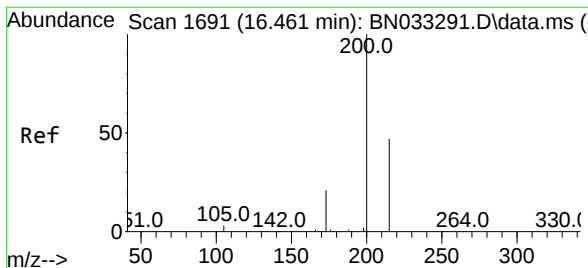

#23

Atrazine

Concen: 0.311 ng

RT: 16.449 min Scan# 1661

Delta R.T. -0.011 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:200 Resp: 2333

Ion Ratio Lower Upper

200 100

173 29.6 18.9 28.3#

215 45.6 38.6 57.8

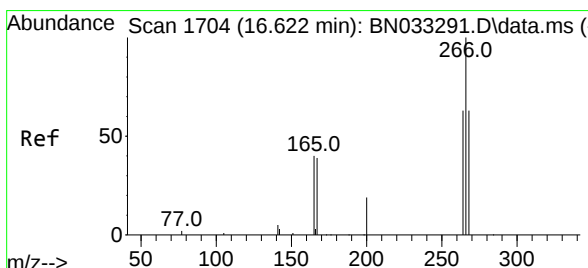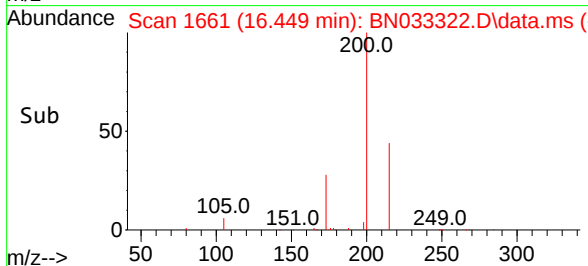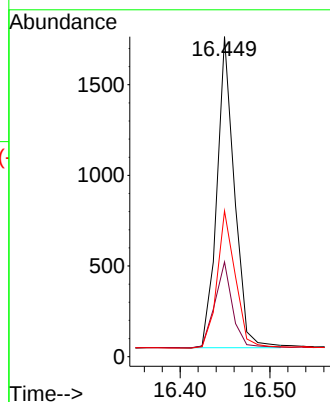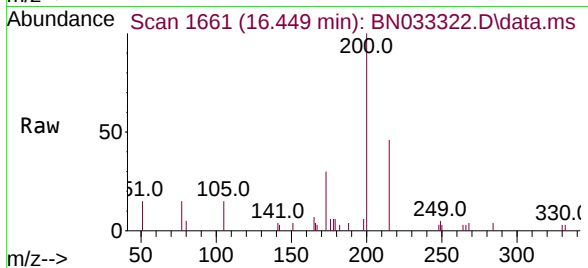

#24

Pentachlorophenol

Concen: 0.358 ng

RT: 16.623 min Scan# 1675

Delta R.T. 0.001 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19




Tgt Ion:266 Resp: 1197


Ion Ratio Lower Upper

266 100

264 64.0 50.3 75.5

268 64.2 51.0 76.4

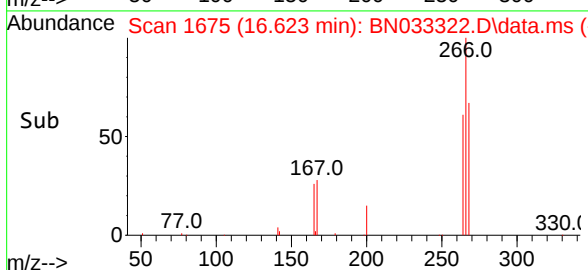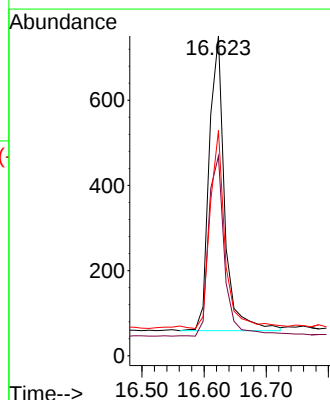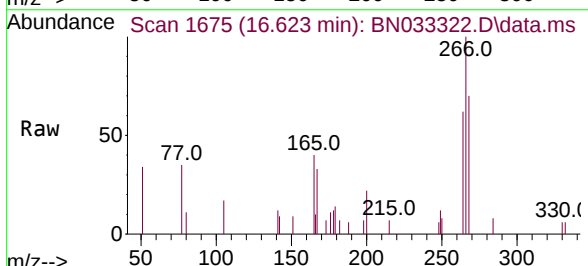



#25

Phenanthrene

Concen: 0.418 ng

RT: 17.008 min Scan# 1712

Delta R.T. 0.001 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:178 Resp: 18121

Ion Ratio Lower Upper

178 100

176 19.4 15.2 22.8

179 15.5 12.0 18.0



#26

Anthracene

Concen: 0.365 ng

RT: 17.095 min Scan# 1713

Delta R.T. -0.011 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19




Tgt Ion:178 Resp: 15384


Ion Ratio Lower Upper

178 100

176 18.4 14.8 22.2

179 15.4 12.2 18.4




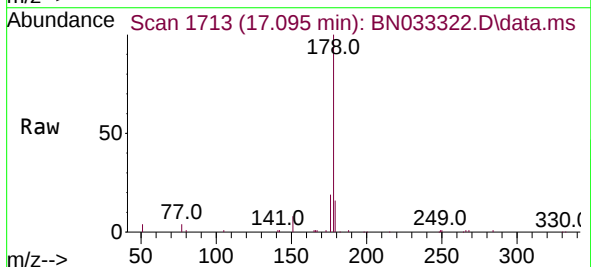




#27
Fluoranthene-d10
Concen: 0.365 ng
RT: 19.007 min Scan# 1940
Delta R.T. -0.004 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 15023
Ion Ratio Lower Upper
212 100
106 16.2 12.2 18.4
104 9.4 6.9 10.3

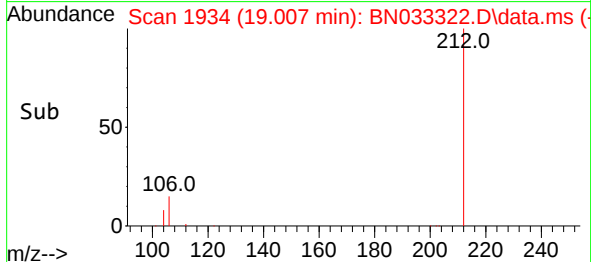

#28
Fluoranthene
Concen: 0.394 ng
RT: 19.035 min Scan# 1940
Delta R.T. -0.008 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:202 Resp: 21500
Ion Ratio Lower Upper
202 100
101 12.1 9.4 14.0
203 17.2 13.8 20.6


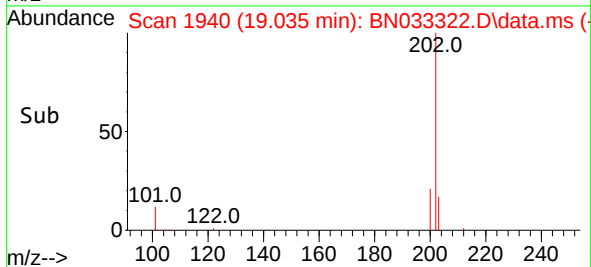

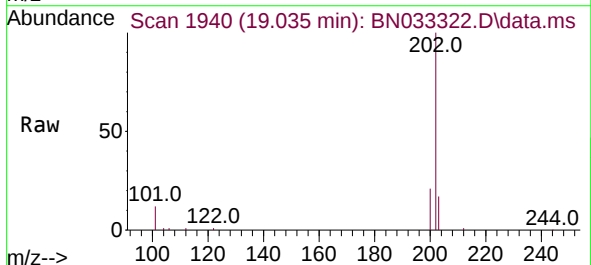


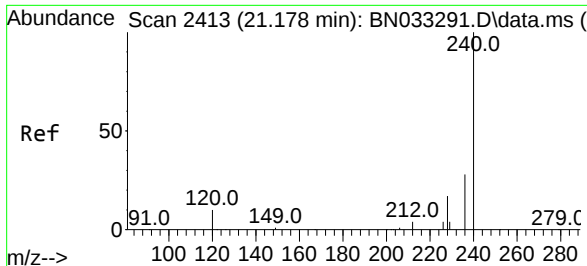

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.175 min Scan# 21185
Delta R.T. -0.004 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 13185
Ion Ratio Lower Upper
240 100
120 11.9 9.0 13.6
236 29.0 22.4 33.6

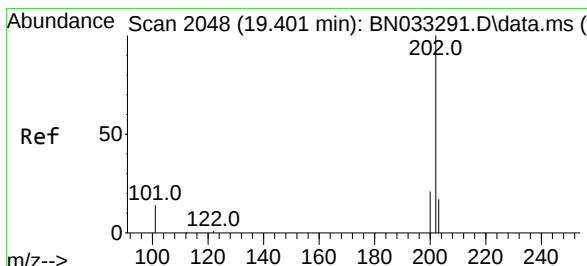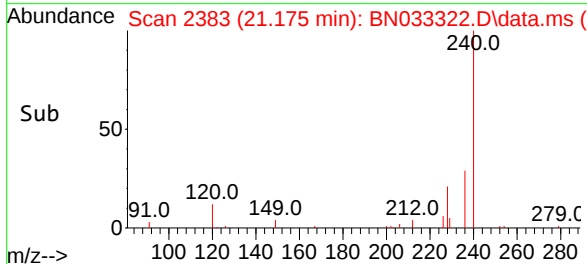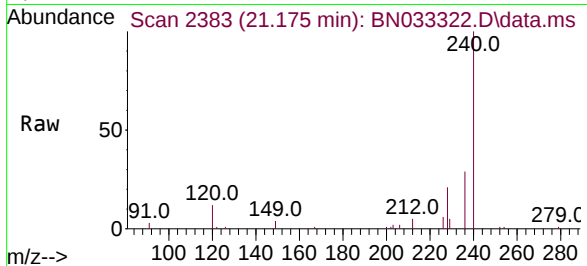

#30
Pyrene
Concen: 0.422 ng
RT: 19.397 min Scan# 2018
Delta R.T. -0.004 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:202 Resp: 21896
Ion Ratio Lower Upper
202 100
200 21.1 16.7 25.1
203 17.9 14.2 21.4


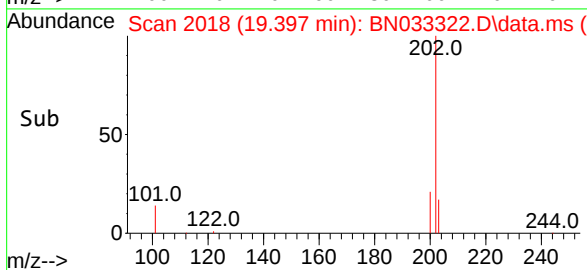

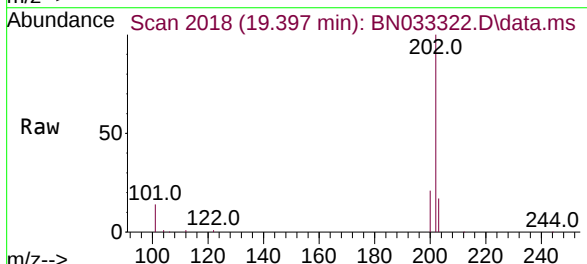




#31
 Terphenyl-d14
 Concen: 0.383 ng
 RT: 19.625 min Scan# 2098
 Delta R.T. -0.008 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 8708
 Ion Ratio Lower Upper
 244 100
 212 10.0 7.2 10.8
 122 18.3 12.7 19.1



#32
 Benzo(a)anthracene
 Concen: 0.381 ng
 RT: 21.157 min Scan# 2381
 Delta R.T. -0.004 min
 Lab File: BN033322.D
 Acq: 09 Aug 2024 18:19

Tgt Ion:228 Resp: 19517
 Ion Ratio Lower Upper
 228 100
 226 27.3 22.1 33.1
 229 19.5 15.6 23.4



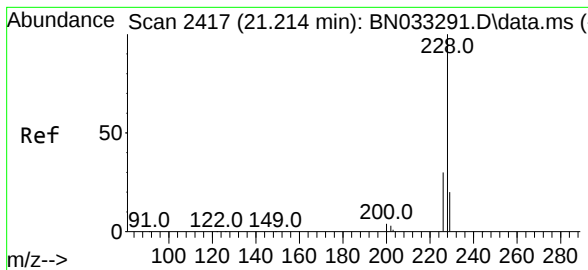

#33

Chrysene

Concen: 0.427 ng

RT: 21.210 min Scan# 21

Delta R.T. -0.004 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 21156

Ion Ratio Lower Upper

228 100

226 29.9 23.8 35.8

229 19.8 15.8 23.8

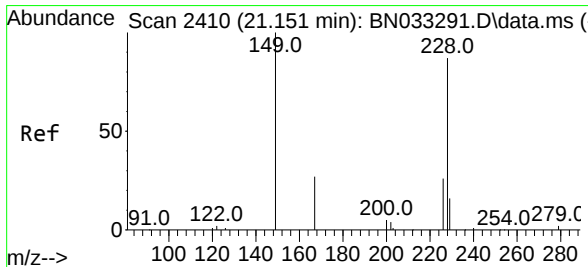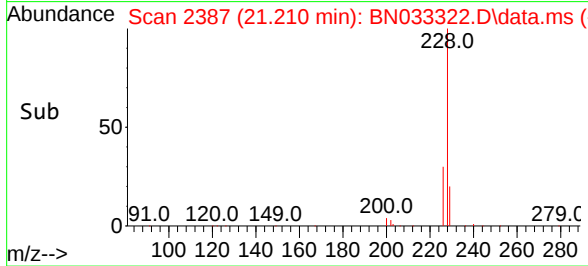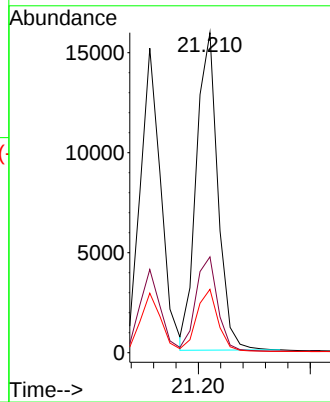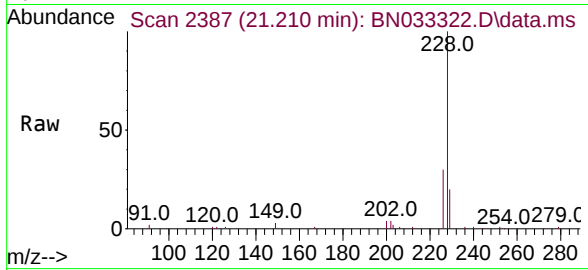

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.274 ng

RT: 21.139 min Scan# 2379

Delta R.T. -0.013 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19




Tgt Ion:149 Resp: 7257


Ion Ratio Lower Upper

149 100

167 26.8 21.6 32.4

279 2.9 2.6 4.0

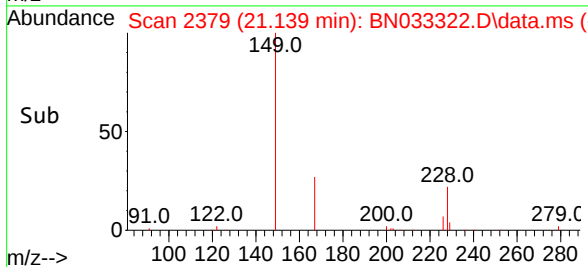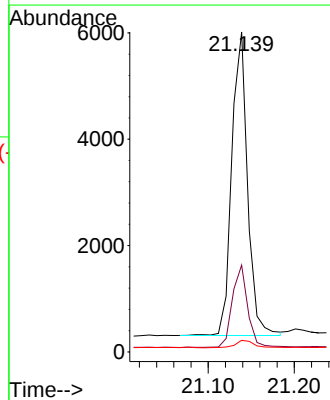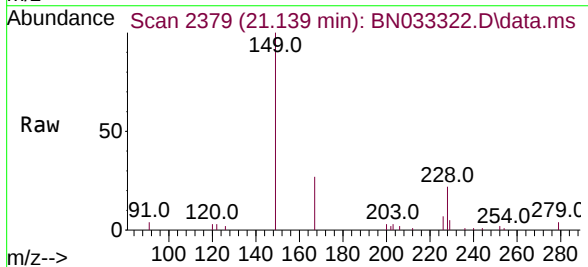



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.358 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN033322.D


Acq: 09 Aug 2024 18:19

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4






Tgt Ion:264 Resp: 14779

Ion Ratio Lower Upper

264 100

260 27.4 21.4 32.0

265 36.0 22.4 33.6#



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.363 ng

RT: 25.536 min Scan# 3590

Delta R.T. -0.009 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19




Tgt Ion:276 Resp: 23480


Ion Ratio Lower Upper

276 100

138 29.1 22.7 34.1

277 24.9 19.8 29.8

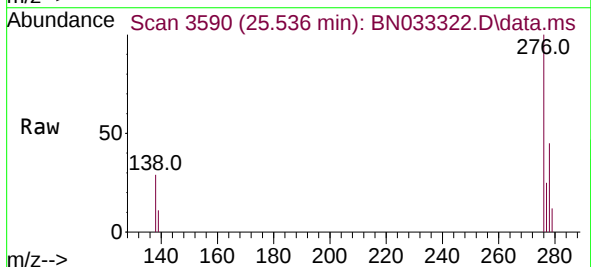



#37

Benzo(b)fluoranthene

Concen: 0.373 ng

RT: 22.709 min Scan# 2623

Delta R.T. -0.006 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:252 Resp: 20479

Ion Ratio Lower Upper

252 100

253 22.9 17.8 26.6

125 14.2 10.0 15.0



#38

Benzo(k)fluoranthene

Concen: 0.415 ng

RT: 22.753 min Scan# 2638

Delta R.T. -0.006 min

Lab File: BN033322.D

Acq: 09 Aug 2024 18:19




Tgt Ion:252 Resp: 22143


Ion Ratio Lower Upper

252 100

253 22.9 18.3 27.5


125 14.4 10.2 15.4








#39
Benzo(a)pyrene
Concen: 0.354 ng
RT: 23.261 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 17277
Ion Ratio Lower Upper
252 100
253 23.3 18.2 27.4
125 16.2 11.4 17.2

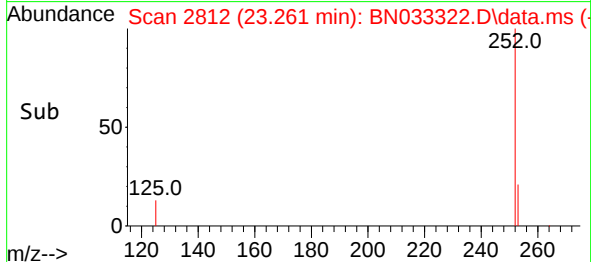

#40
Dibenzo(a,h)anthracene
Concen: 0.366 ng
RT: 25.556 min Scan# 3597
Delta R.T. -0.015 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Tgt Ion:278 Resp: 18680
Ion Ratio Lower Upper
278 100
139 21.7 16.3 24.5
279 25.1 19.4 29.2

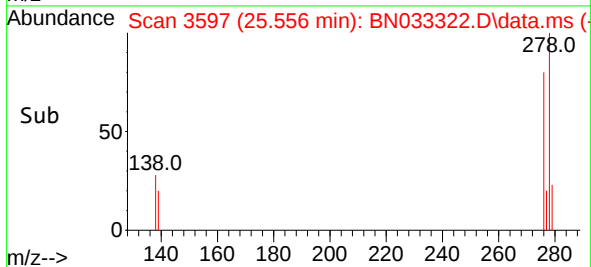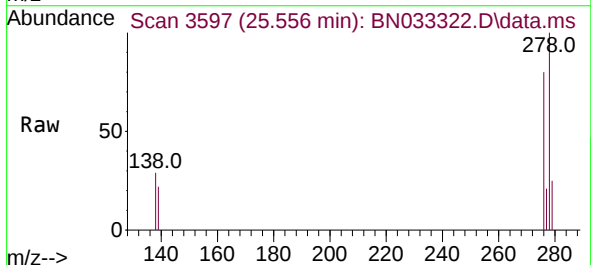

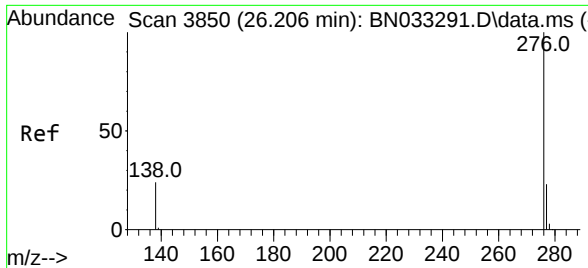

#41
Benzo(g,h,i)perylene
Concen: 0.385 ng
RT: 26.194 min Scan# 3815
Delta R.T. -0.012 min
Lab File: BN033322.D
Acq: 09 Aug 2024 18:19

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	276	Resp:	21397
Ion Ratio	Lower	Upper	
276	100		
277	24.7	19.0	28.4
138	27.7	20.8	31.2

