
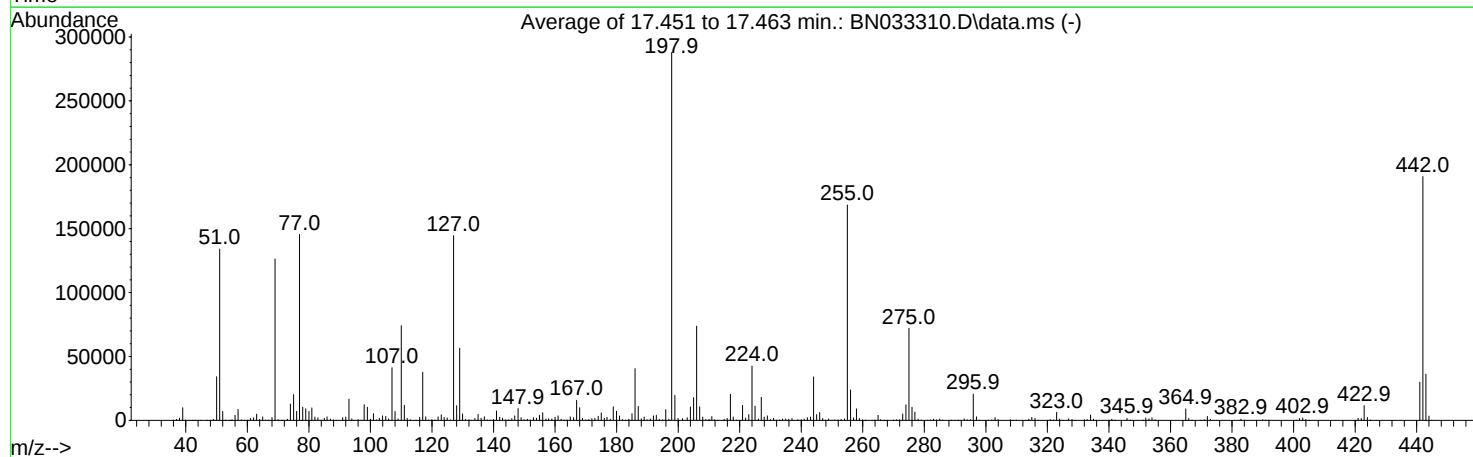


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033310.D
Acq On : 09 Aug 2024 08:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 08 04:39:01 2024

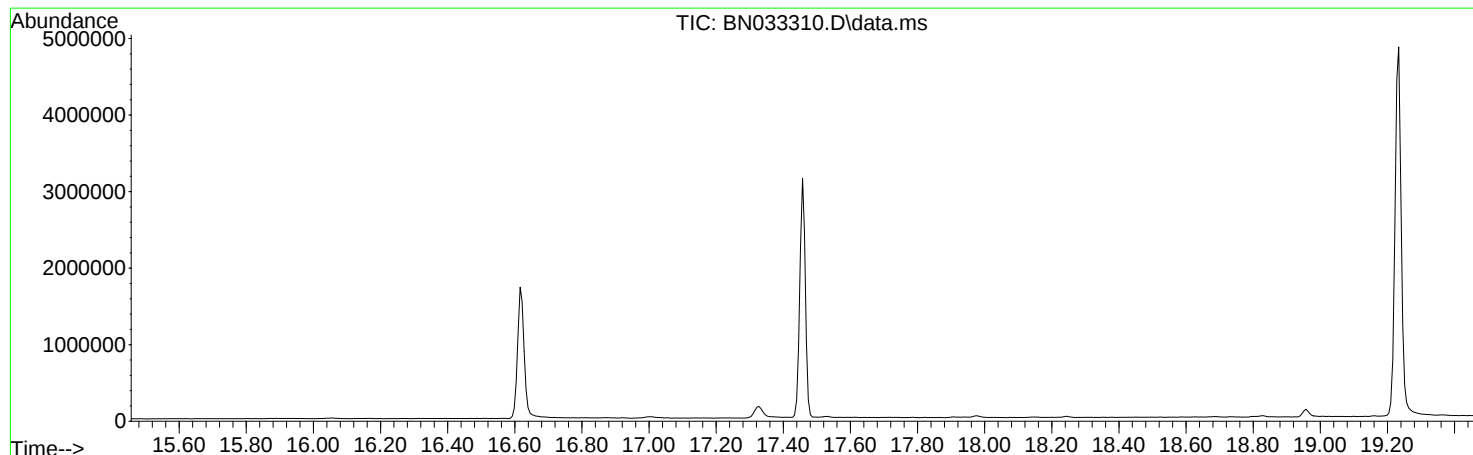

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	134119	PASS
68	69	0.00	2	1.8	2245	PASS
69	198	0.00	100	43.9	126326	PASS
70	69	0.00	2	0.5	592	PASS
127	198	10	80	50.3	144656	PASS
197	198	0.00	2	0.3	849	PASS
198	198	100	100	100.0	287872	PASS
199	198	5	9	6.8	19526	PASS
275	198	10	60	25.0	71957	PASS
365	198	1	100	3.1	8988	PASS
441	198	0.01	100	10.4	29992	PASS
442	442	50	100	100.0	190819	PASS
443	442	15	24	18.9	36144	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/9/2024	BNA_N	<u>BN033310.D</u>
Compound Name	Response	Retention Time
DDT	977599	20.492
DDD	14426	20.098
DDE	387	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14813	992412	1.49

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033310.D
Acq On : 09 Aug 2024 08:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 10 00:40:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

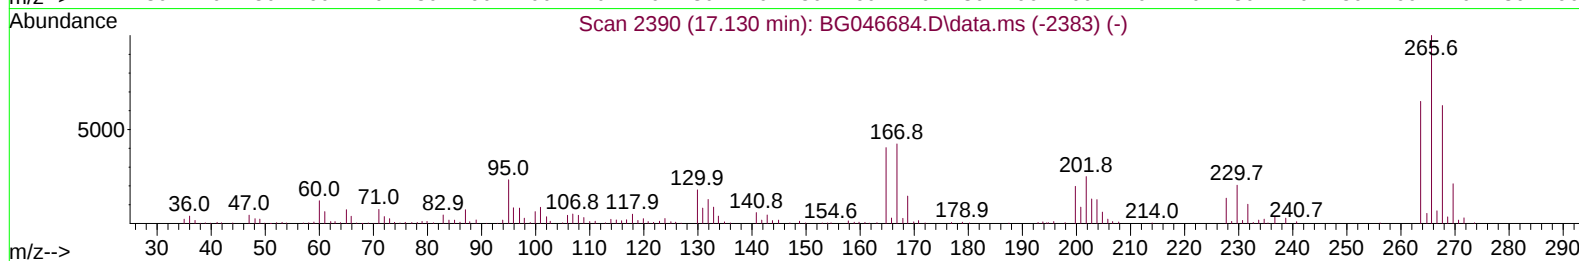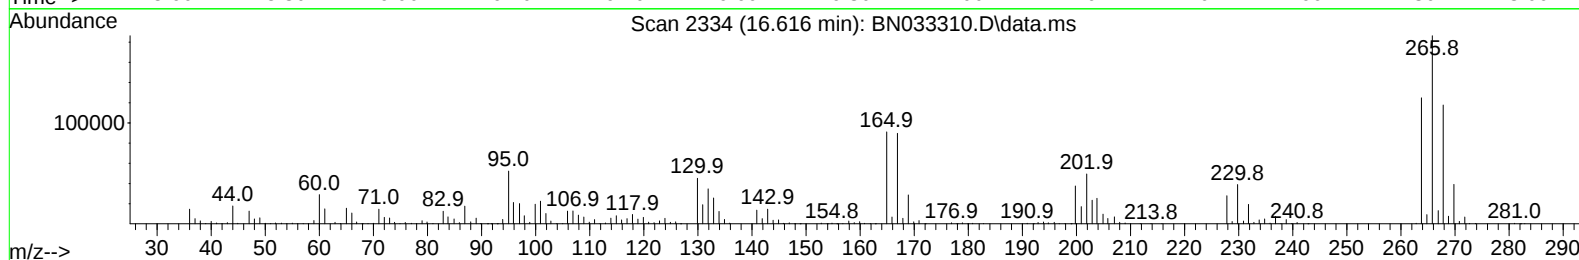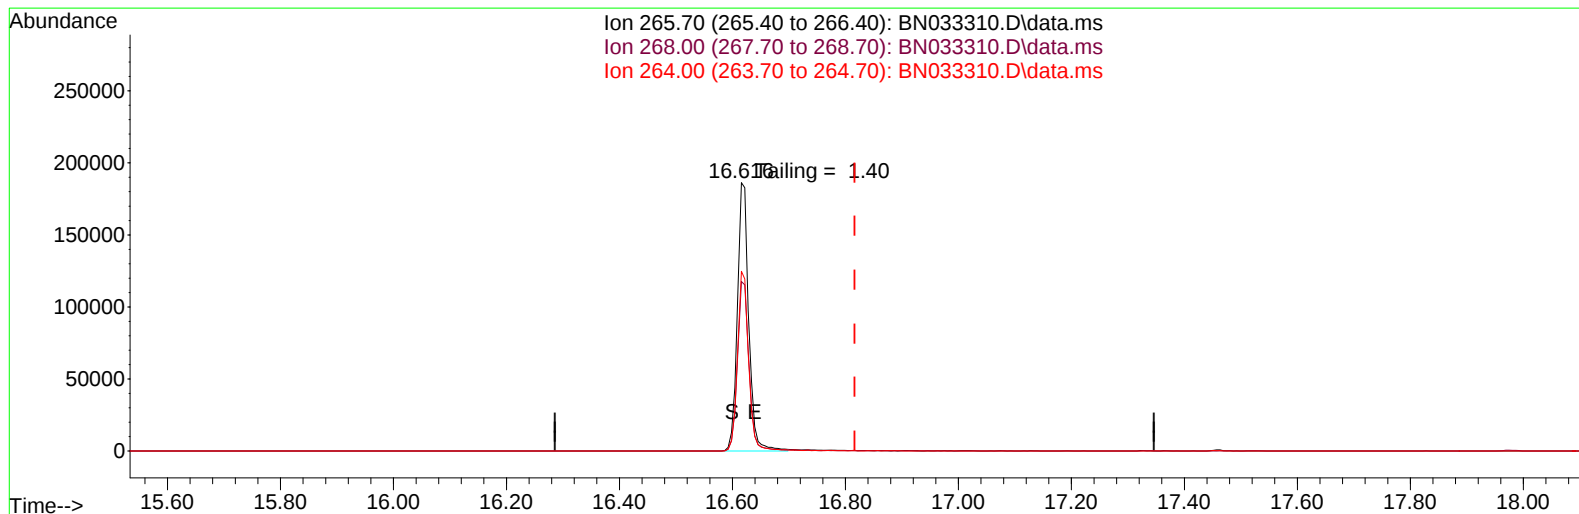

TIC: BN033310.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.200) 19307.72 ng




response 263194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.15
264.00	61.60	66.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033310.D
Acq On : 09 Aug 2024 08:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 10 00:40:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

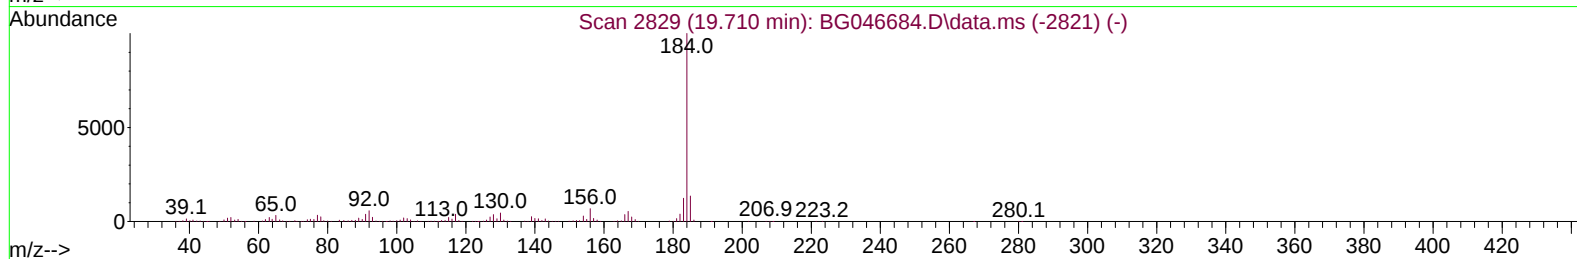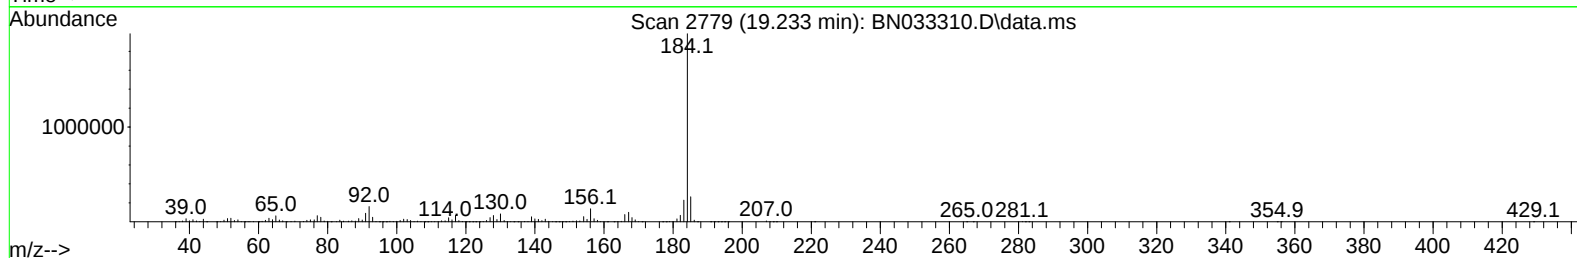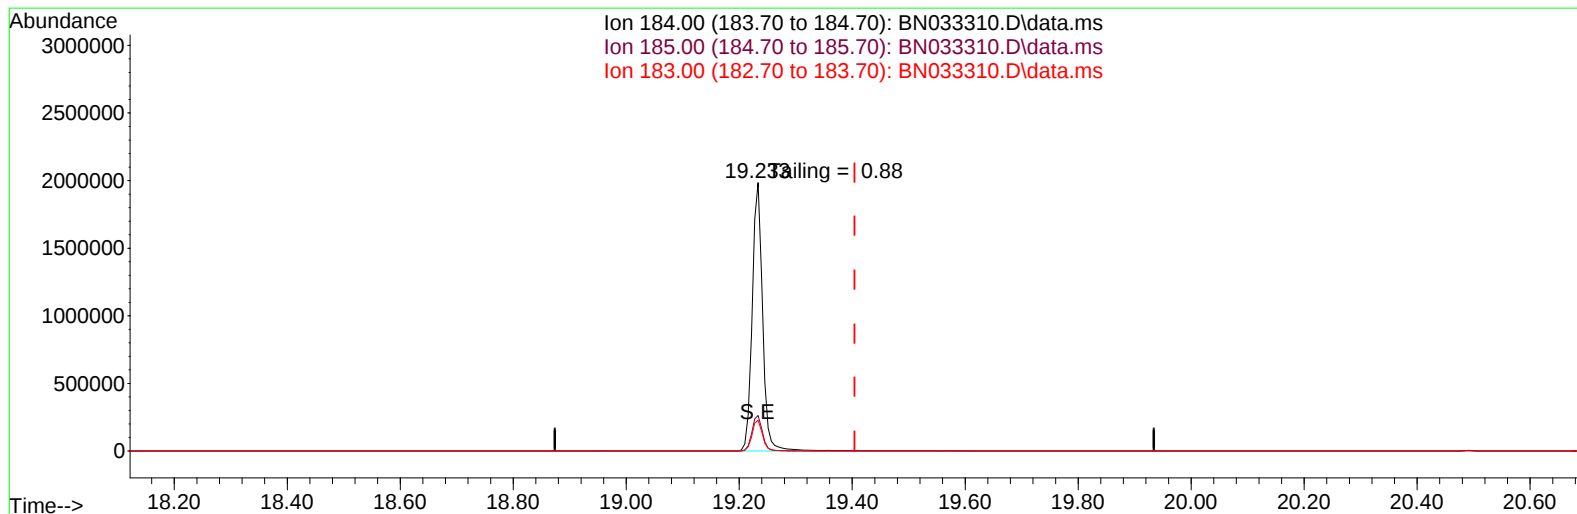

TIC: BN033310.D\data.ms

(77) Benzidine

19.233min (-0.171) 0.00 ng

response 2534372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.25
183.00	13.20	11.47
0.00	0.00	0.00