


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033321.D
Acq On : 09 Aug 2024 17:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 08 04:39:01 2024

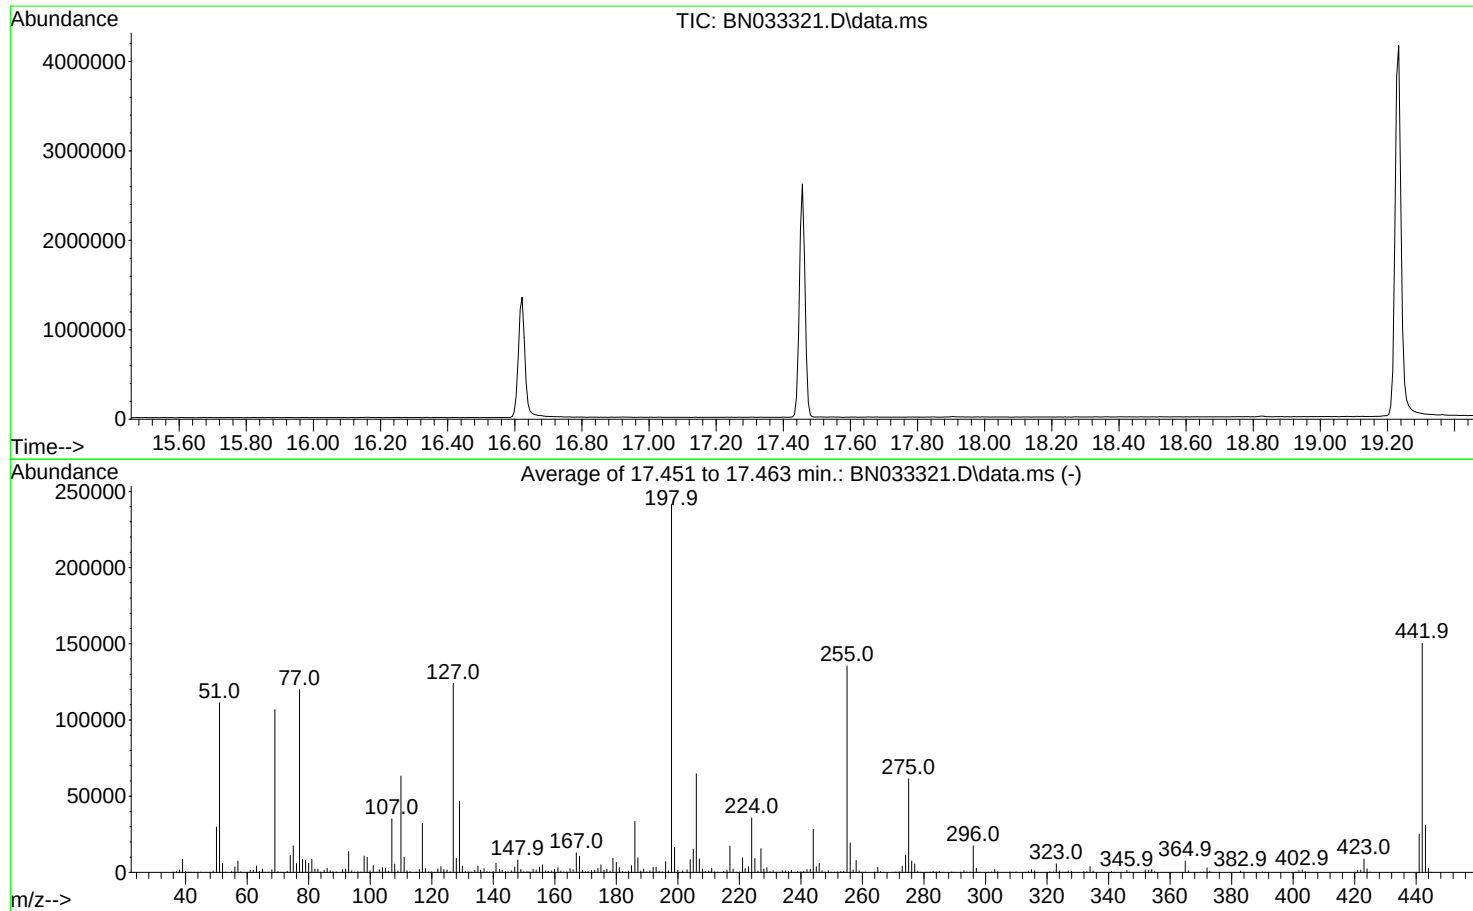

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	111246	PASS
68	69	0.00	2	1.6	1701	PASS
69	198	0.00	100	44.2	106789	PASS
70	69	0.00	2	0.5	567	PASS
127	198	10	80	51.4	123976	PASS
197	198	0.00	2	0.5	1113	PASS
198	198	100	100	100.0	241365	PASS
199	198	5	9	6.8	16464	PASS
275	198	10	60	25.5	61469	PASS
365	198	1	100	3.1	7421	PASS
441	198	0.01	100	10.4	25136	PASS
442	442	50	100	100.0	150363	PASS
443	442	15	24	20.5	30840	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/9/2024	BNA_N	<u>BN033321.D</u>
Compound Name	Response	Retention Time
DDT	840662	20.486
DDD	11136	20.098
DDE	304	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11440	852102	1.34

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033321.D
Acq On : 09 Aug 2024 17:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 10 00:51:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

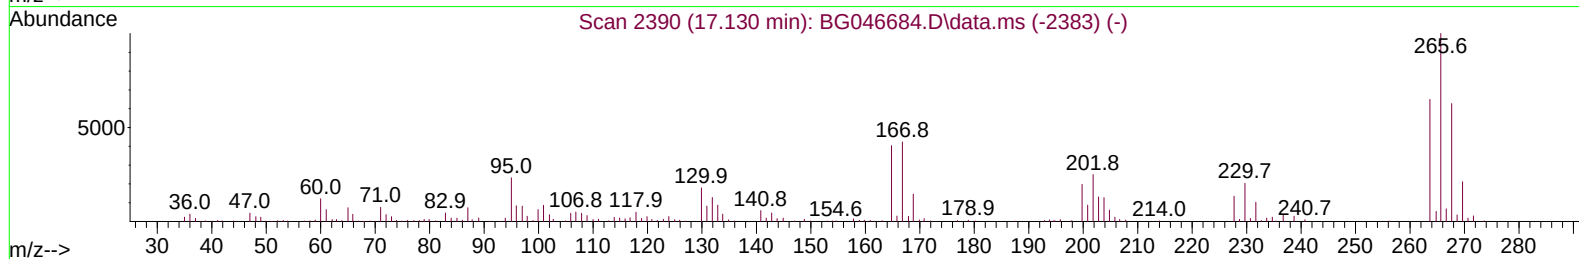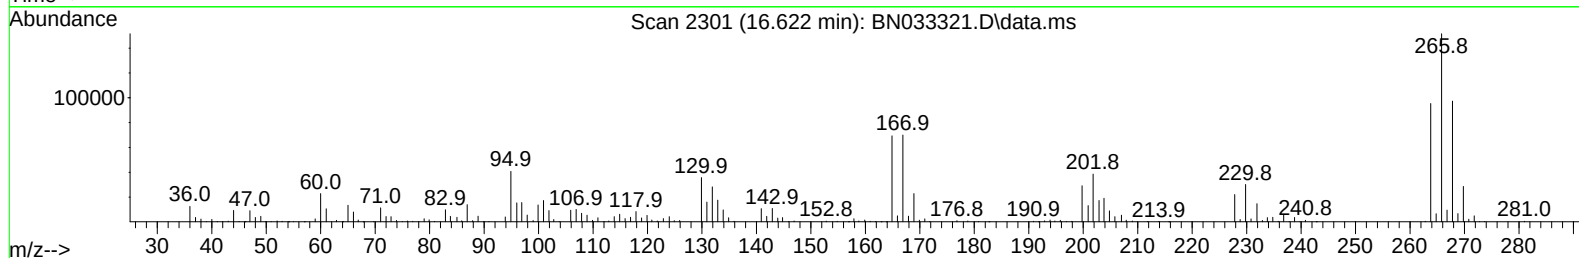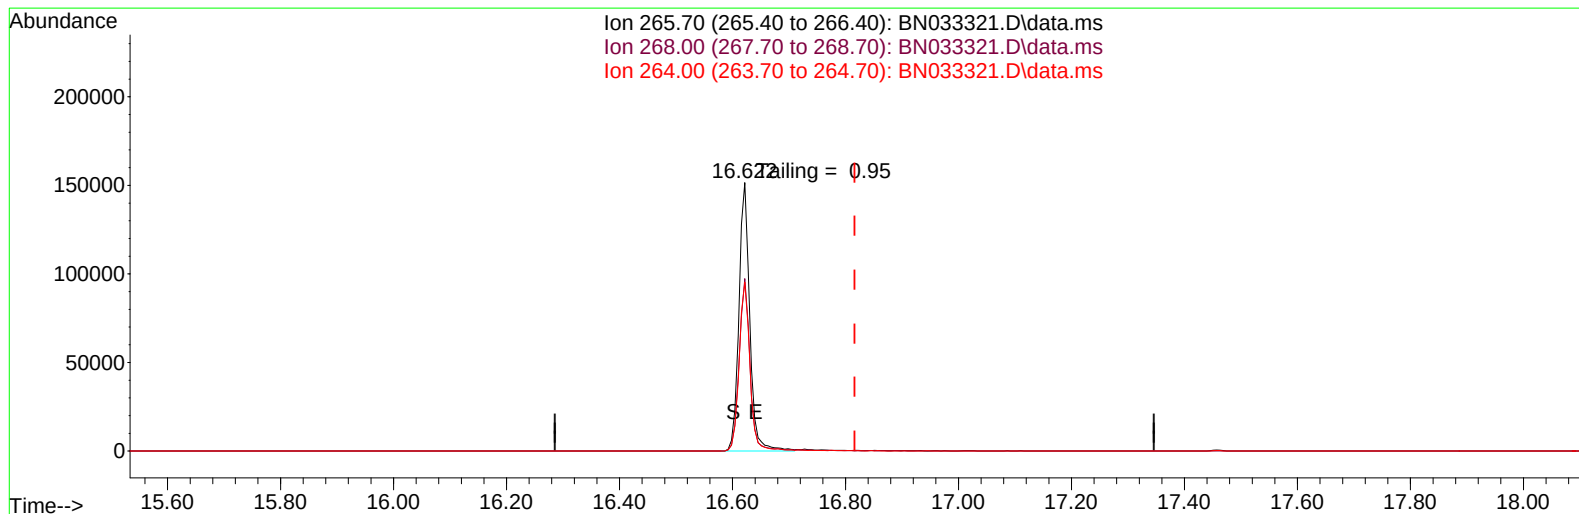

TIC: BN033321.D\data.ms

(70) Pentachlorophenol (C)

16.622min (-0.194) 18948.77 ng




response 202239

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080924\
Data File : BN033321.D
Acq On : 09 Aug 2024 17:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 10 00:51:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

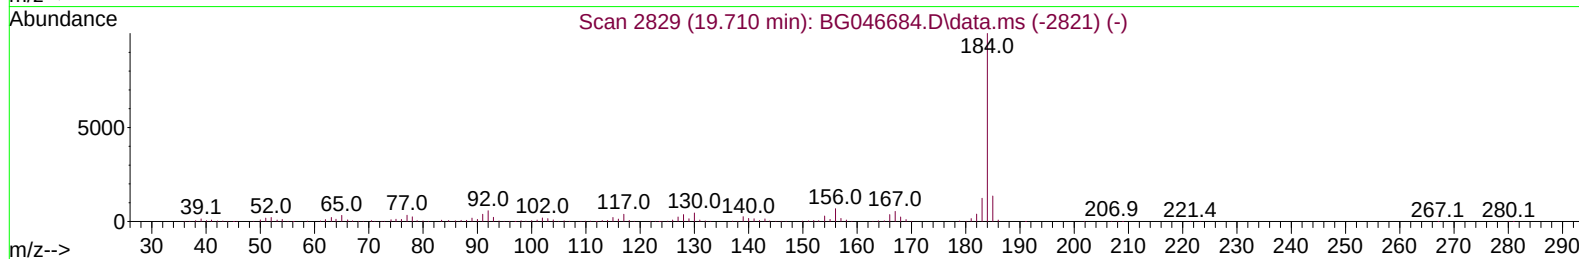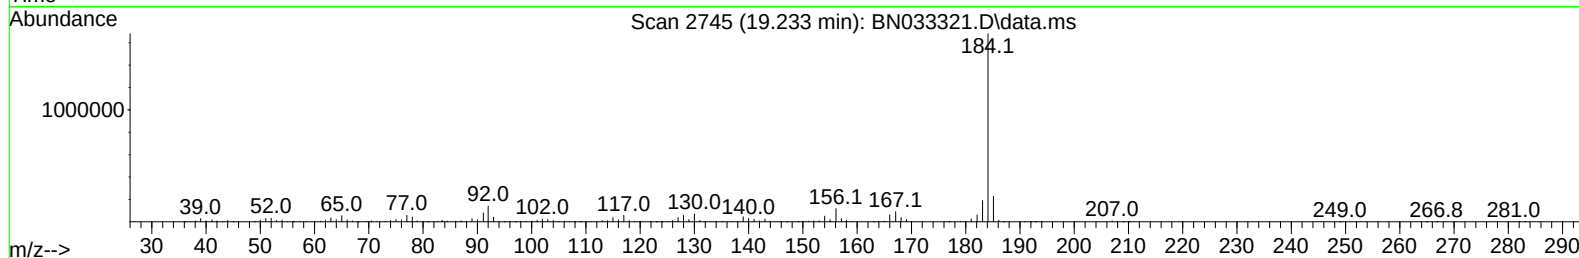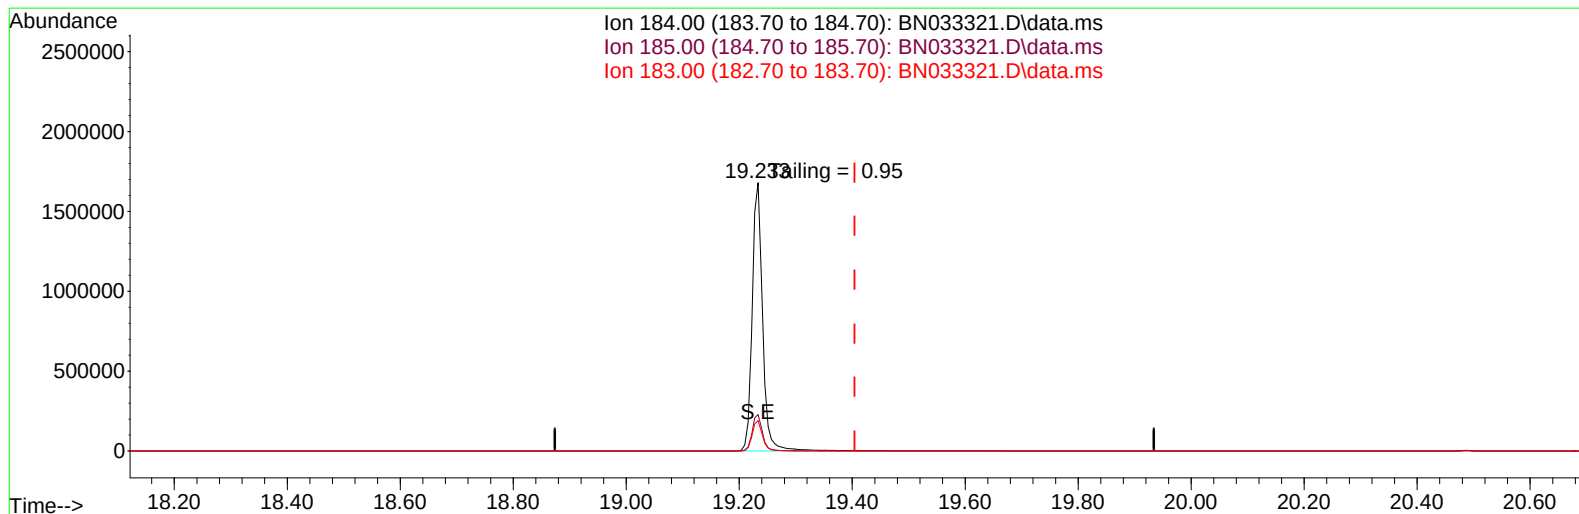

TIC: BN033321.D\data.ms

(77) Benzidine

19.233min (-0.171) 0.00 ng

response 2159782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.35
0.00	0.00	0.00