

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081021\
 Data File : BN015836.D
 Acq On : 10 Aug 2021 12:48
 Operator : CG/JU
 Sample : PB137773BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB138187BL

Quant Time: Aug 11 10:51:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 19:13:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	9933	0.400	ng	0.00
7) Naphthalene-d8	10.724	136	49653	0.400	ng	0.00
13) Acenaphthene-d10	14.561	164	28812	0.400	ng	0.00
19) Phenanthrene-d10	17.298	188	59215	0.400	ng	#-0.01
29) Chrysene-d12	21.493	240	63452	0.400	ng	# 0.00
35) Perylene-d12	23.919	264	59373	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.494	112	9517	0.368	ng	0.00
5) Phenol-d6	7.080	99	12733	0.363	ng	0.00
8) Nitrobenzene-d5	9.076	82	14291	0.367	ng	0.00
11) 2-Methylnaphthalene-d10	12.314	152	34092	0.428	ng	0.00
14) 2,4,6-Tribromophenol	16.044	330	3641	0.283	ng	0.00
15) 2-Fluorobiphenyl	13.190	172	45118	0.390	ng	0.00
27) Fluoranthene-d10	19.336	212	80389	0.447	ng	0.00
31) Terphenyl-d14	19.932	244	82903	0.445	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081021\
Data File : BN015836.D
Acq On : 10 Aug 2021 12:48
Operator : CG/JU
Sample : PB137773BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB138187BL

Quant Time: Aug 11 10:51:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 19:13:08 2021
Response via : Initial Calibration




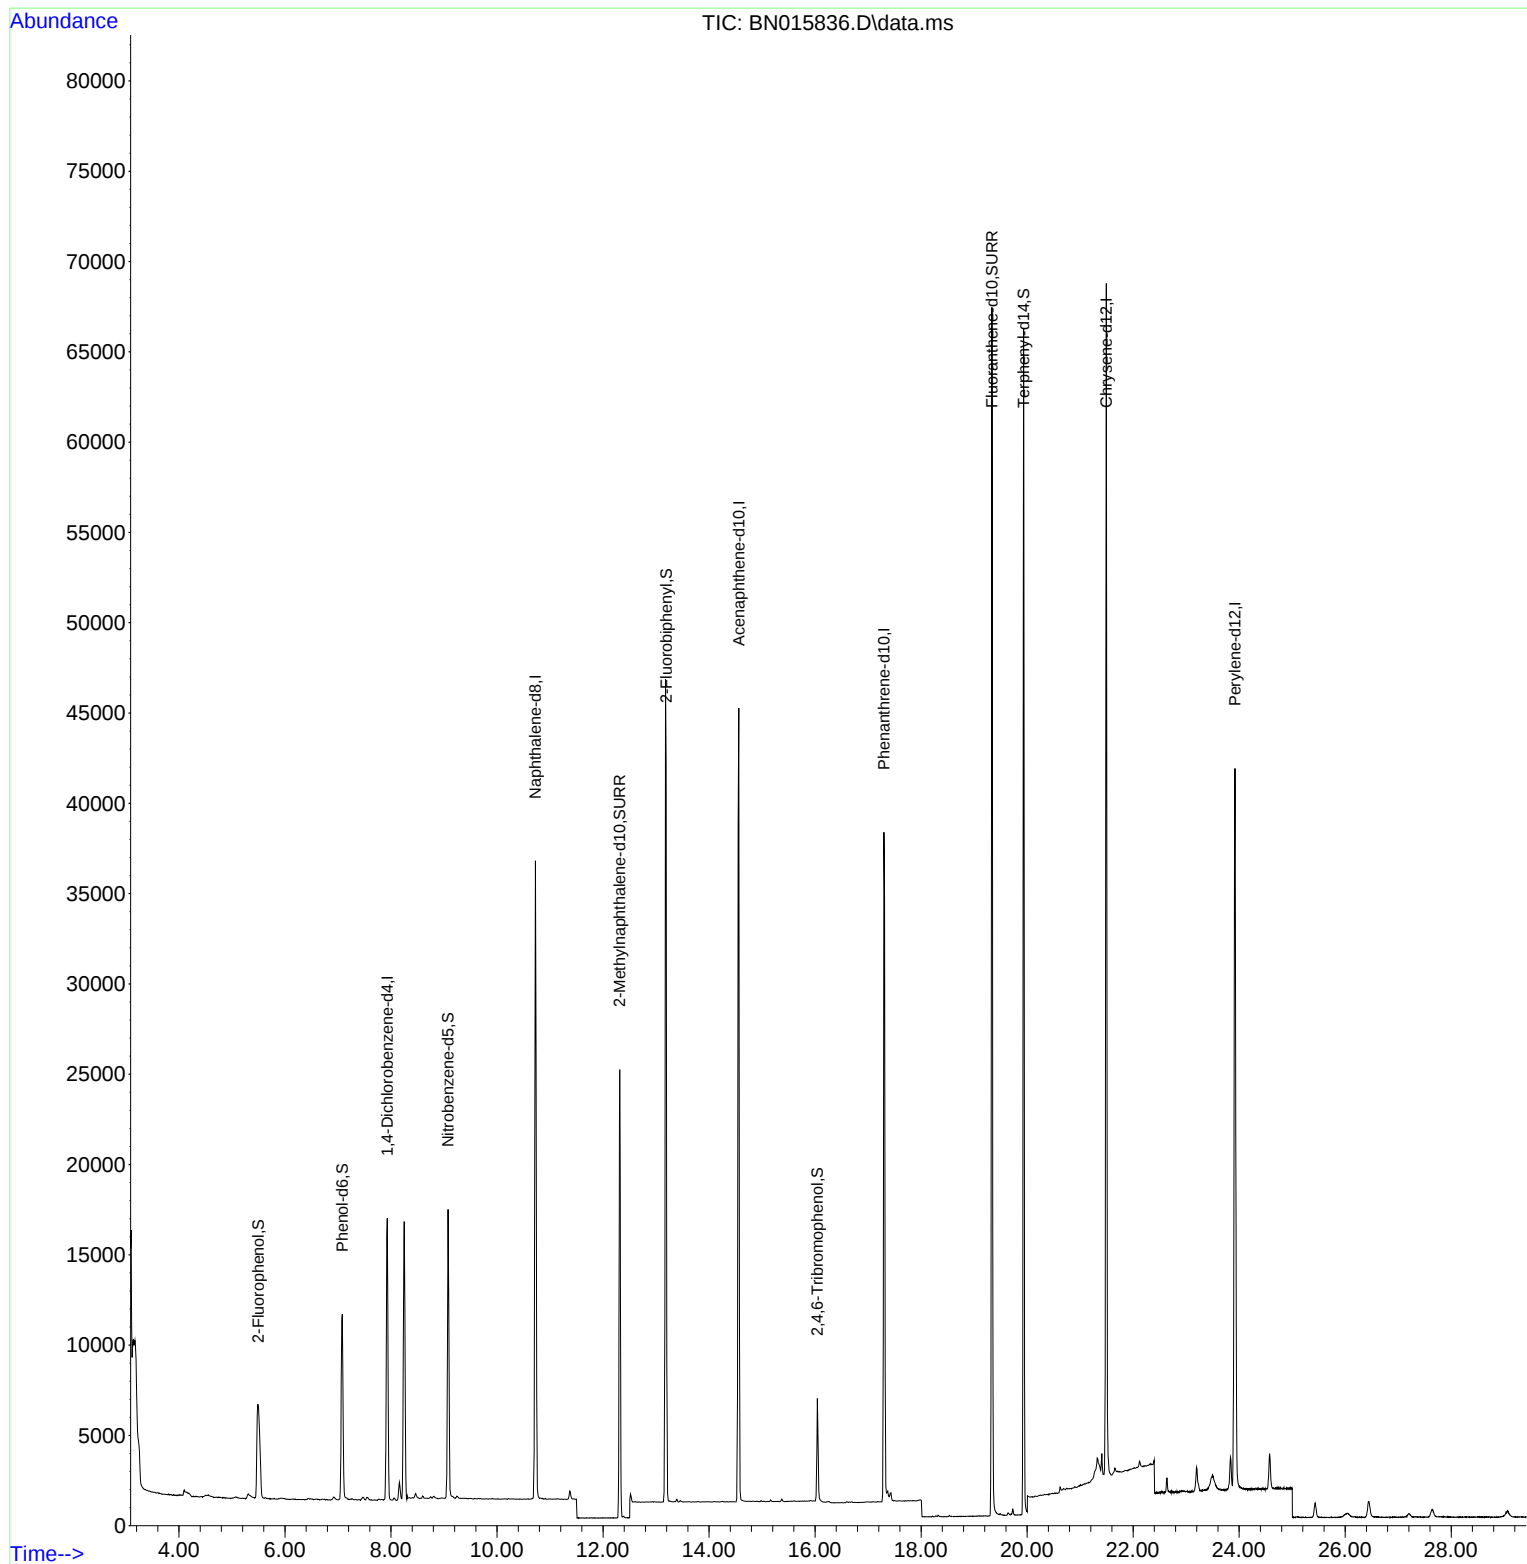


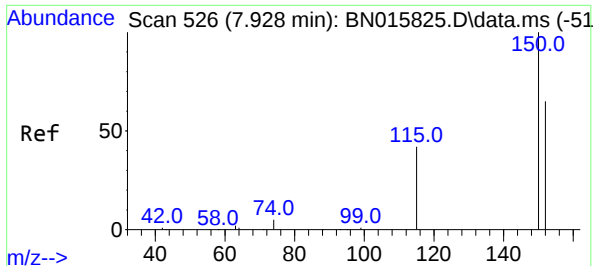

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.928 min Scan# 526
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampleId :
PB138187BL


Tgt Ion:152 Resp: 9933
Ion Ratio Lower Upper
152 100
150 155.3 123.0 184.4
115 64.8 52.2 78.2

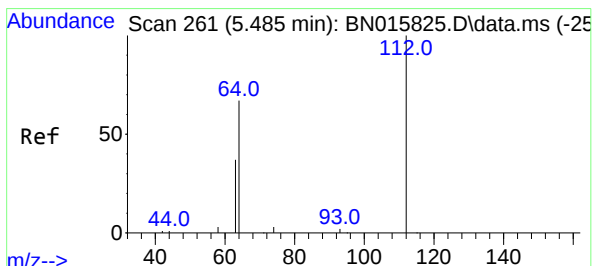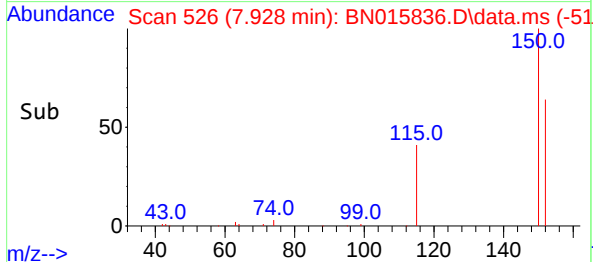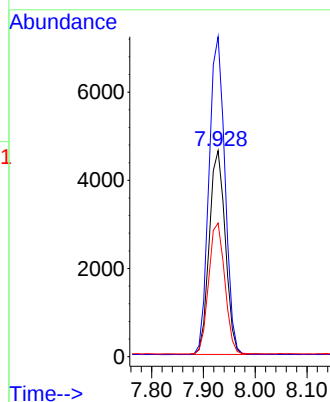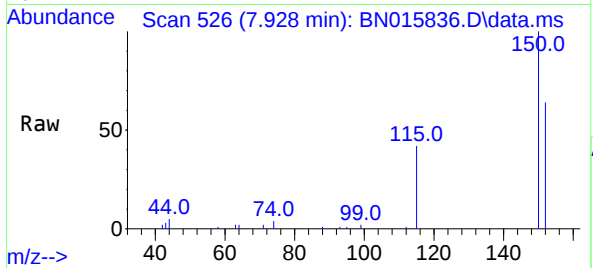

#4
2-Fluorophenol
Concen: 0.368 ng
RT: 5.494 min Scan# 262
Delta R.T. 0.009 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion:112 Resp: 9517
Ion Ratio Lower Upper
112 100
64 67.4 53.4 80.0
63 36.3 28.6 43.0


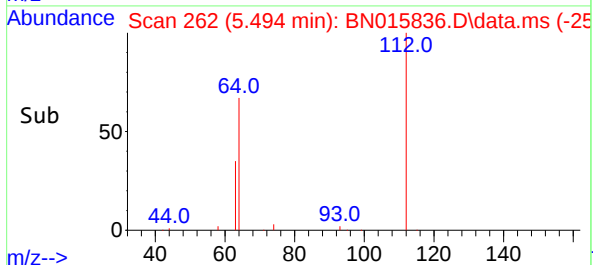
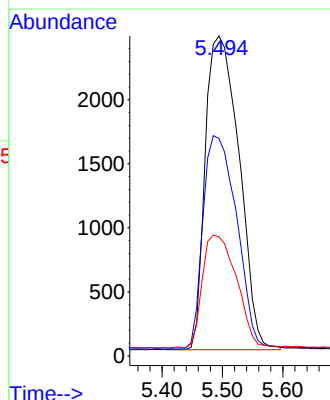
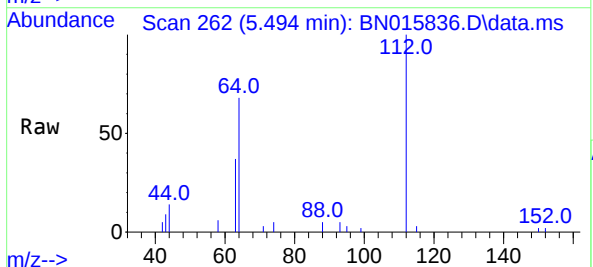




#5
Phenol-d6
Concen: 0.363 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampled :
PB138187BL


Tgt Ion: 99 Resp: 12733
Ion Ratio Lower Upper
99 100
42 21.7 19.0 28.4
71 39.7 31.2 46.8

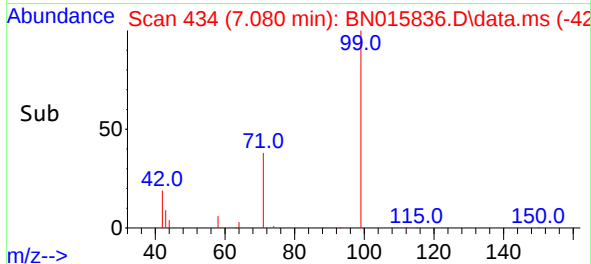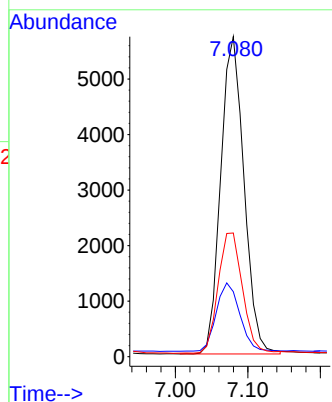

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.724 min Scan# 758
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion: 136 Resp: 49653
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 8.1 7.1 10.7
68 5.6 4.9 7.3


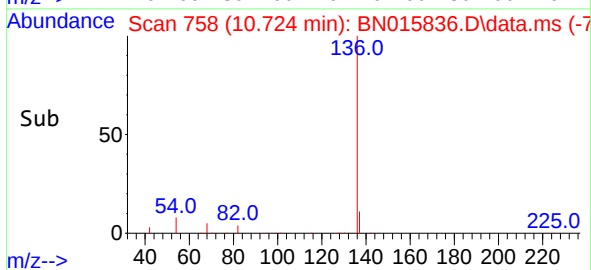
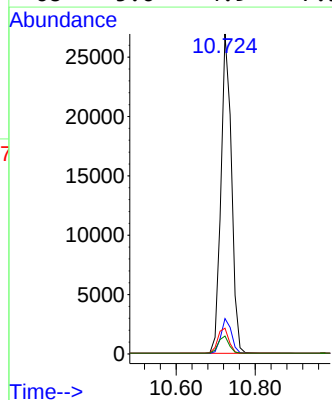
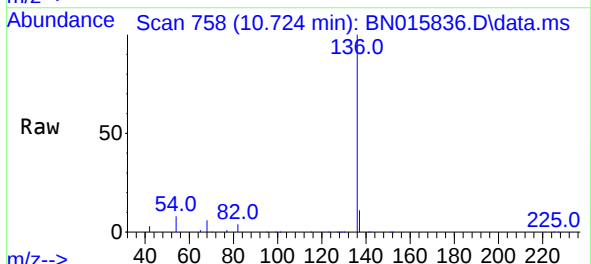




#8
Nitrobenzene-d5
Concen: 0.367 ng
RT: 9.076 min Scan# 628
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampleId :
PB138187BL


Tgt Ion: 82 Resp: 14291
Ion Ratio Lower Upper
82 100
128 33.9 26.2 39.2
54 55.7 45.4 68.0

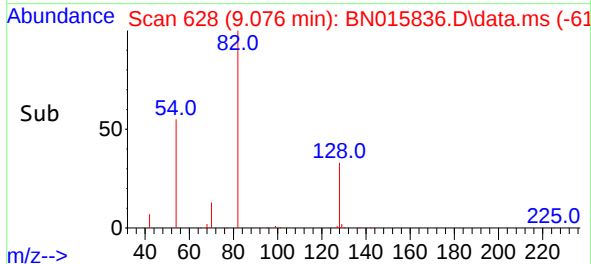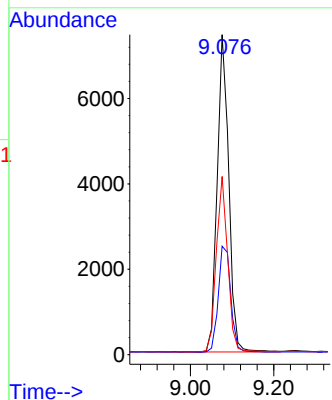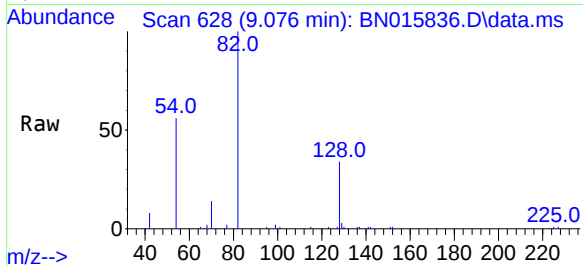

#11
2-Methylnaphthalene-d10
Concen: 0.428 ng
RT: 12.314 min Scan# 1001
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion: 152 Resp: 34092
Ion Ratio Lower Upper
152 100
151 20.5 16.4 24.6


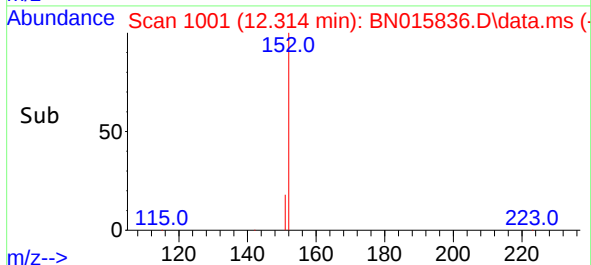
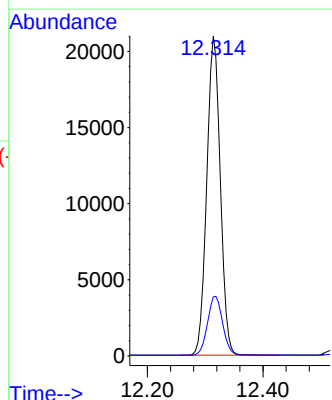
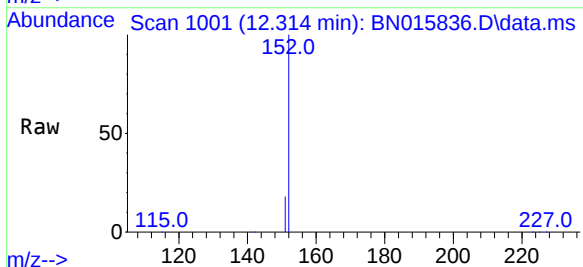




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.561 min Scan# 1206
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampleId :
PB138187BL


Tgt Ion:	164	Resp:	28812
Ion	Ratio	Lower	Upper
164	100		
162	98.8	81.2	121.8
160	42.4	35.0	52.4

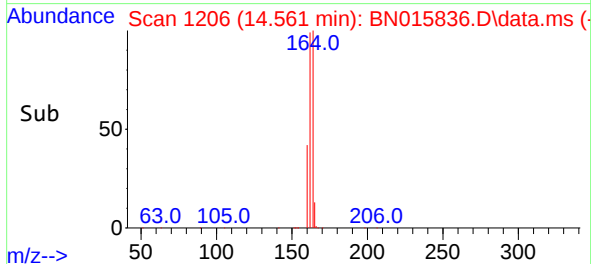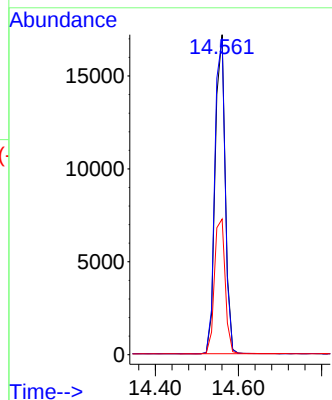

#14
2,4,6-Tribromophenol
Concen: 0.283 ng
RT: 16.044 min Scan# 1323
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion:	330	Resp:	3641
Ion	Ratio	Lower	Upper
330	100		
332	106.4	86.2	129.2
141	30.7	25.0	37.6


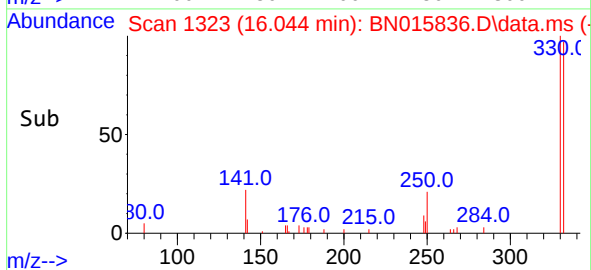
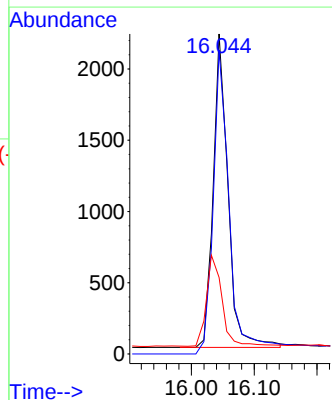
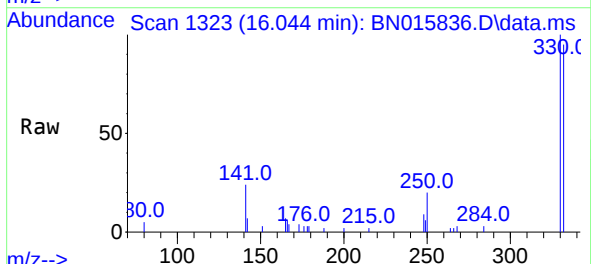




#15
2-Fluorobiphenyl
Concen: 0.390 ng
RT: 13.190 min Scan# 1098
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampleId :
PB138187BL


Tgt Ion:	172	Resp:	45118
Ion	Ratio	Lower	Upper
172	100		
171	33.5	26.9	40.3
170	21.4	17.3	25.9

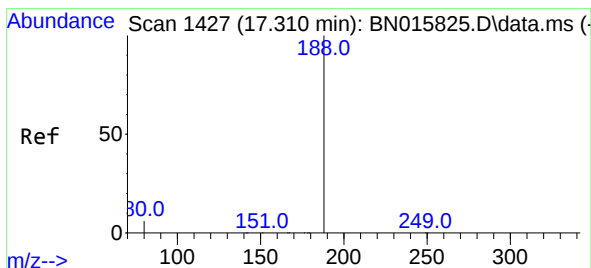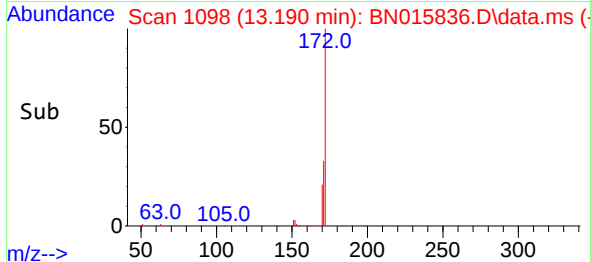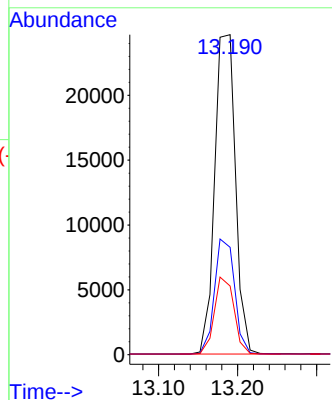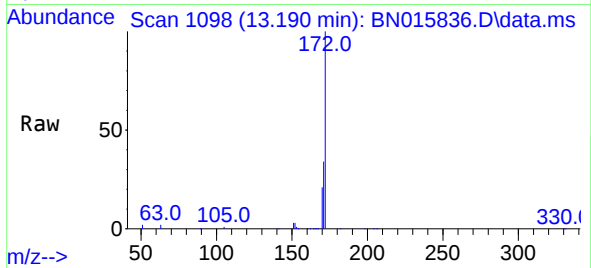

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.298 min Scan# 1426
Delta R.T. -0.012 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion:	188	Resp:	59215
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	10.7	4.7	7.1


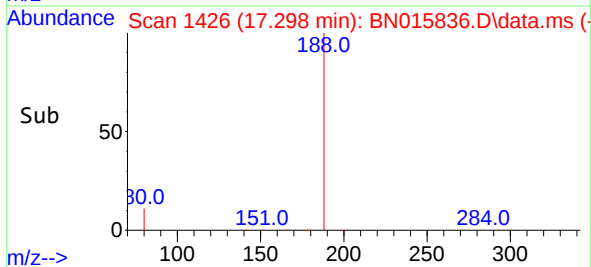
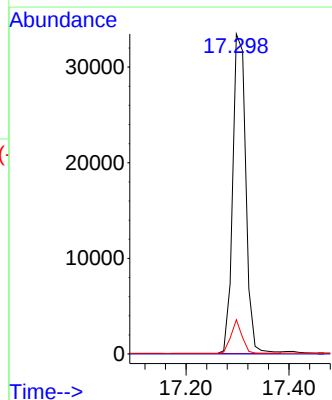
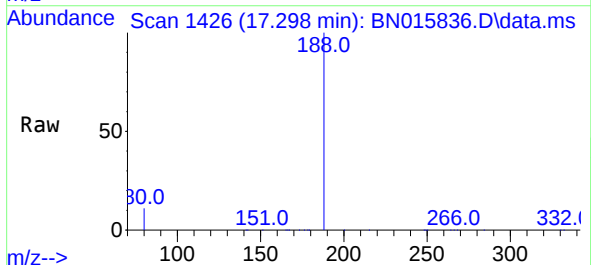




#27
Fluoranthene-d10
Concen: 0.447 ng
RT: 19.336 min Scan# 1751
Delta R.T. -0.005 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48




Instrument :
BNA_N
ClientSampleId :
PB138187BL


Tgt Ion:212 Resp: 80389
Ion Ratio Lower Upper
212 100
106 9.4 7.8 11.8
104 5.4 4.6 6.8

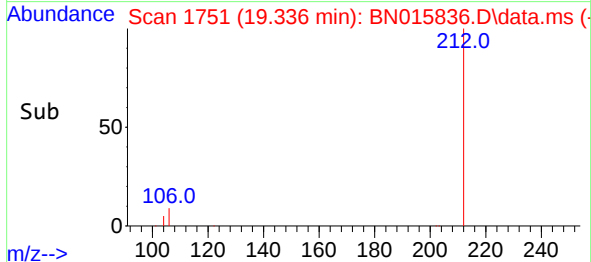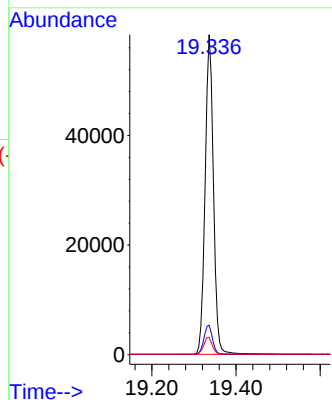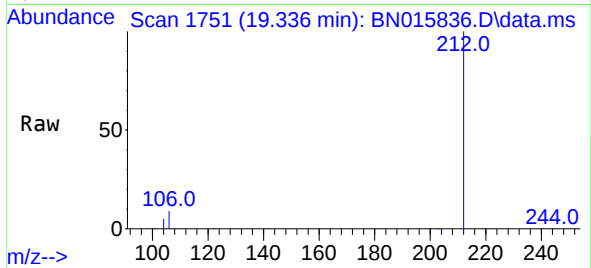

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.493 min Scan# 2026
Delta R.T. 0.000 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion:240 Resp: 63452
Ion Ratio Lower Upper
240 100
120 5.9 7.8 11.8#
236 25.9 21.1 31.7


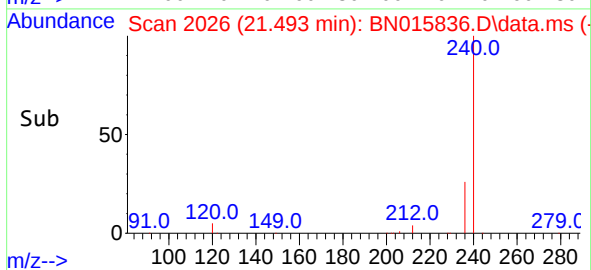
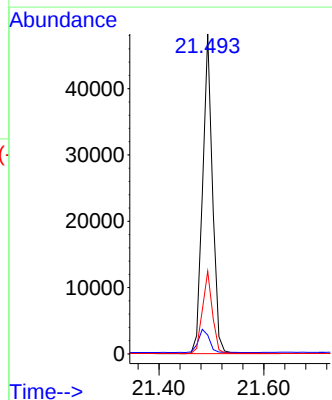
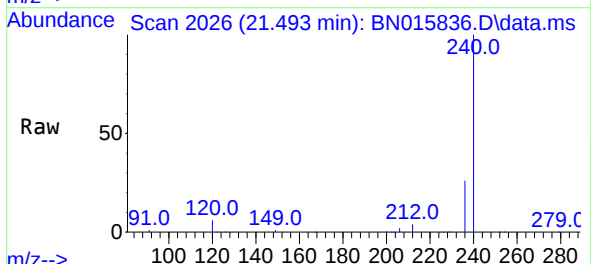




#31
Terphenyl-d14
Concen: 0.445 ng
RT: 19.932 min Scan# 1871
Delta R.T. -0.005 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Instrument :
BNA_N
ClientSampleId :
PB138187BL

Tgt Ion:244 Resp: 82903
Ion Ratio Lower Upper
244 100
212 7.3 6.1 9.1
122 8.7 7.0 10.4

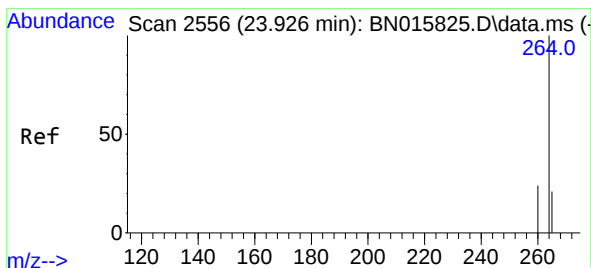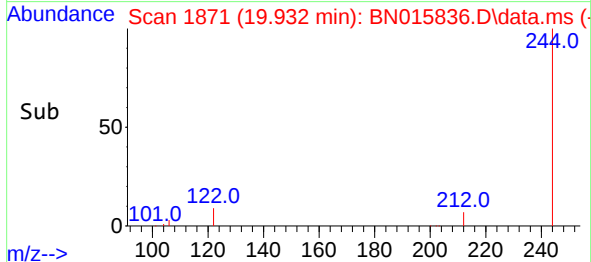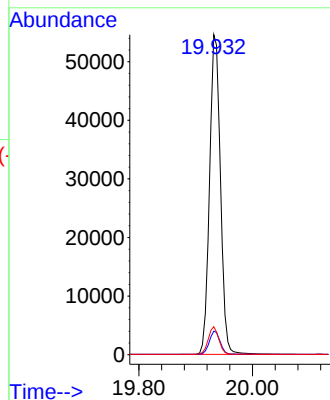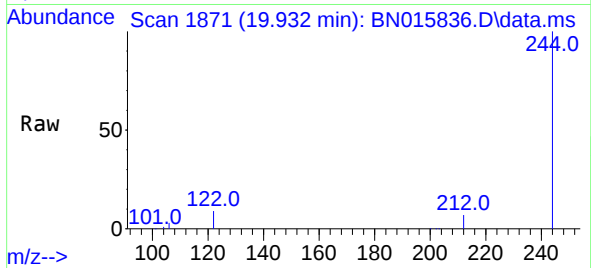

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.919 min Scan# 2554
Delta R.T. -0.007 min
Lab File: BN015836.D
Acq: 10 Aug 2021 12:48

Tgt Ion:264 Resp: 59373
Ion Ratio Lower Upper
264 100
260 24.0 19.6 29.4
265 25.2 21.7 32.5

