
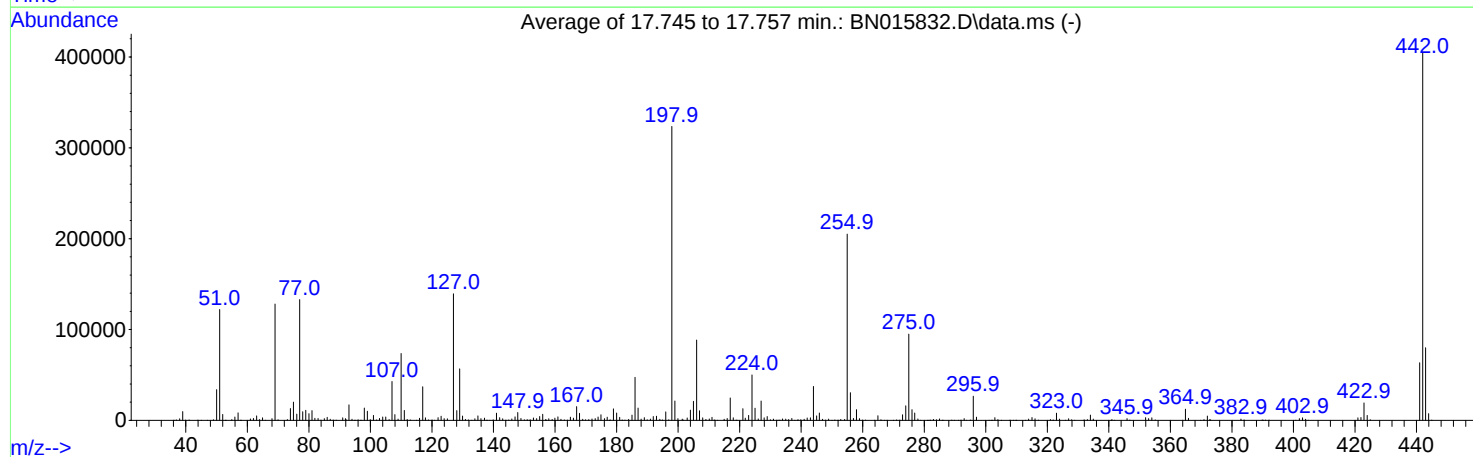


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081021\
 Data File : BN015832.D
 Acq On : 10 Aug 2021 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 09 19:13:08 2021

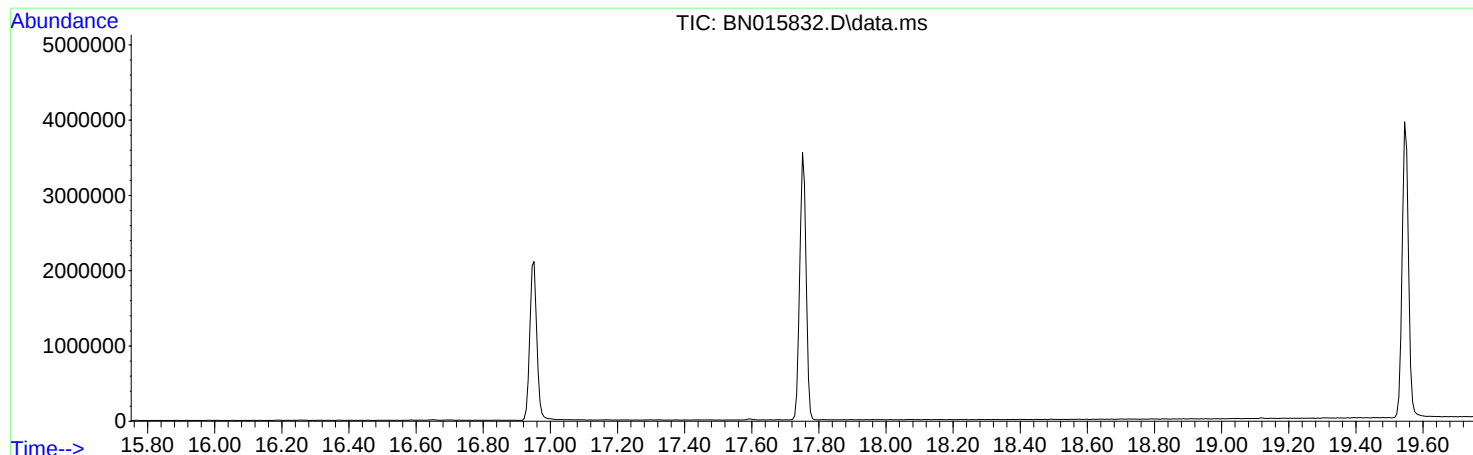

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	122032	PASS
68	69	0.00	2	1.5	1905	PASS
69	198	0.00	100	39.6	128123	PASS
70	69	0.00	2	0.5	669	PASS
127	198	10	80	43.1	139288	PASS
197	198	0.00	2	0.2	717	PASS
198	198	100	100	100.0	323499	PASS
199	198	5	9	6.6	21269	PASS
275	198	10	60	29.4	95005	PASS
365	198	1	100	3.8	12274	PASS
441	198	0.01	100	19.6	63483	PASS
442	442	50	100	100.0	404949	PASS
443	442	15	24	19.8	79997	PASS